

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051220\
 Data File : BG045329.D
 Acq On : 12 May 2020 15:08
 Operator : CG/JU
 Sample : PB128795BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB128795BL

Quant Time: May 12 15:52:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 12 15:48:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	63053	20.00	ng	0.00
21) Naphthalene-d8	10.79	136	250542	20.00	ng	0.00
39) Acenaphthene-d10	14.63	164	181356	20.00	ng	0.00
64) Phenanthrene-d10	17.37	188	426020	20.00	ng	0.00
76) Chrysene-d12	21.63	240	439556	20.00	ng	0.00
87) Perylene-d12	24.80	264	457116	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	470720	123.25	ng	0.00
7) Phenol-d6	7.14	99	664838	117.16	ng	0.00
23) Nitrobenzene-d5	9.14	82	465005	84.69	ng	0.00
42) 2,4,6-Tribromophenol	16.11	330	338100	120.68	ng	0.00
45) 2-Fluorobiphenyl	13.25	172	1050660	84.95	ng	0.00
79) Terphenyl-d14	19.98	244	1946586	96.52	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051220\
Data File : BG045329.D
Acq On : 12 May 2020 15:08
Operator : CG/JU
Sample : PB128795BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB128795BL

Quant Time: May 12 15:52:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 12 15:48:20 2020
Response via : Initial Calibration

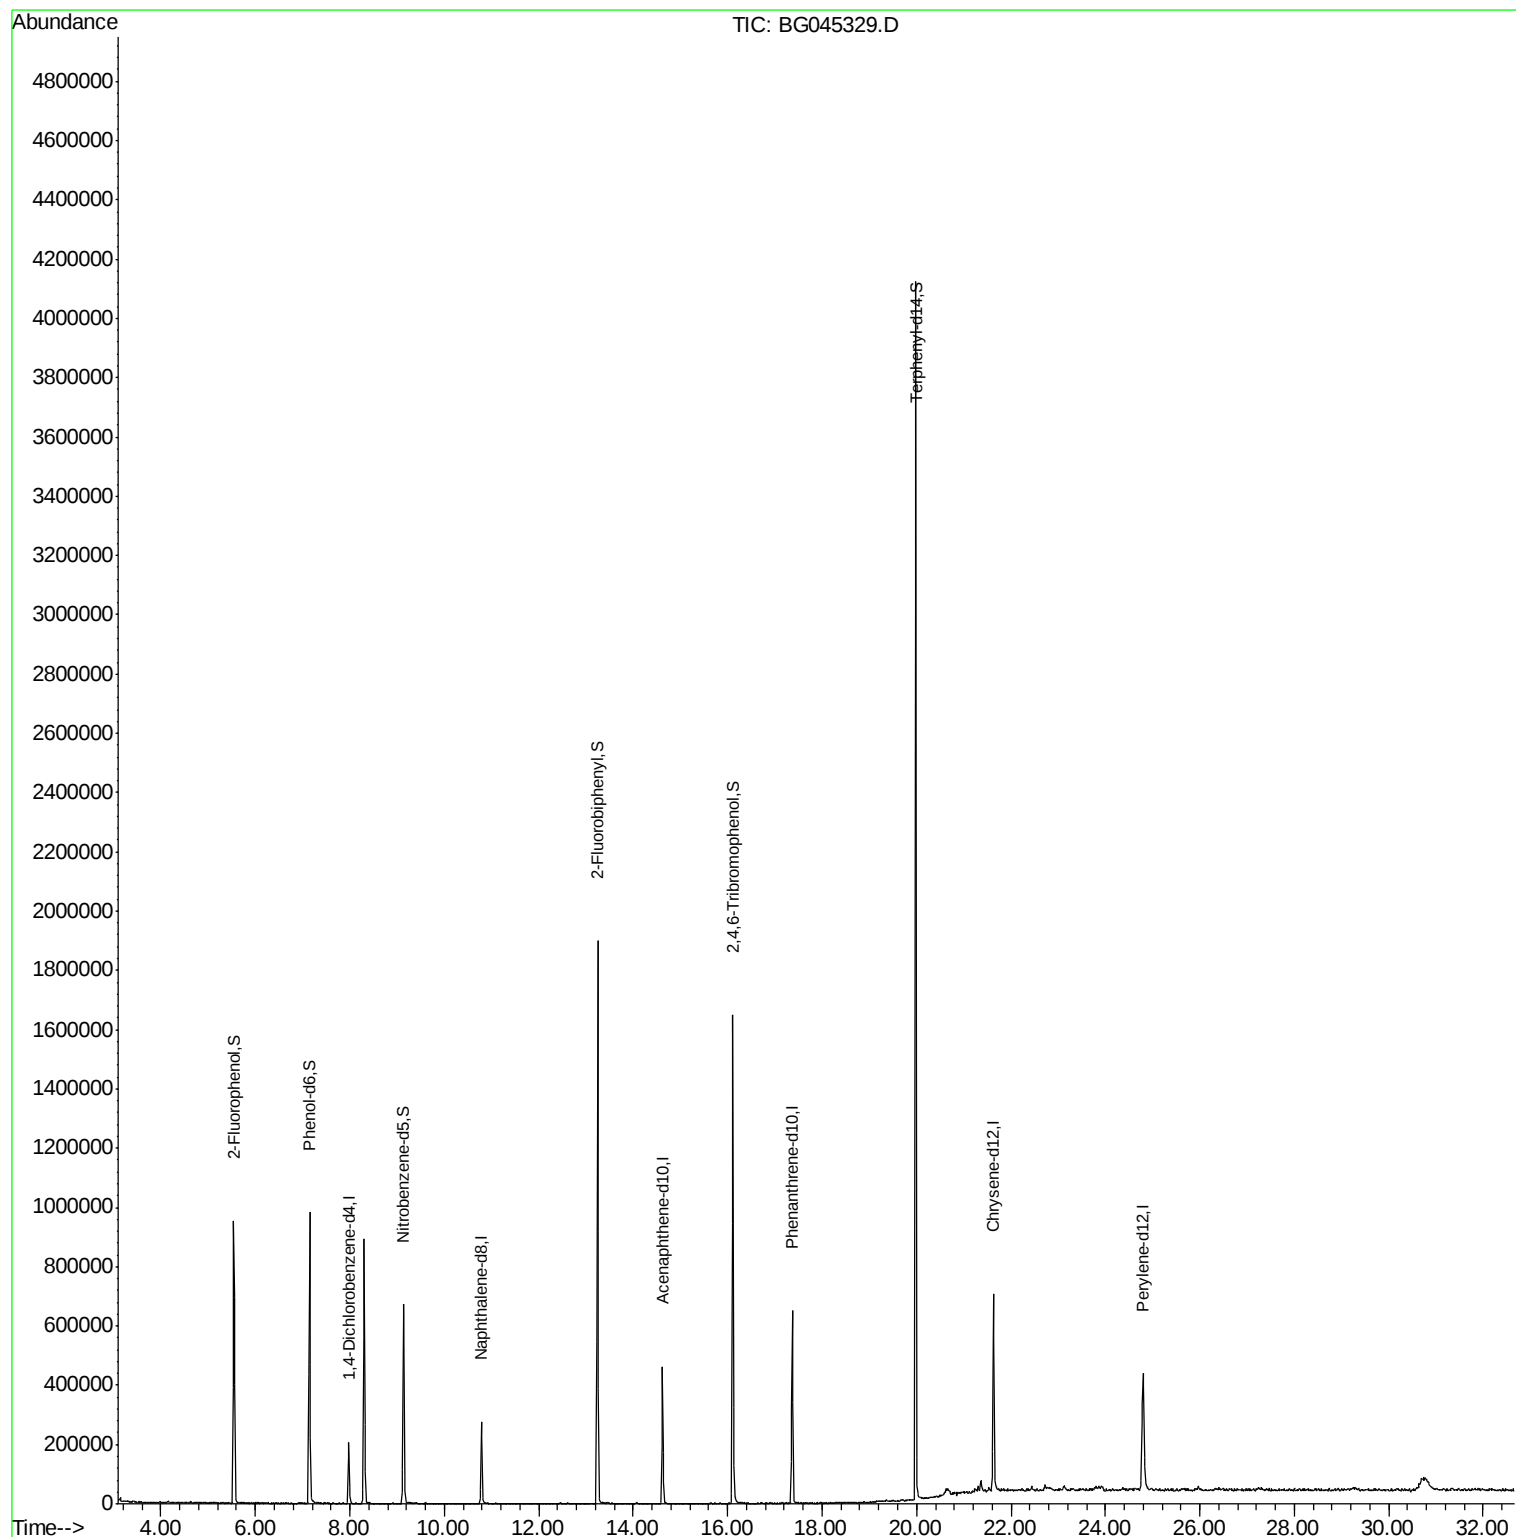

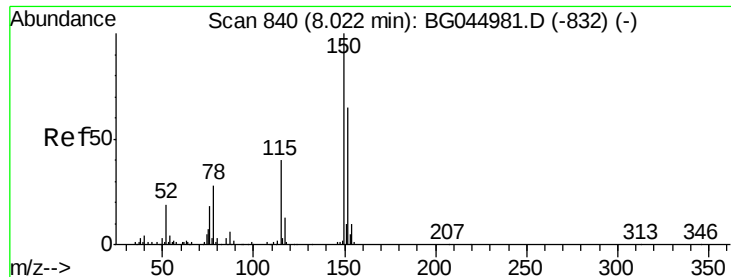


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.98 min Scan# 833
 Delta R.T. 0.00 min
 Lab File: BG045329.D
 Acq: 12 May 2020 15:08

Instrument :
 BNA_G
 ClientSampleId :
 PB128795BL

Tot Ion:152 Resp: 63053
 Ion Ratio Lower Upper
 152 100
 150 153.6 123.6 185.4
 115 60.5 49.1 73.7

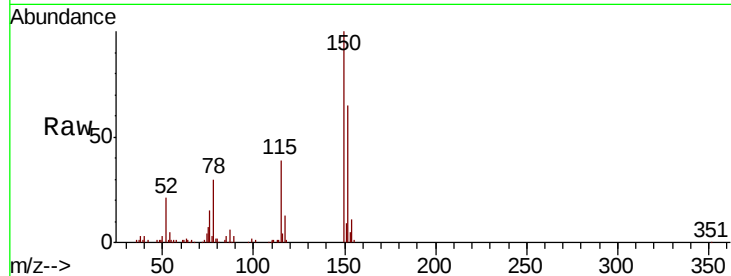


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

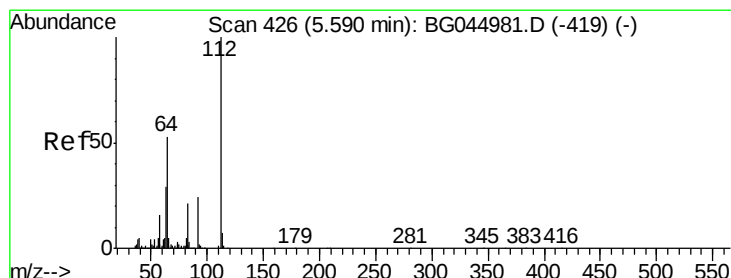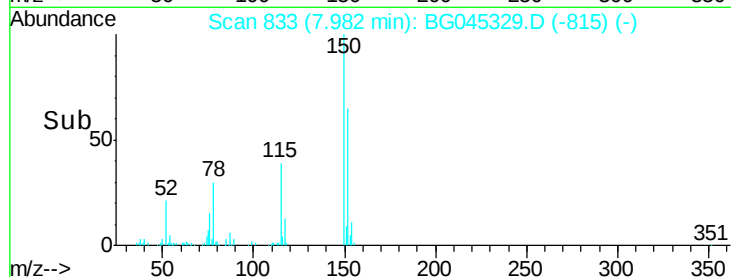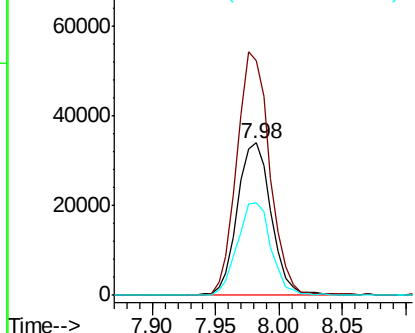



#5


2-Fluorophenol
 Concen: 123.251 ng
 RT: 5.54 min Scan# 418
 Delta R.T. 0.00 min
 Lab File: BG045329.D
 Acq: 12 May 2020 15:08

Tgt Ion:112 Resp: 470720
 Ion Ratio Lower Upper
 112 100
 64 58.5 42.4 63.6
 63 33.9 23.1 34.7

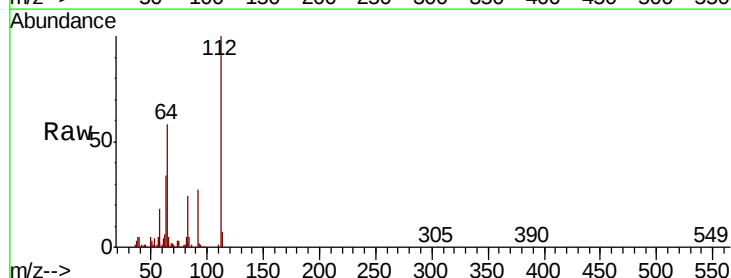

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

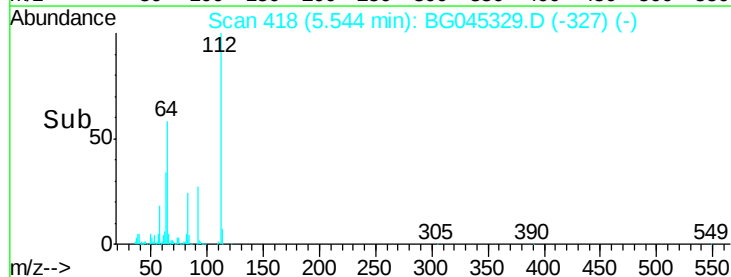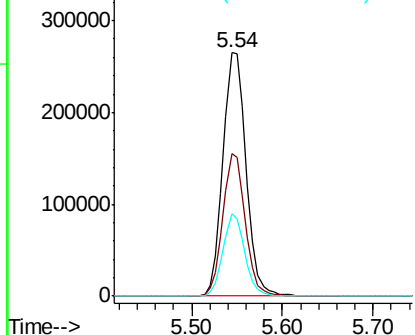

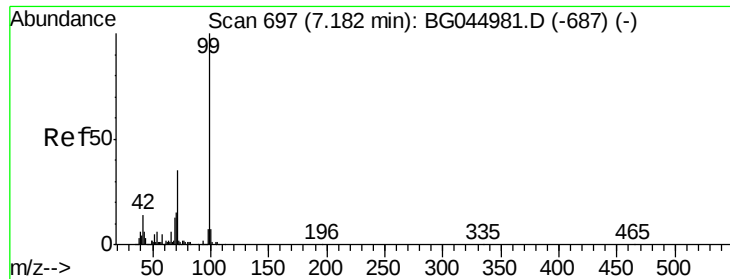

#7

Phenol-d6

Concen: 117.165 ng

RT: 7.14 min Scan# 690

Delta R.T. -0.00 min

Lab File: BG045329.D

Acq: 12 May 2020 15:08

Instrument :

BNA_G

ClientSampleId :

PB128795BL


Tot Ion: 99 Resp: 664838

Ion Ratio Lower Upper




99 100

42 14.5 11.3 16.9

71 36.8 28.3 42.5

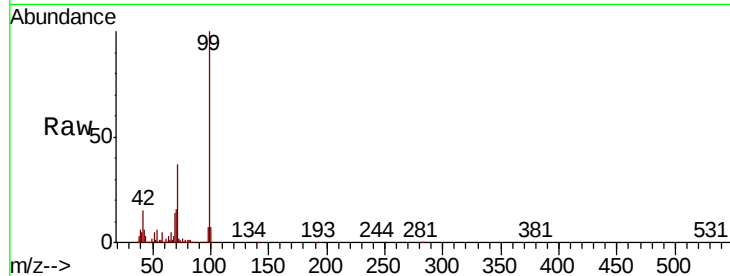

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

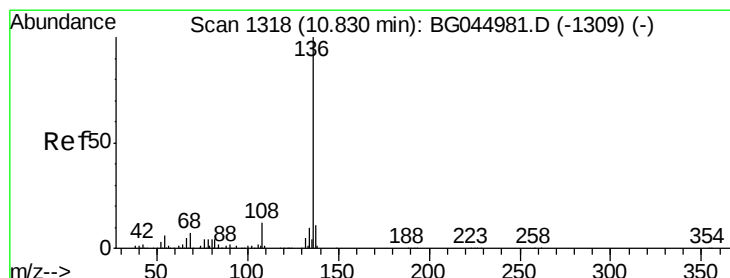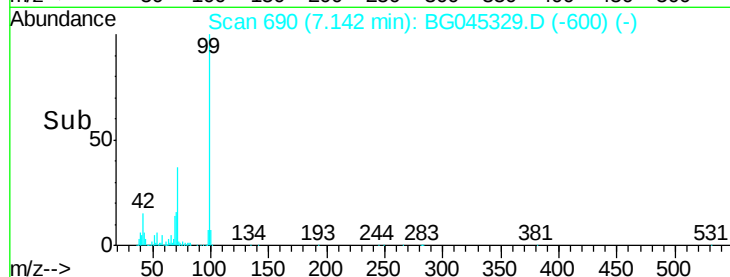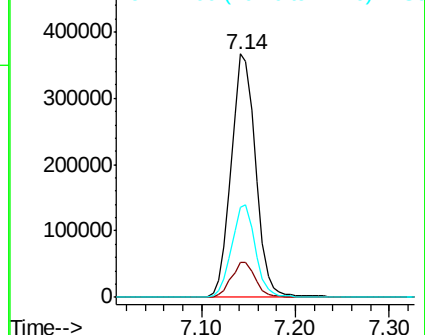

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.79 min Scan# 1311

Delta R.T. 0.00 min

Lab File: BG045329.D

Acq: 12 May 2020 15:08

Tgt Ion: 136 Resp: 250542


Ion Ratio Lower Upper

136 100



137 9.9 8.6 13.0

54 6.2 4.8 7.2

68 5.5 5.2 7.8

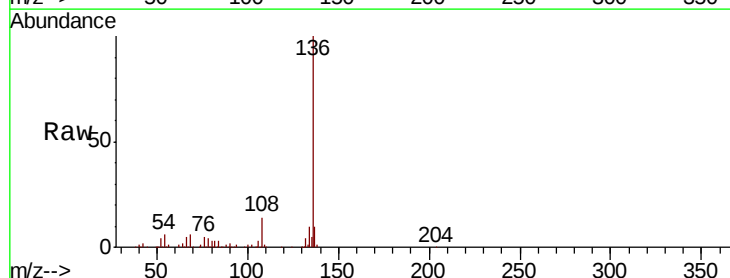

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



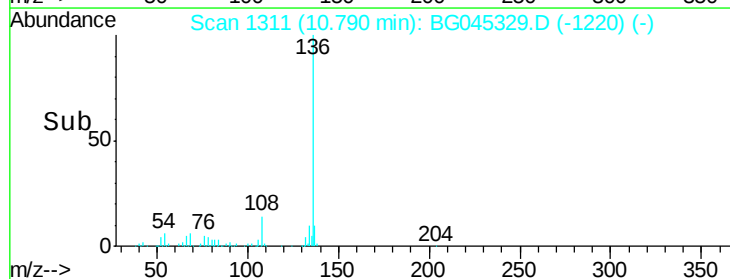
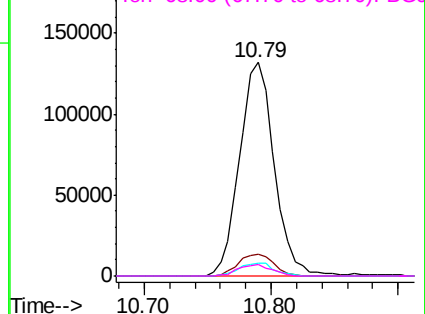




#23
Nitrobenzene-d5
Concen: 84.687 ng
RT: 9.14 min Scan# 1030
Delta R.T. 0.00 min
Lab File: BG045329.D
Acq: 12 May 2020 15:08




Instrument :
BNA_G
ClientSampleId :
PB128795BL

Tot Ion	82	Resp	465005
Ion Ratio	Lower	Upper	
82	100		
128	41.6	33.0	49.4
54	40.5	30.4	45.6

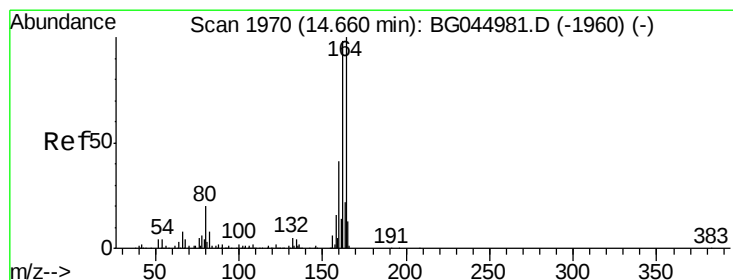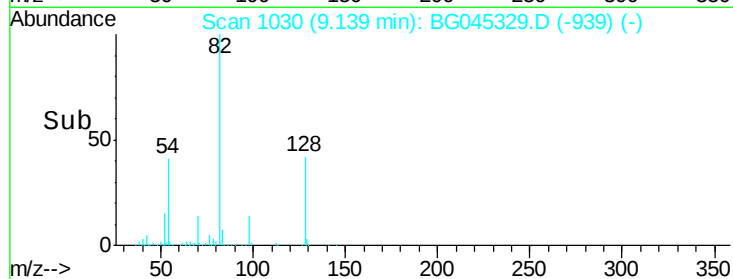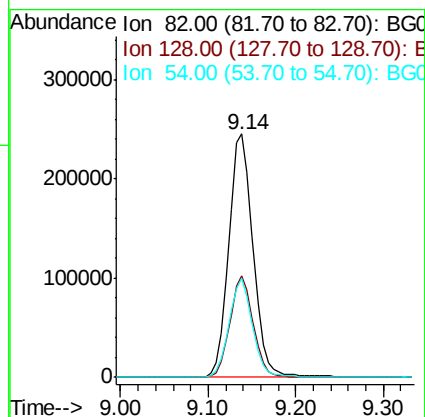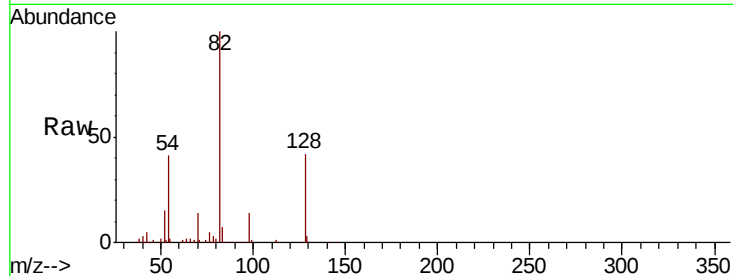

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.63 min Scan# 1964
Delta R.T. 0.00 min
Lab File: BG045329.D
Acq: 12 May 2020 15:08

Tgt Ion	164	Resp	181356
Ion Ratio	Lower	Upper	
164	100		
162	91.2	78.7	118.1
160	43.1	32.8	49.2


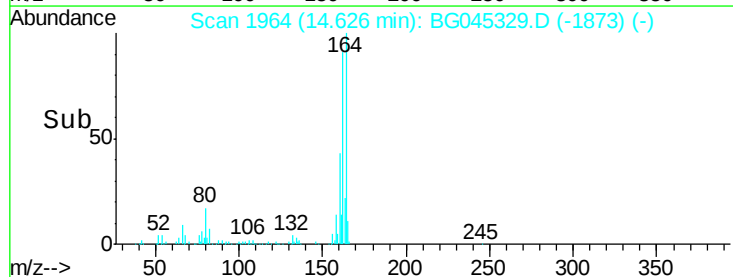
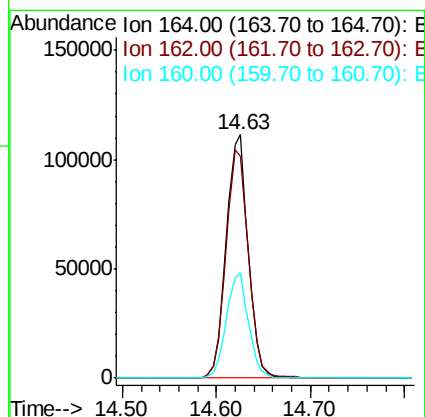
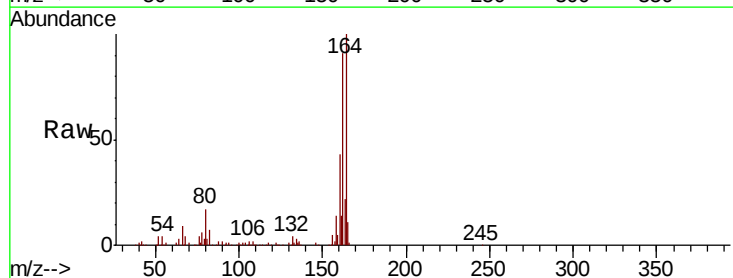




#42
 2,4,6-Tribromophenol
 Concen: 120.676 ng
 RT: 16.11 min Scan# 2217
 Delta R.T. 0.00 min
 Lab File: BG045329.D
 Acq: 12 May 2020 15:08




Instrument :
 BNA_G
 ClientSampleId :
 PB128795BL


Tot Ion	Ratio	Lower	Upper
330	100		
332	98.6	79.1	118.7
141	35.1	27.1	40.7

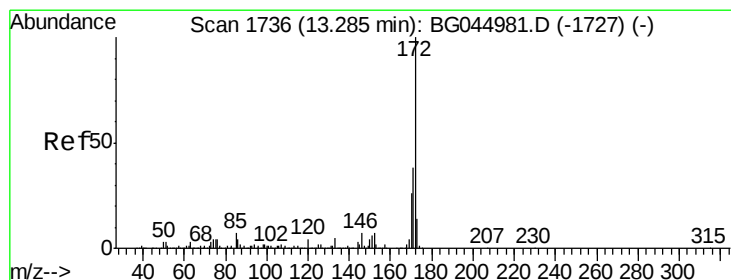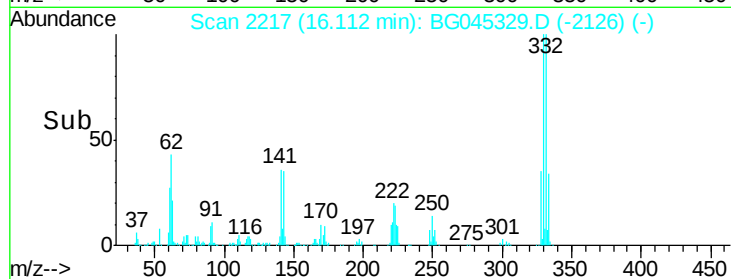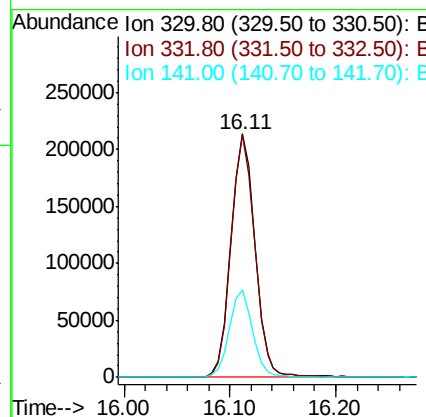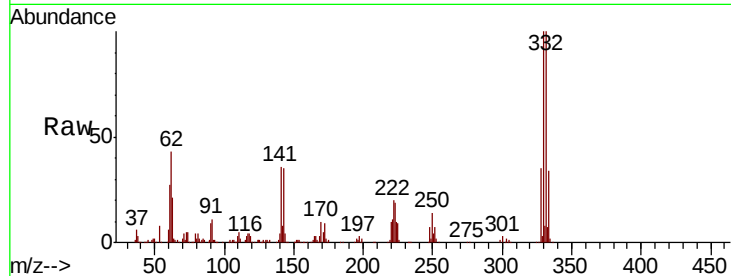

#45
 2-Fluorobiphenyl
 Concen: 84.949 ng
 RT: 13.25 min Scan# 1729
 Delta R.T. 0.00 min
 Lab File: BG045329.D
 Acq: 12 May 2020 15:08

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.8	30.6	46.0
170	23.9	20.5	30.7

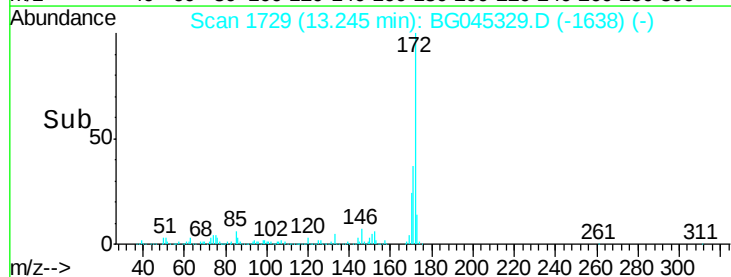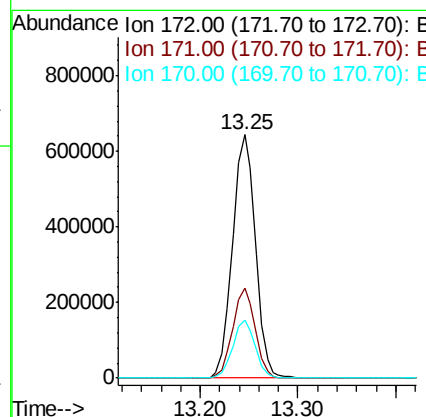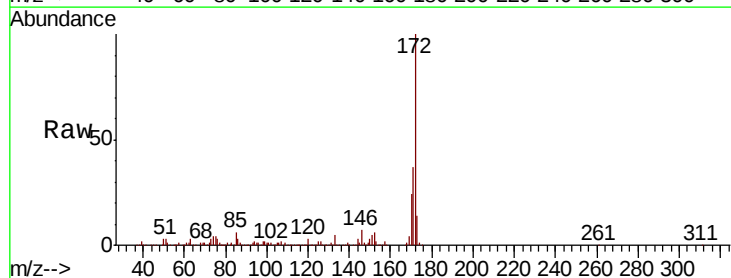

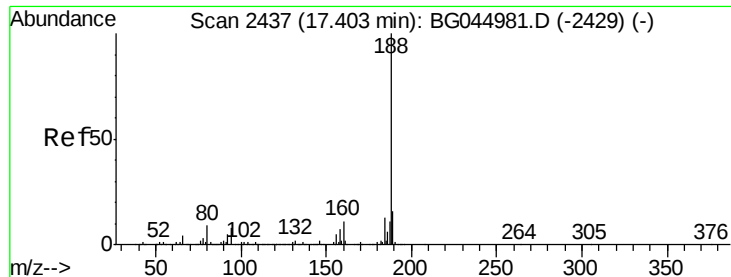

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.37 min Scan# 2431

Delta R.T. 0.00 min

Lab File: BG045329.D

Acq: 12 May 2020 15:08

Instrument :

BNA_G

ClientSampleId :

PB128795BL


Tot Ion:188 Resp: 426020

Ion Ratio Lower Upper

188 100

94 6.8 6.2 9.4




80 8.7 7.0 10.6

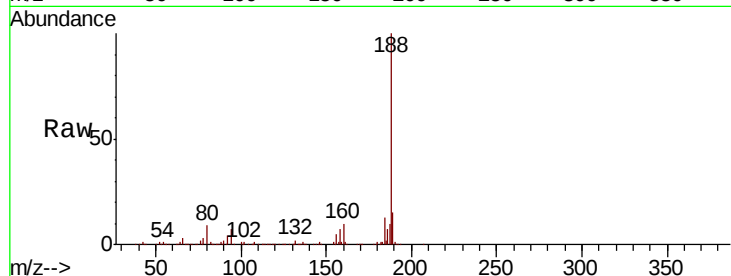

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG0

Ion 80.00 (79.70 to 80.70): BG0

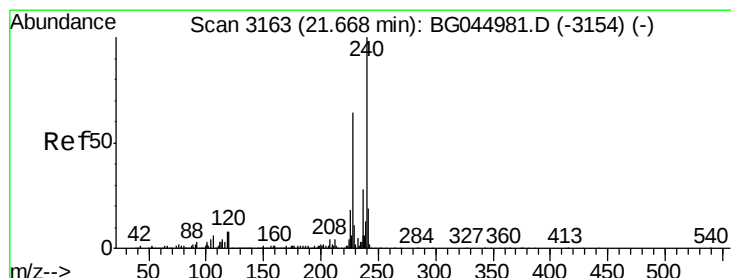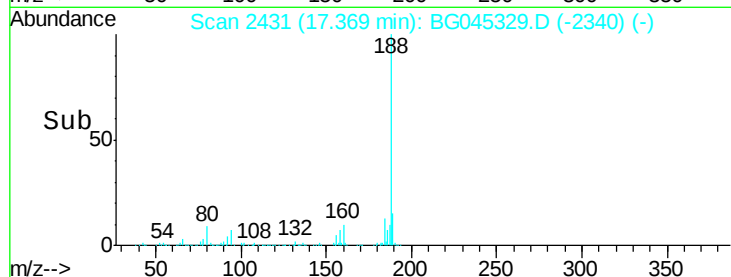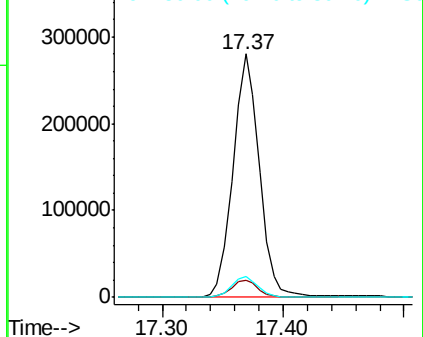

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.63 min Scan# 3157

Delta R.T. 0.00 min

Lab File: BG045329.D

Acq: 12 May 2020 15:08


Tgt Ion:240 Resp: 439556

Ion Ratio Lower Upper

240 100

120 6.9 6.6 10.0



236 26.5 22.2 33.2

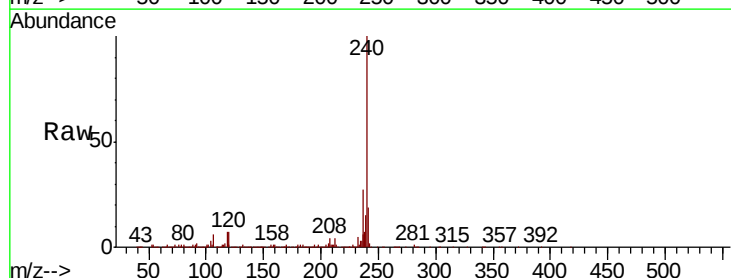


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

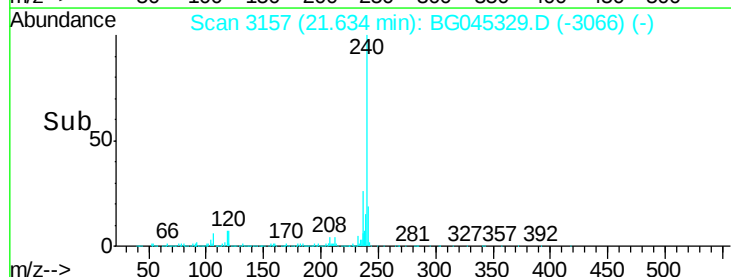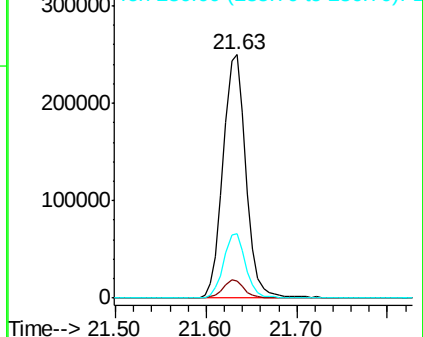

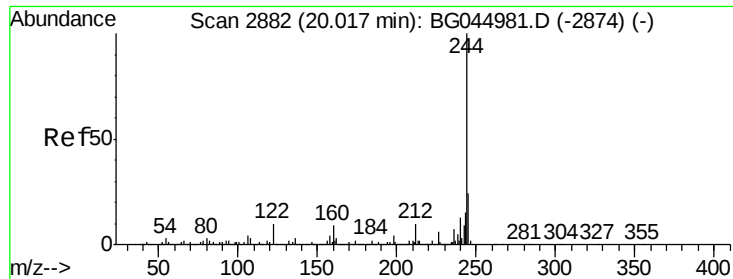

#79

Terphenyl-d14

Concen: 96.523 ng

RT: 19.98 min Scan# 2876

Delta R.T. 0.00 min

Lab File: BG045329.D

Acq: 12 May 2020 15:08

Instrument :

BNA_G

ClientSampleId :

PB128795BL


Tot Ion:244 Resp: 1946586

Ion Ratio Lower Upper

244 100

212 9.5 7.9 11.9




122 9.7 7.7 11.5

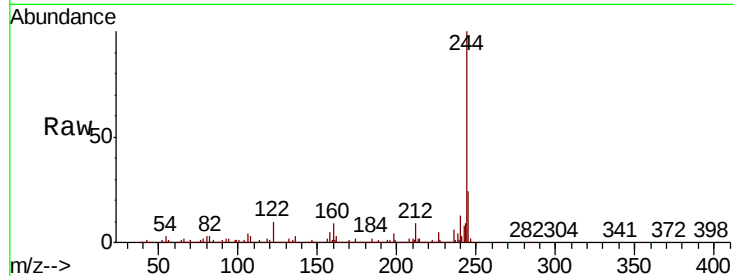

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

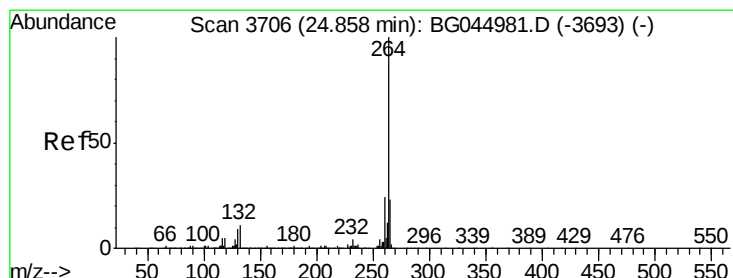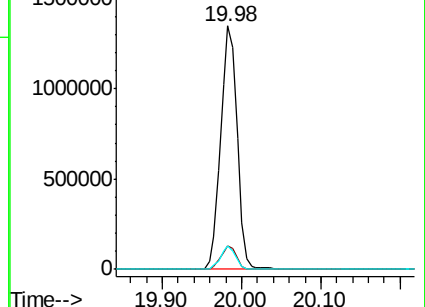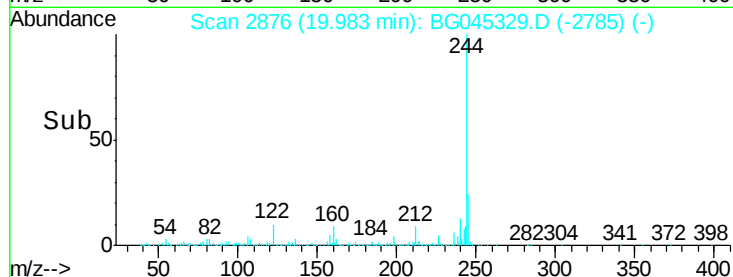

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.80 min Scan# 3696

Delta R.T. 0.00 min

Lab File: BG045329.D

Acq: 12 May 2020 15:08


Tgt Ion:264 Resp: 457116

Ion Ratio Lower Upper

264 100

260 23.1 19.2 28.8

265 21.7 19.0 28.4

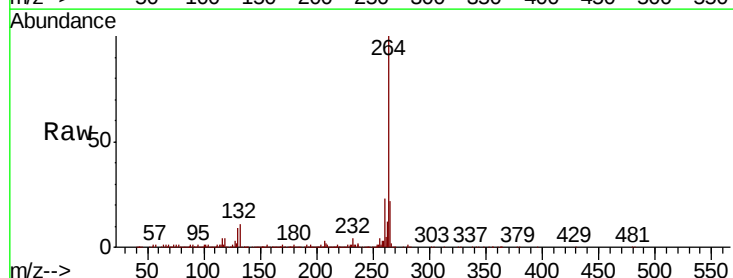

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

