


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051220\
 Data File : BG045327.D
 Acq On : 12 May 2020 13:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 11:40:01 2020

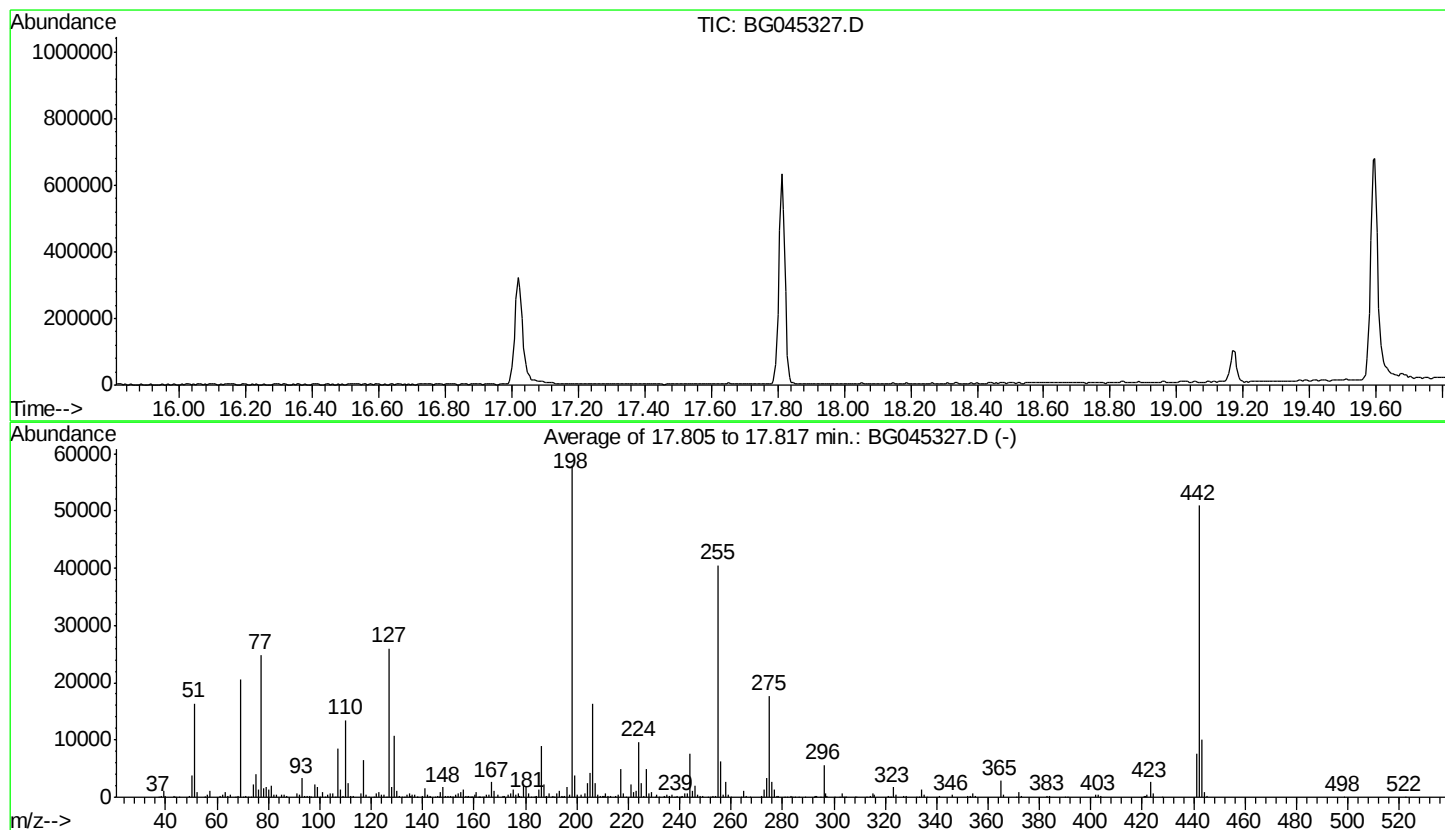

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	16342	PASS
68	69	0.00	2	0.7	139	PASS
69	198	0.00	100	35.4	20491	PASS
70	69	0.00	2	0.4	82	PASS
127	198	10	80	44.8	25957	PASS
197	198	0.00	2	0.7	384	PASS
198	198	100	100	100.0	57885	PASS
199	198	5	9	6.8	3913	PASS
275	198	10	60	30.6	17720	PASS
365	198	1	100	4.9	2813	PASS
441	198	0.01	100	13.2	7655	PASS
442	198	50	100	88.0	50946	PASS
443	442	15	24	19.8	10098	PASS