


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051220\
 Data File : BG045344.D
 Acq On : 13 May 2020 1:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 11:40:01 2020

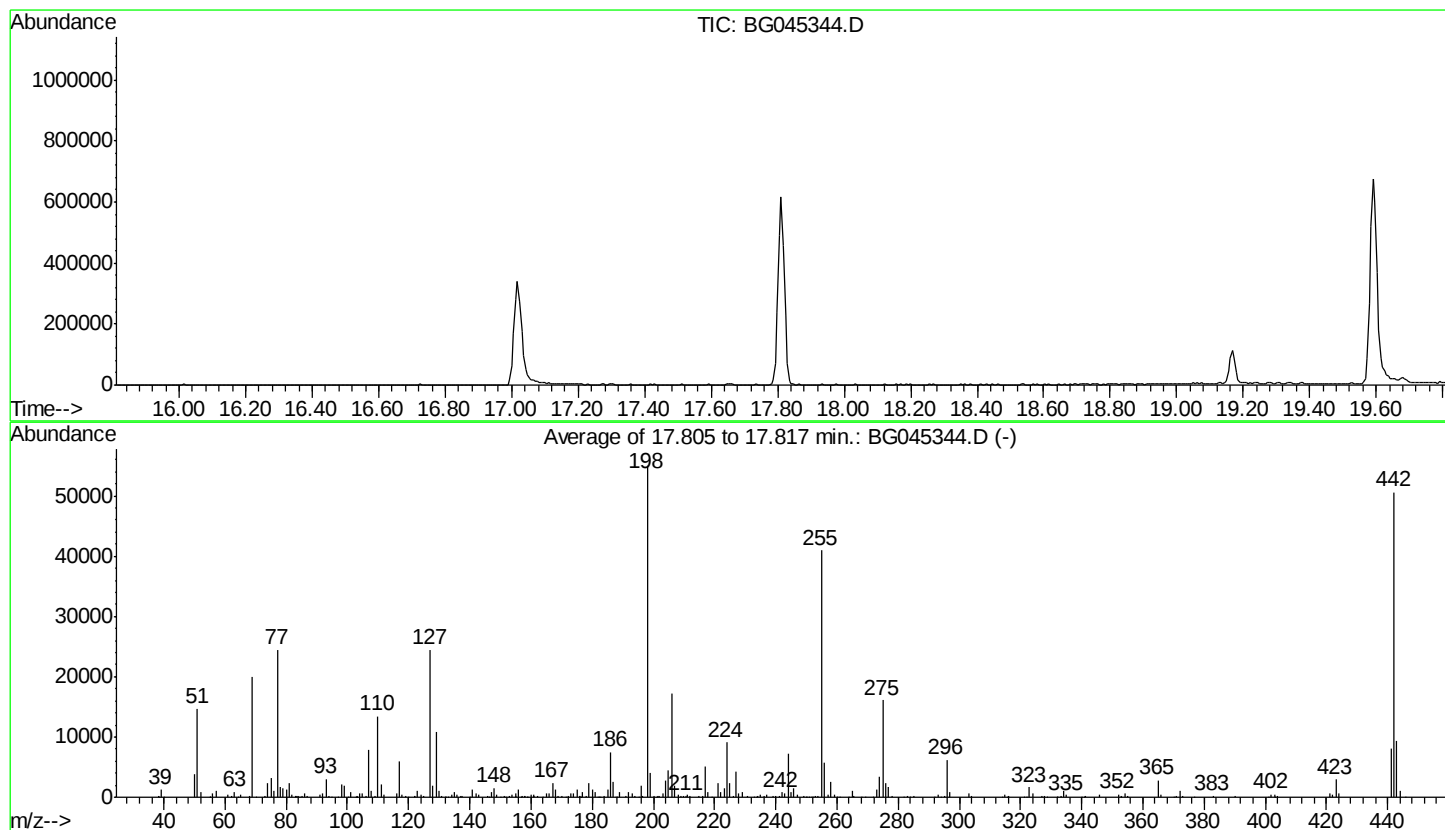

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	14769	PASS
68	69	0.00	2	0.6	120	PASS
69	198	0.00	100	36.3	19965	PASS
70	69	0.00	2	0.3	57	PASS
127	198	10	80	44.6	24517	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55026	PASS
199	198	5	9	7.3	3994	PASS
275	198	10	60	29.3	16107	PASS
365	198	1	100	5.1	2809	PASS
441	198	0.01	100	14.7	8096	PASS
442	198	50	100	92.0	50642	PASS
443	442	15	24	18.7	9457	PASS