
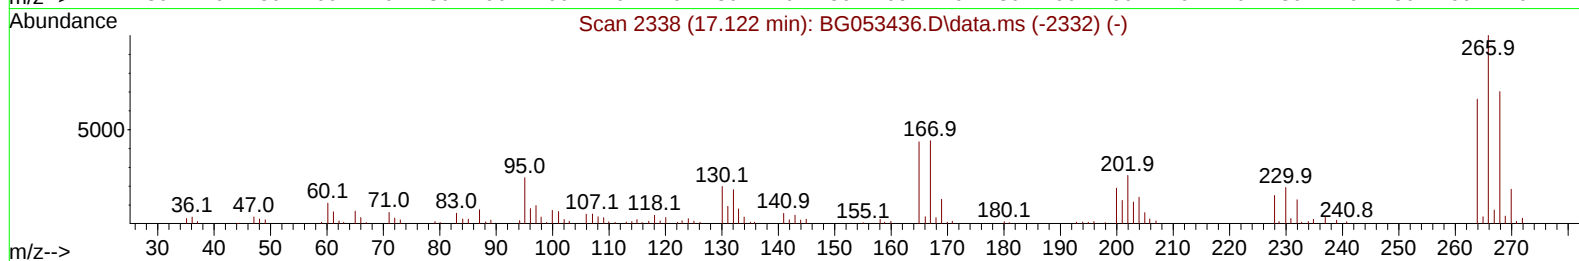
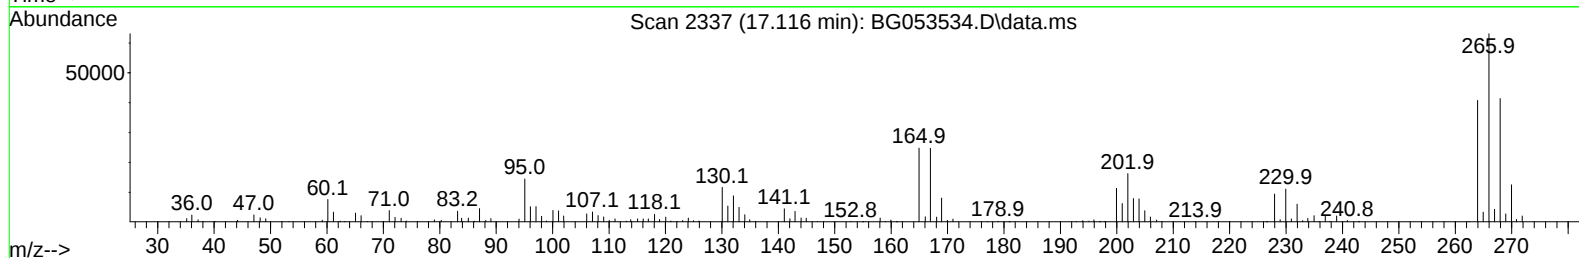


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051322\
Data File : BG053534.D
Acq On : 13 May 2022 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 05:53:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

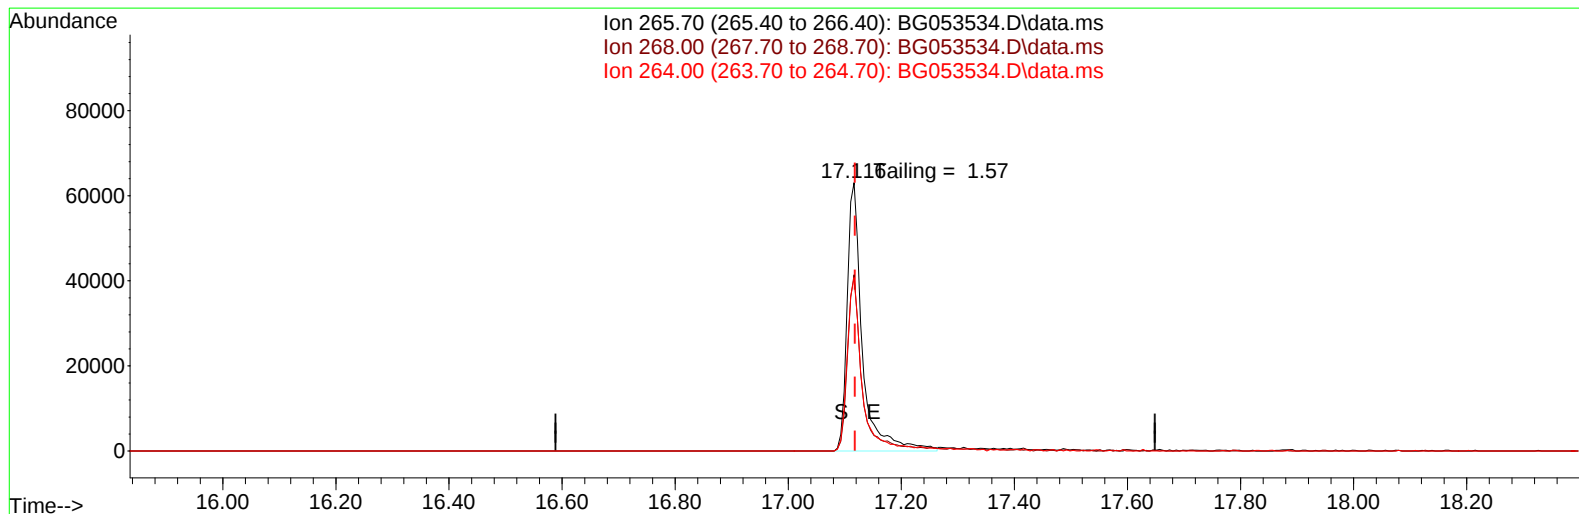

TIC: BG053534.D\data.ms

(70) Pentachlorophenol (C)




17.116min (-0.002) 28614.38 ng

response 118842

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.64
264.00	66.20	64.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051322\
Data File : BG053534.D
Acq On : 13 May 2022 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 05:53:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

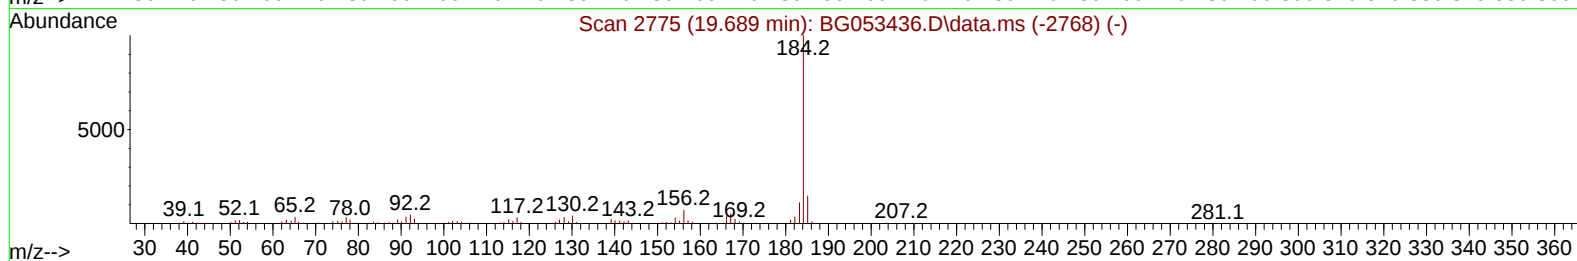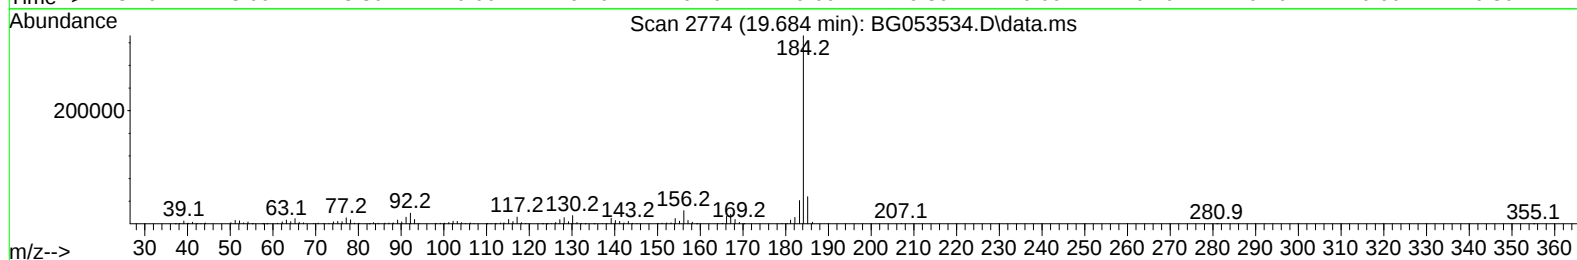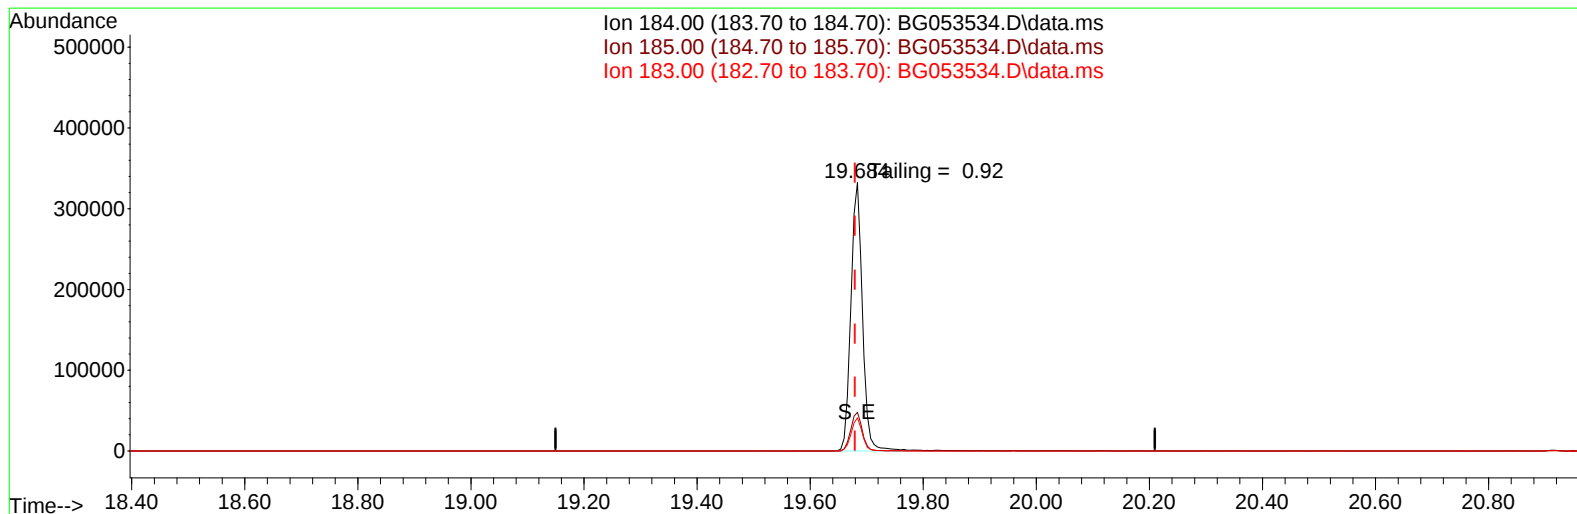

TIC: BG053534.D\data.ms

(77) Benzidine**19.684min (+ 0.004) 48733.17 ng****response 472671**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.44
183.00	11.10	12.37
0.00	0.00	0.00