

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051322\
 Data File : BG053548.D
 Acq On : 13 May 2022 18:26
 Operator : CG/JU
 Sample : N2823-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SC-9

Quant Time: May 14 03:14:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 11 06:00:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.084	152	25866	20.000	ng	0.00
21) Naphthalene-d8	10.892	136	107782	20.000	ng	0.00
39) Acenaphthene-d10	14.710	164	84193	20.000	ng	0.00
64) Phenanthrene-d10	17.454	188	195500	20.000	ng	0.00
76) Chrysene-d12	21.736	240	175980	20.000	ng	0.00
86) Perylene-d12	25.008	264	190034	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.652	112	89663	58.830	ng	0.00
7) Phenol-d6	7.256	99	196126	84.791	ng	0.00
23) Nitrobenzene-d5	9.247	82	93409	36.892	ng	0.00
42) 2,4,6-Tribromophenol	16.196	330	90095	72.555	ng	0.00
45) 2-Fluorobiphenyl	13.330	172	323081	56.075	ng	0.00
79) Terphenyl-d14	20.056	244	744635	78.808	ng	0.00
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	21.607	149	32381	5.616	ng	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051322\
Data File : BG053548.D
Acq On : 13 May 2022 18:26
Operator : CG/JU
Sample : N2823-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SC-9

Quant Time: May 14 03:14:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration




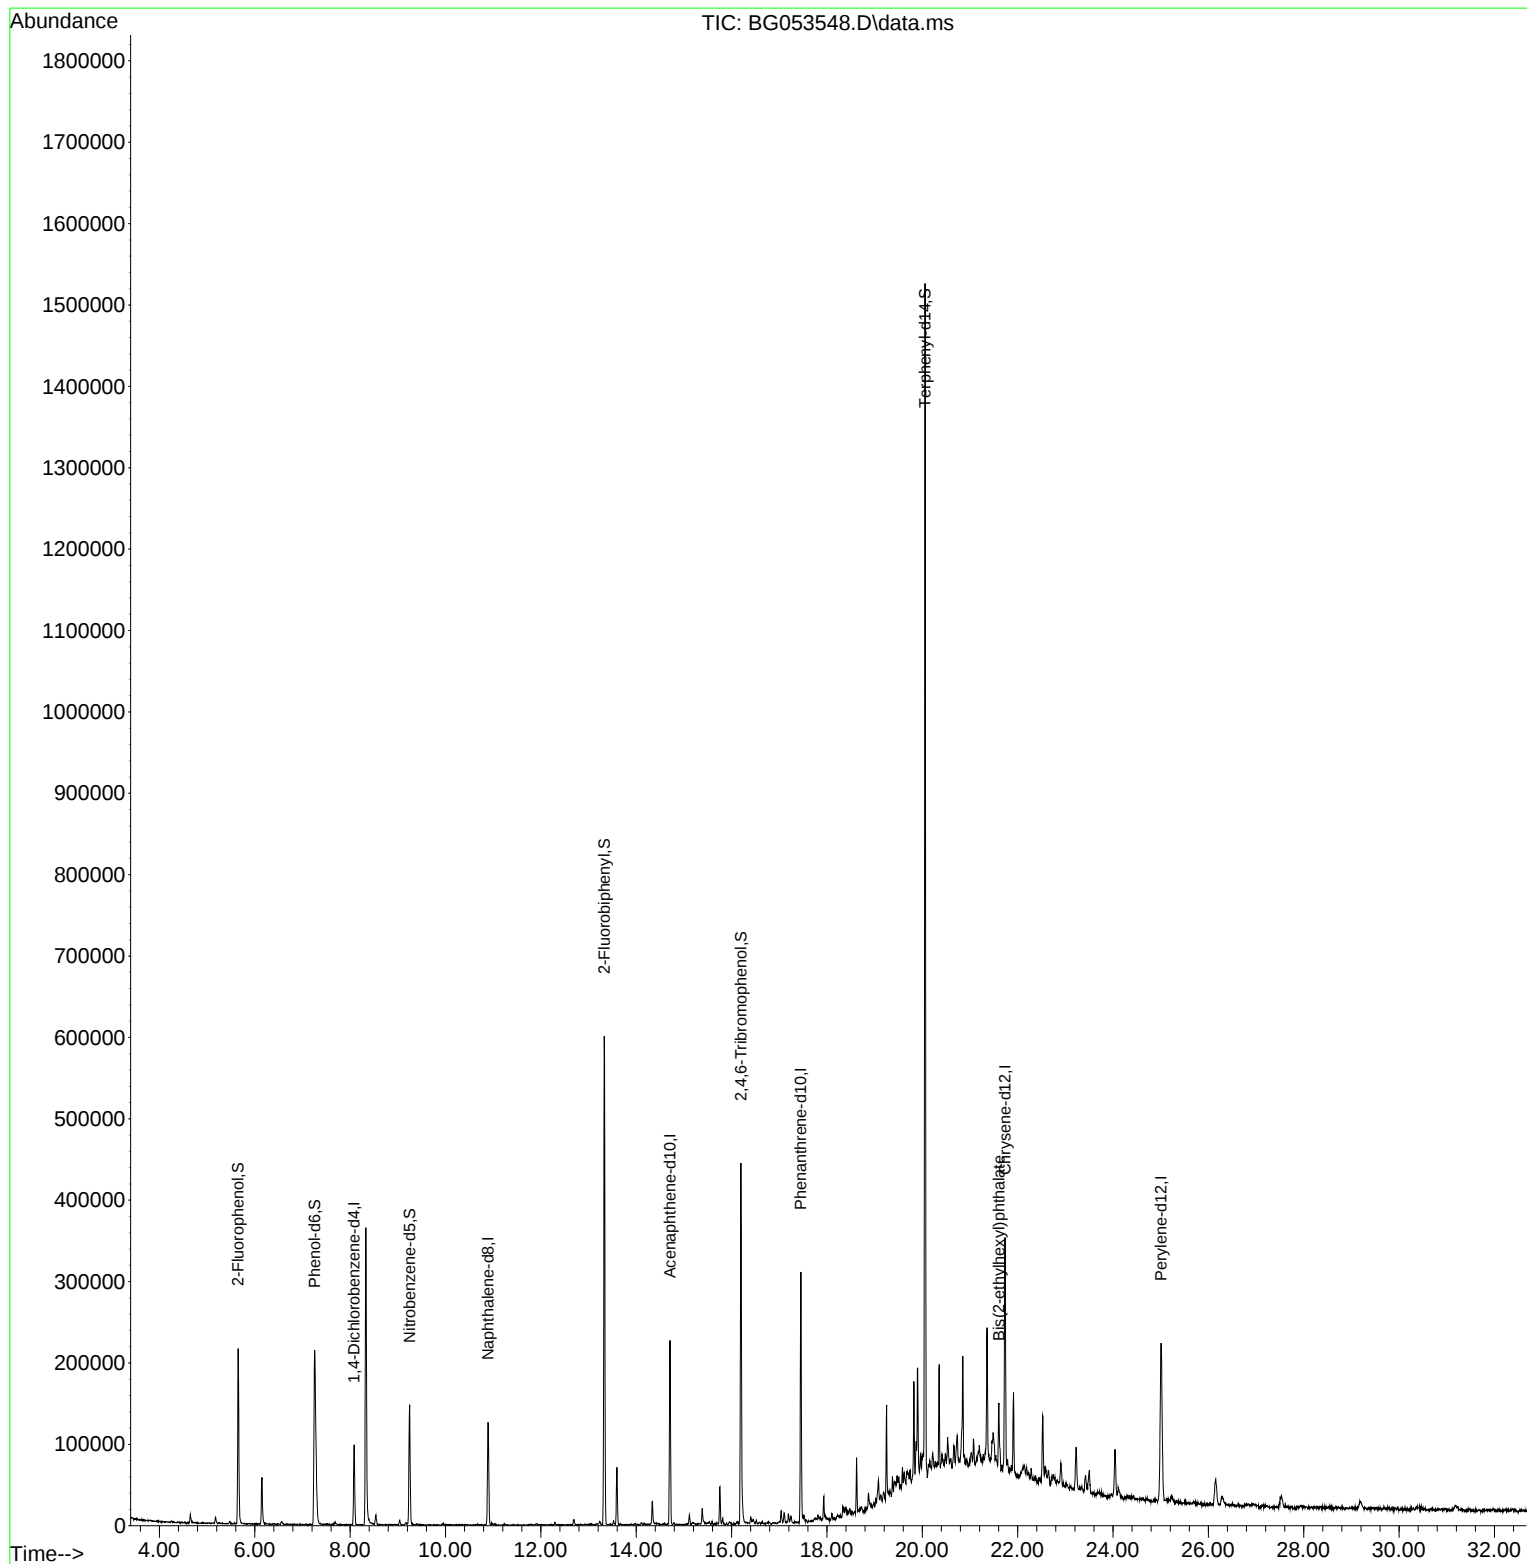


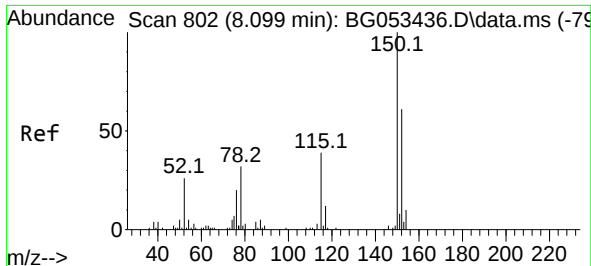

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.084 min Scan# 799
Delta R.T. -0.005 min
Lab File: BG053548.D
Acq: 13 May 2022 18:26




Instrument :
BNA_G
ClientSampleId :
SC-9


Tgt Ion:152 Resp: 25866
Ion Ratio Lower Upper
152 100
150 159.8 131.6 197.4
115 59.9 50.9 76.3

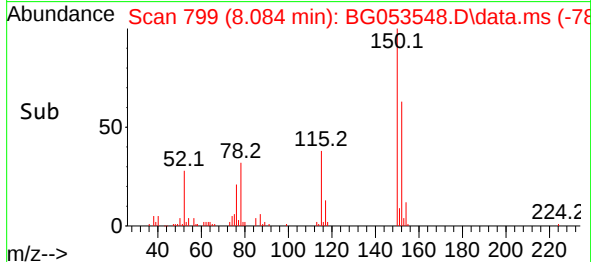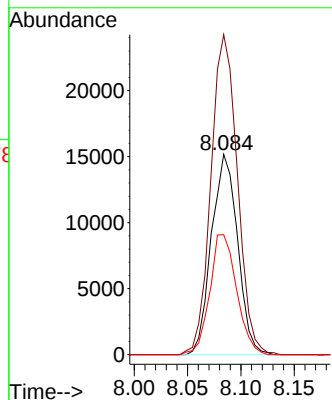

#5
2-Fluorophenol
Concen: 58.830 ng
RT: 5.652 min Scan# 385
Delta R.T. 0.000 min
Lab File: BG053548.D
Acq: 13 May 2022 18:26

Tgt Ion:112 Resp: 89663
Ion Ratio Lower Upper
112 100
64 68.9 55.1 82.7
63 39.1 30.4 45.6


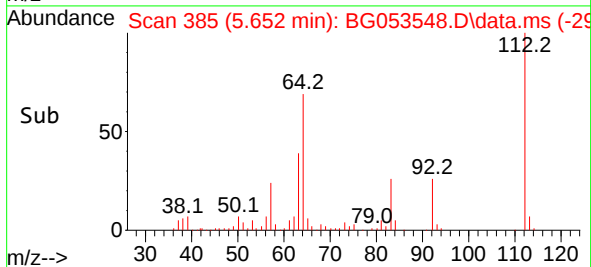
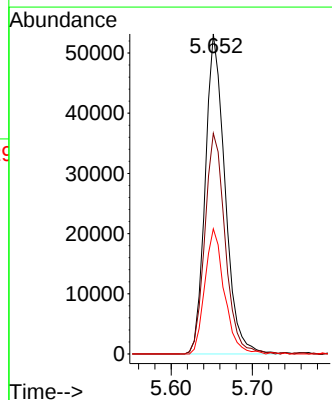
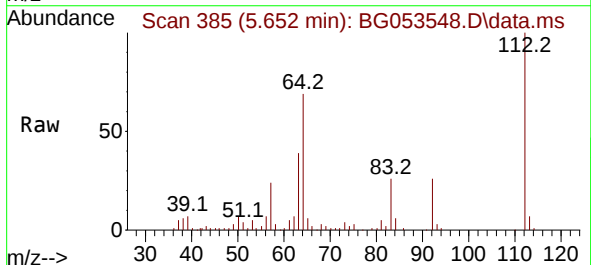


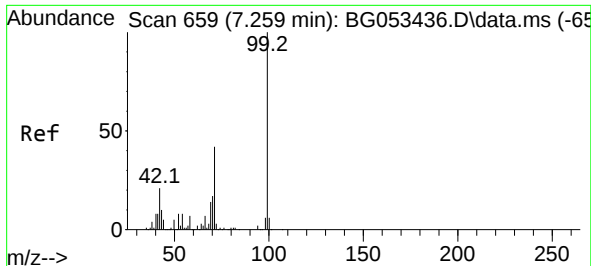

#7
Phenol-d6
Concen: 84.791 ng
RT: 7.256 min Scan# 61
Delta R.T. 0.006 min
Lab File: BG053548.D
Acq: 13 May 2022 18:26




Instrument :
BNA_G
ClientSampleId :
SC-9


Tgt Ion: 99 Resp: 196126
Ion Ratio Lower Upper
99 100
42 19.2 17.0 25.6
71 41.0 33.8 50.8

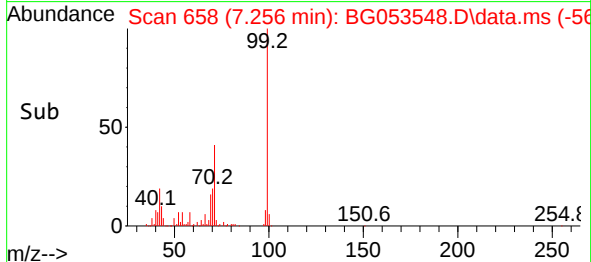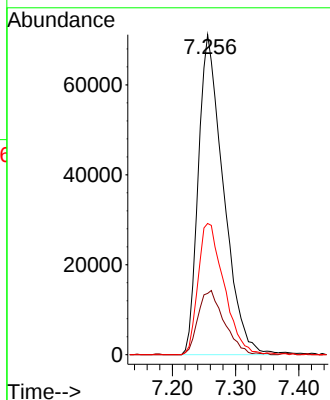

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.892 min Scan# 1277
Delta R.T. -0.006 min
Lab File: BG053548.D
Acq: 13 May 2022 18:26

Tgt Ion: 136 Resp: 107782
Ion Ratio Lower Upper
136 100
137 10.7 8.5 12.7
54 8.2 7.4 11.2
68 7.1 4.9 7.3

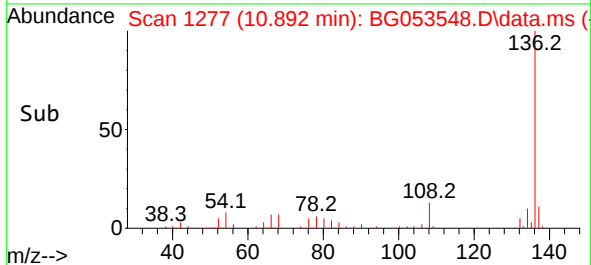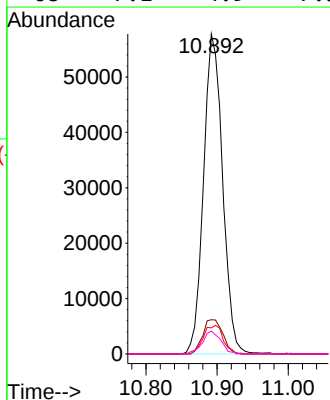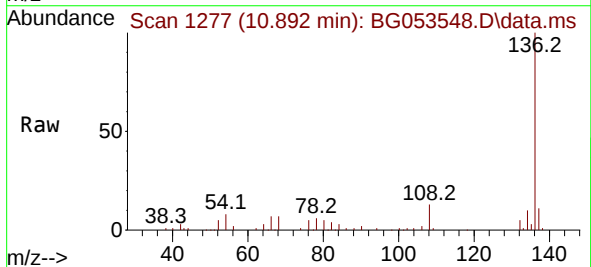



#23

Nitrobenzene-d5

Concen: 36.892 ng

RT: 9.247 min Scan# 91

Delta R.T. -0.006 min

Lab File: BG053548.D

Acq: 13 May 2022 18:26

Instrument :

BNA_G

ClientSampleId :

SC-9





Tgt Ion: 82 Resp: 93409

Ion Ratio Lower Upper

82 100

128 35.5 27.9 41.9

54 51.8 41.2 61.8

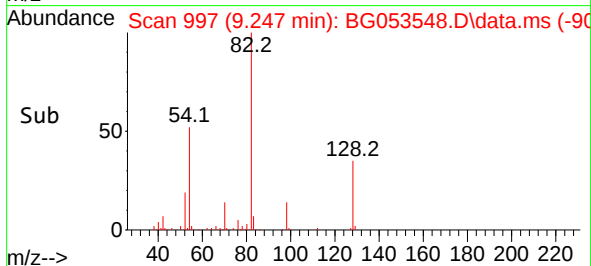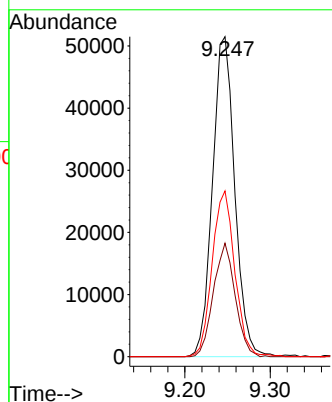

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.710 min Scan# 1927

Delta R.T. -0.006 min

Lab File: BG053548.D

Acq: 13 May 2022 18:26




Tgt Ion: 164 Resp: 84193


Ion Ratio Lower Upper

164 100

162 100.2 82.3 123.5

160 40.4 34.2 51.2


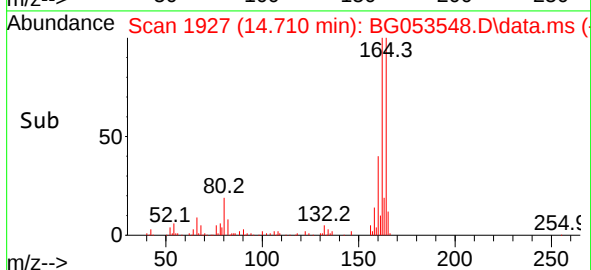
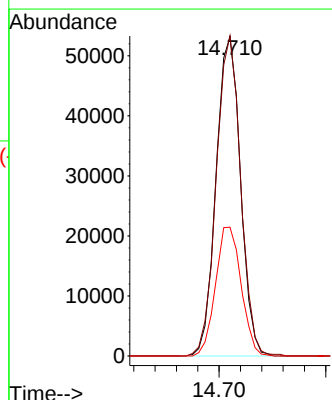
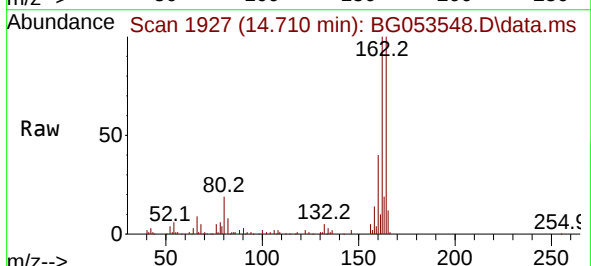


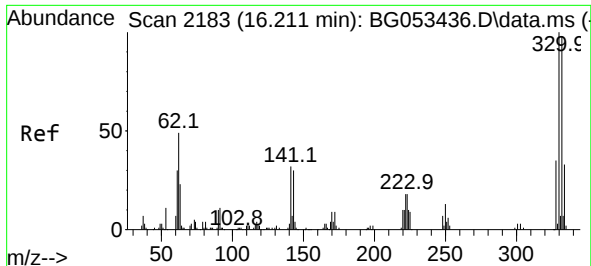

#42
2,4,6-Tribromophenol
Concen: 72.555 ng
RT: 16.196 min Scan# 2183
Delta R.T. -0.006 min
Lab File: BG053548.D
Acq: 13 May 2022 18:26




Instrument :
BNA_G
ClientSampleId :
SC-9


Tgt Ion:330 Resp: 90095
Ion Ratio Lower Upper
330 100
332 94.7 76.0 114.0
141 33.9 27.1 40.7

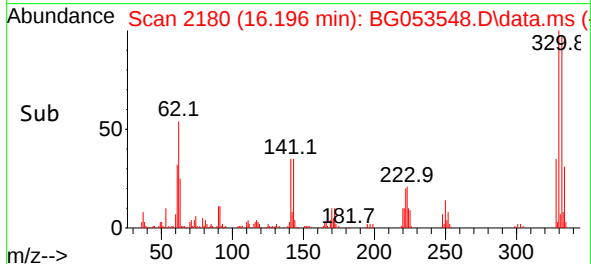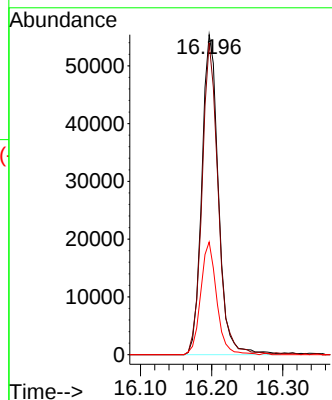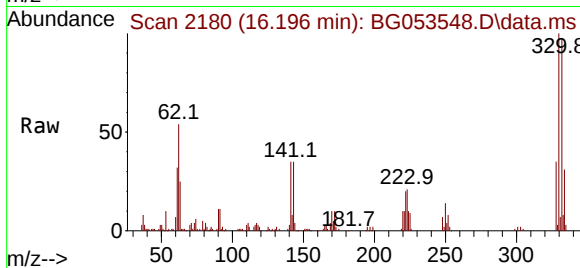

#45
2-Fluorobiphenyl
Concen: 56.075 ng
RT: 13.330 min Scan# 1692
Delta R.T. -0.006 min
Lab File: BG053548.D
Acq: 13 May 2022 18:26

Tgt Ion:172 Resp: 323081
Ion Ratio Lower Upper
172 100
171 35.0 28.5 42.7
170 22.4 18.9 28.3


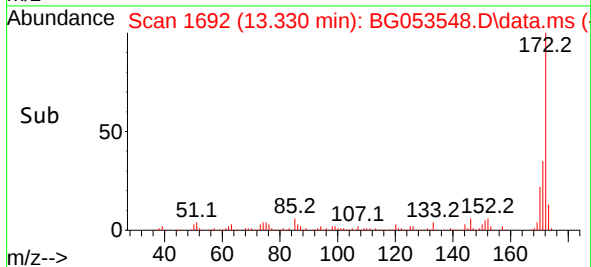
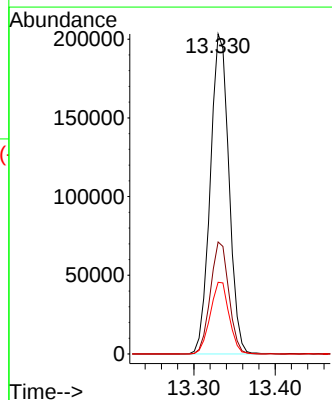
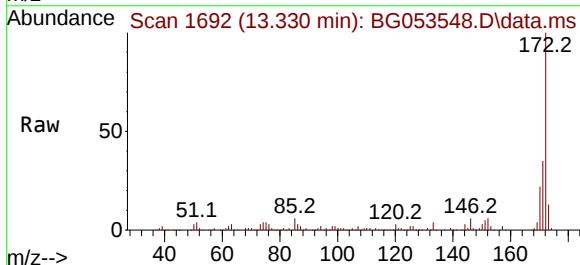


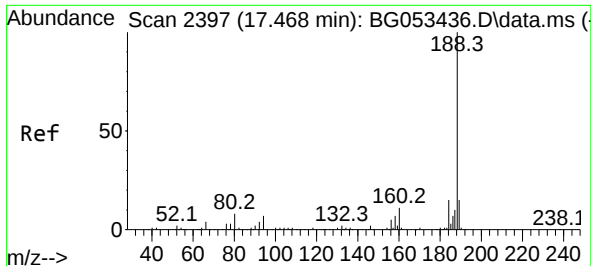

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.454 min Scan# 21
Delta R.T. -0.006 min
Lab File: BG053548.D
Acq: 13 May 2022 18:26




Instrument :
BNA_G
ClientSampleId :
SC-9


Tgt Ion:188 Resp: 195500
Ion Ratio Lower Upper
188 100
94 7.0 5.4 8.0
80 8.6 6.8 10.2

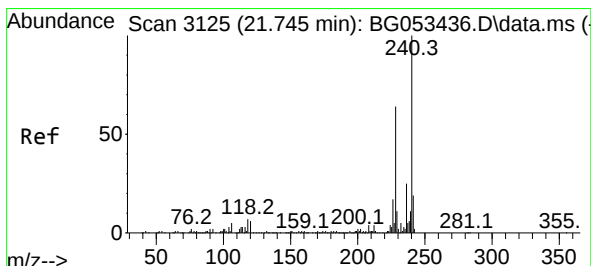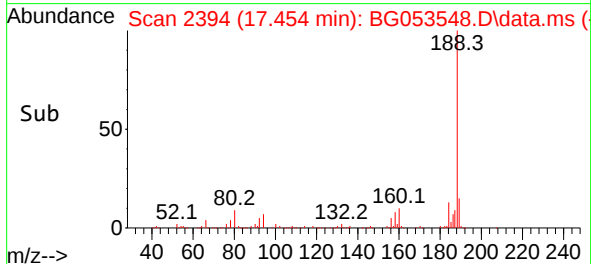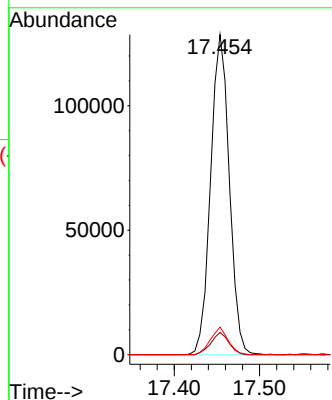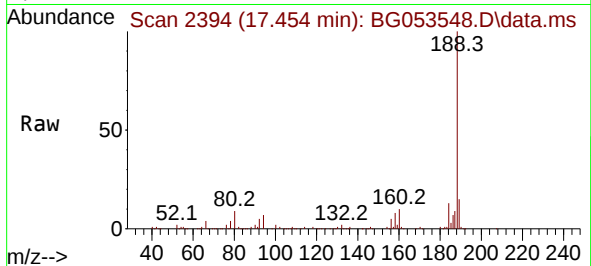

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.736 min Scan# 3123
Delta R.T. -0.006 min
Lab File: BG053548.D
Acq: 13 May 2022 18:26

Tgt Ion:240 Resp: 175980
Ion Ratio Lower Upper
240 100
120 6.3 4.6 7.0
236 24.5 20.2 30.4

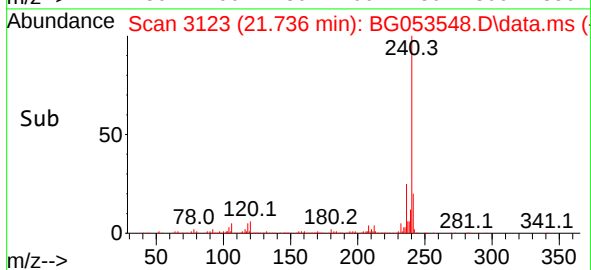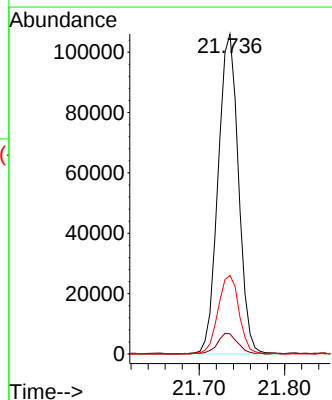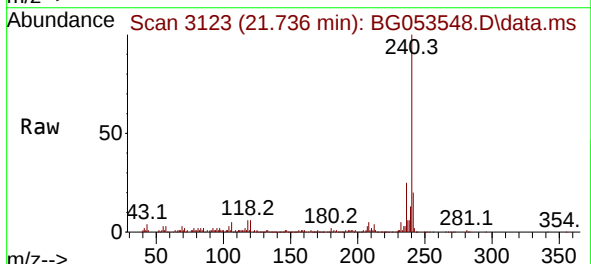



#79

Terphenyl-d14

Concen: 78.808 ng

RT: 20.056 min Scan# 21

Delta R.T. -0.006 min

Lab File: BG053548.D

Acq: 13 May 2022 18:26

Instrument :

BNA_G

ClientSampleId :

SC-9





Tgt Ion:244 Resp: 744635

Ion Ratio Lower Upper

244 100

212 7.4 6.5 9.7

122 6.4 5.0 7.4

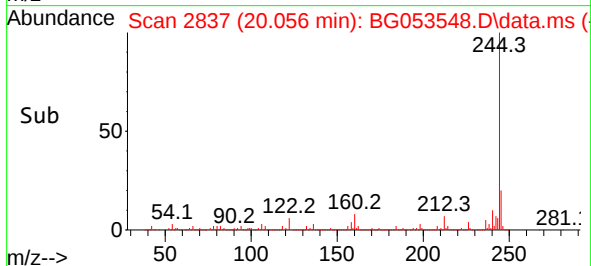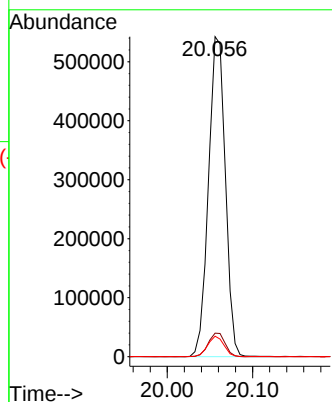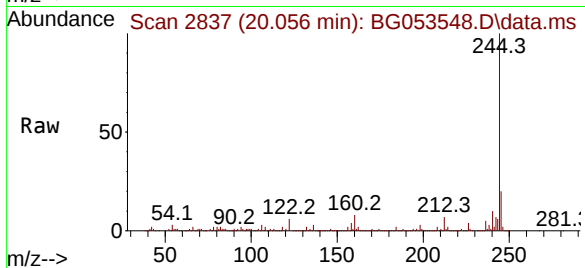

#84

Bis(2-ethylhexyl)phthalate

Concen: 5.616 ng

RT: 21.607 min Scan# 3101

Delta R.T. 0.000 min

Lab File: BG053548.D

Acq: 13 May 2022 18:26




Tgt Ion:149 Resp: 32381


Ion Ratio Lower Upper

149 100

167 28.2 20.2 30.4

279 4.7 3.6 5.4

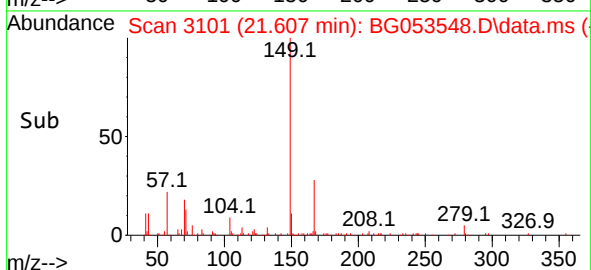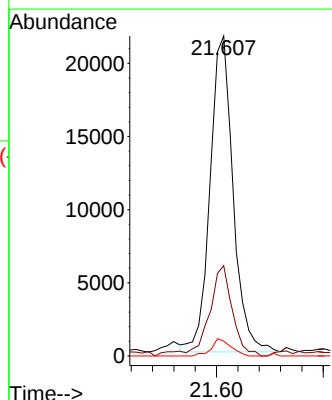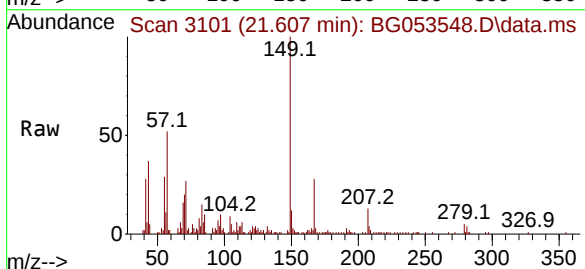

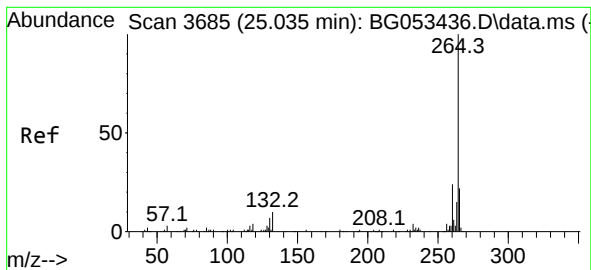

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.008 min Scan# 30
 Delta R.T. -0.011 min
 Lab File: BG053548.D
 Acq: 13 May 2022 18:26

Instrument :
 BNA_G
 ClientSampleId :
 SC-9

Tgt Ion:264 Resp: 190034
 Ion Ratio Lower Upper
 264 100
 260 22.8 19.0 28.6
 265 21.7 17.4 26.2

