
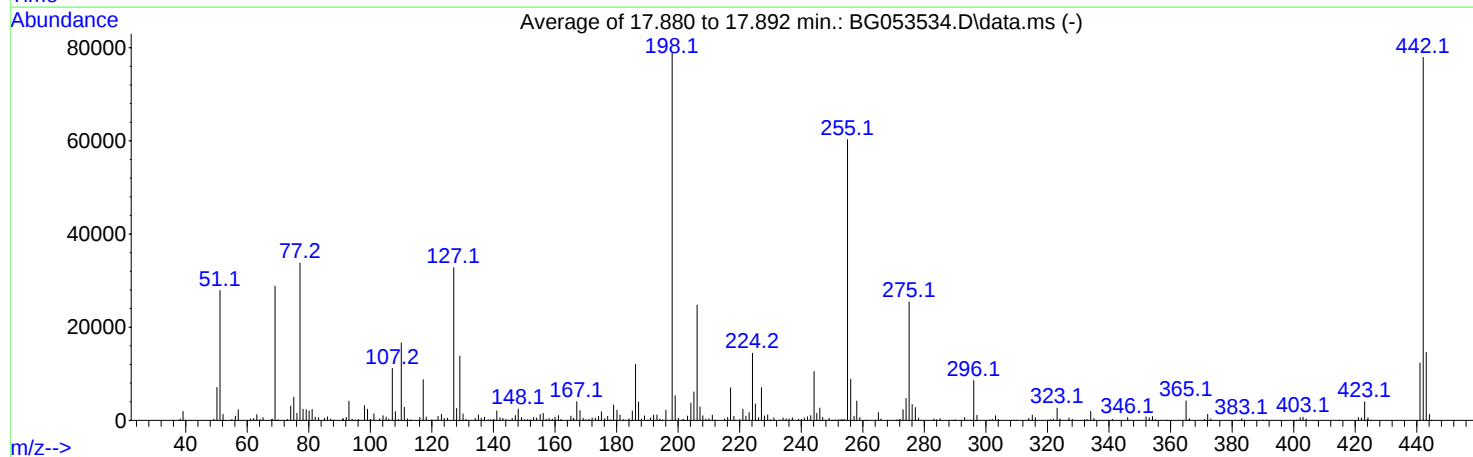


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051322\
 Data File : BG053534.D
 Acq On : 13 May 2022 9:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 11 06:00:46 2022

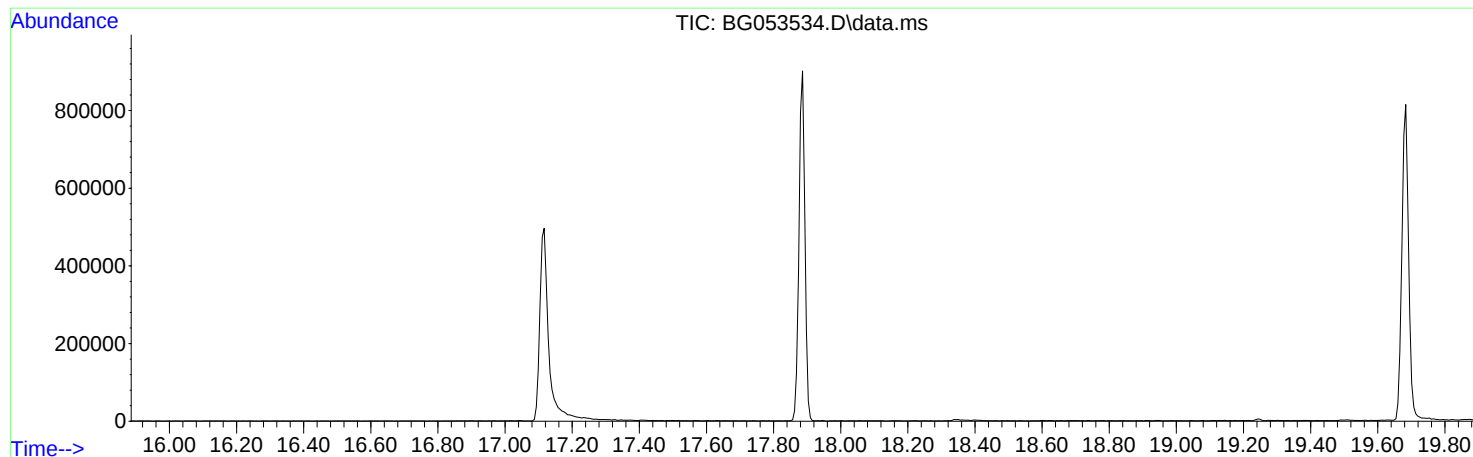




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	27877	PASS
68	69	0.00	2	0.9	248	PASS
69	198	0.00	100	36.5	28824	PASS
70	69	0.00	2	0.3	85	PASS
127	198	10	80	41.5	32760	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78971	PASS
199	198	5	9	6.7	5311	PASS
275	198	10	60	32.2	25408	PASS
365	198	1	100	5.3	4181	PASS
441	198	0.01	100	15.6	12341	PASS
442	442	50	100	100.0	77909	PASS
443	442	15	24	18.8	14615	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051322\
Data File : BG053534.D
Acq On : 13 May 2022 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 14 05:53:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

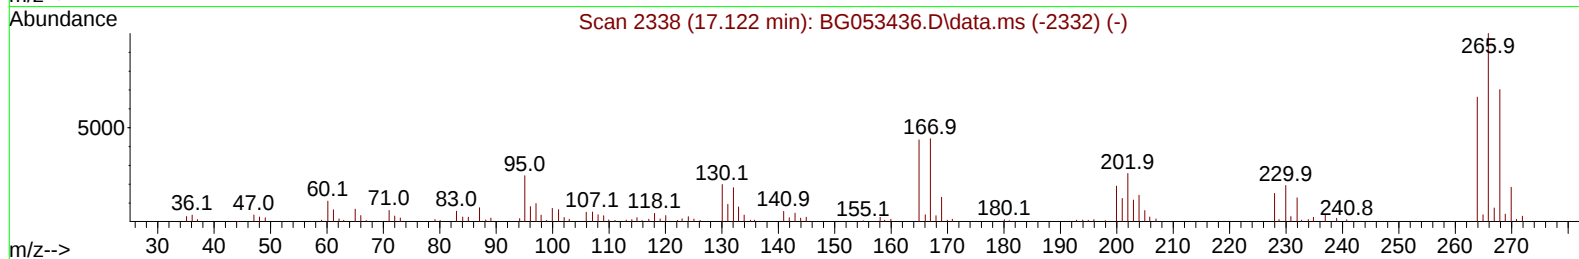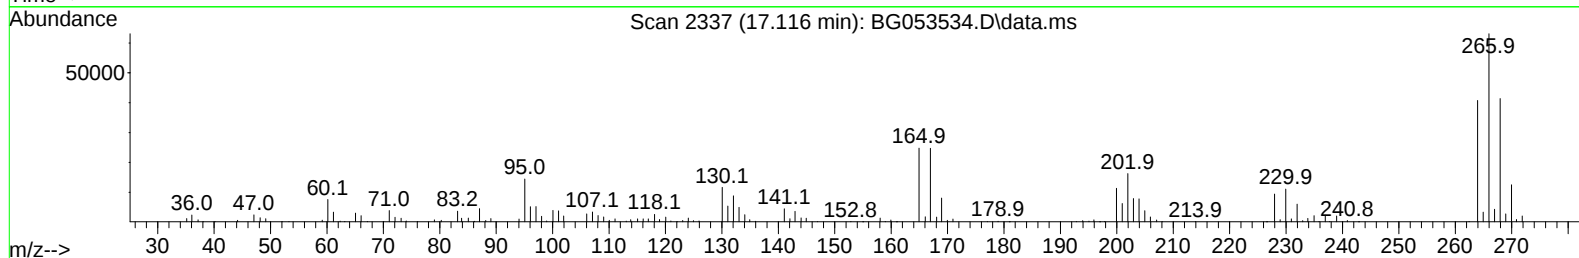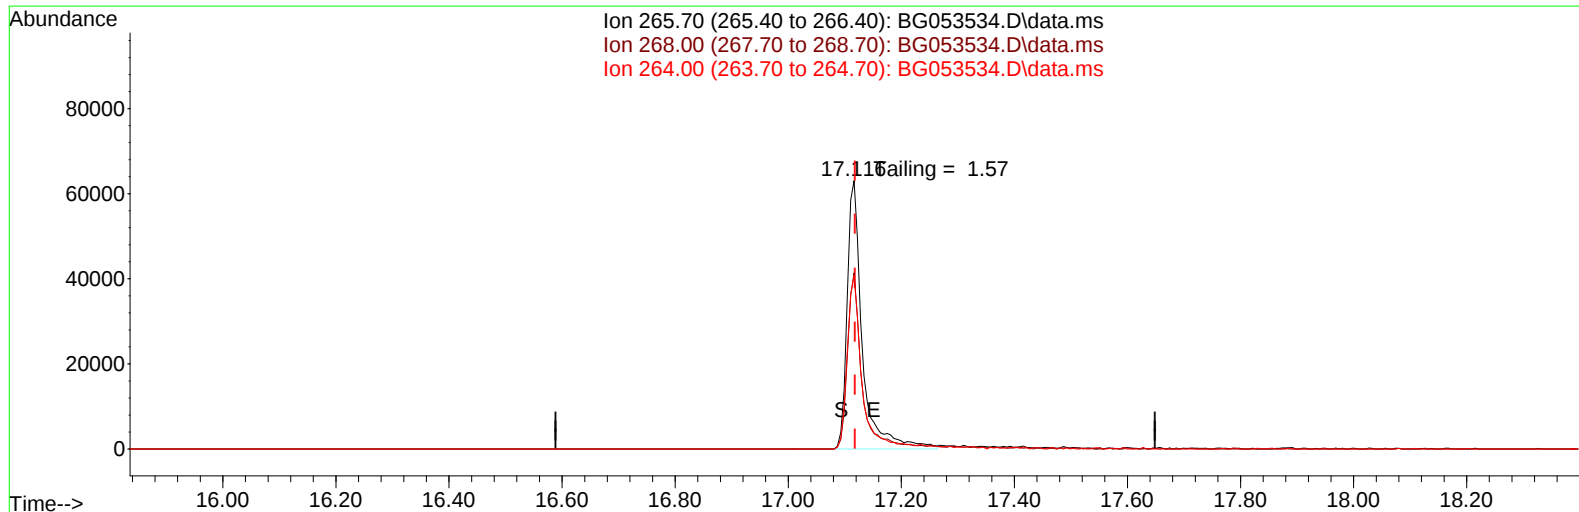

TIC: BG053534.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.002) 28614.38 ng




response 118842

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.64
264.00	66.20	64.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051322\
Data File : BG053534.D
Acq On : 13 May 2022 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 14 05:53:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

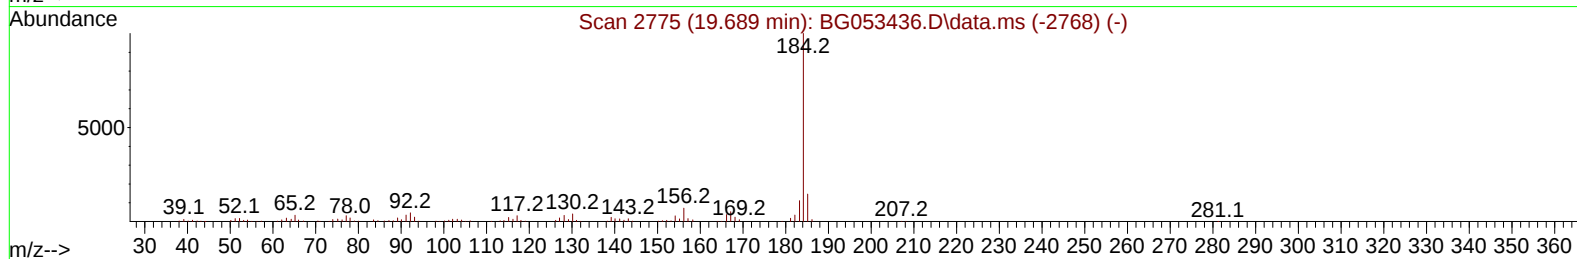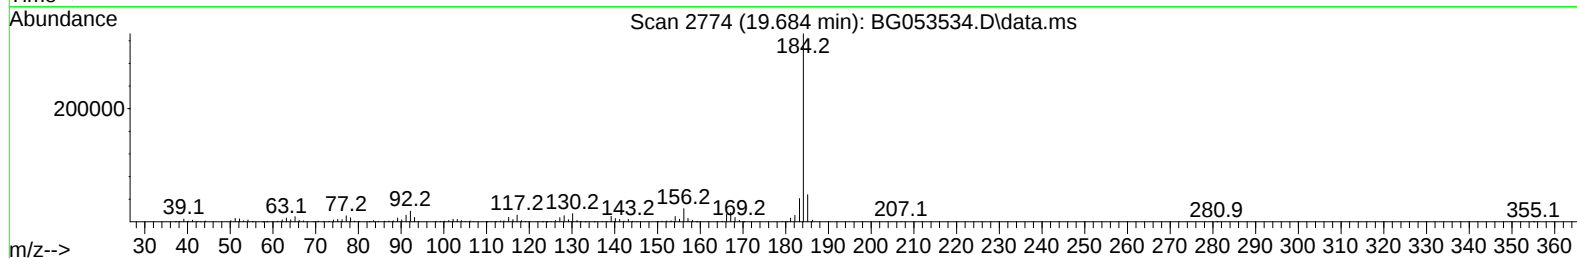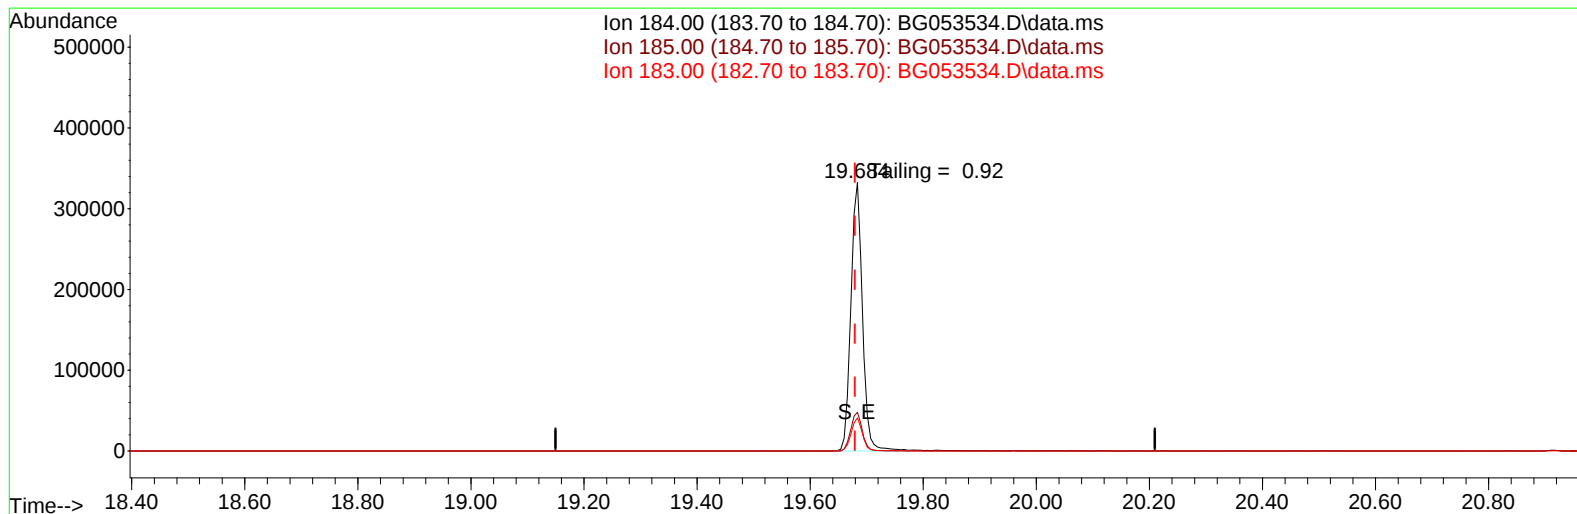

TIC: BG053534.D\data.ms

(77) Benzdine

19.684min (+ 0.004) 48733.17 ng

response 472671

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.44
183.00	11.10	12.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/13/2022	BNA_G	<u>BG053534.D</u>
Compound Name	Response	Retention Time
DDT	260059	20.917
DDD	9401	20.471
DDE	517	19.966
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9918	269977	3.67

Instrument :
BNA_G
ClientSampleId :
DFTPP