
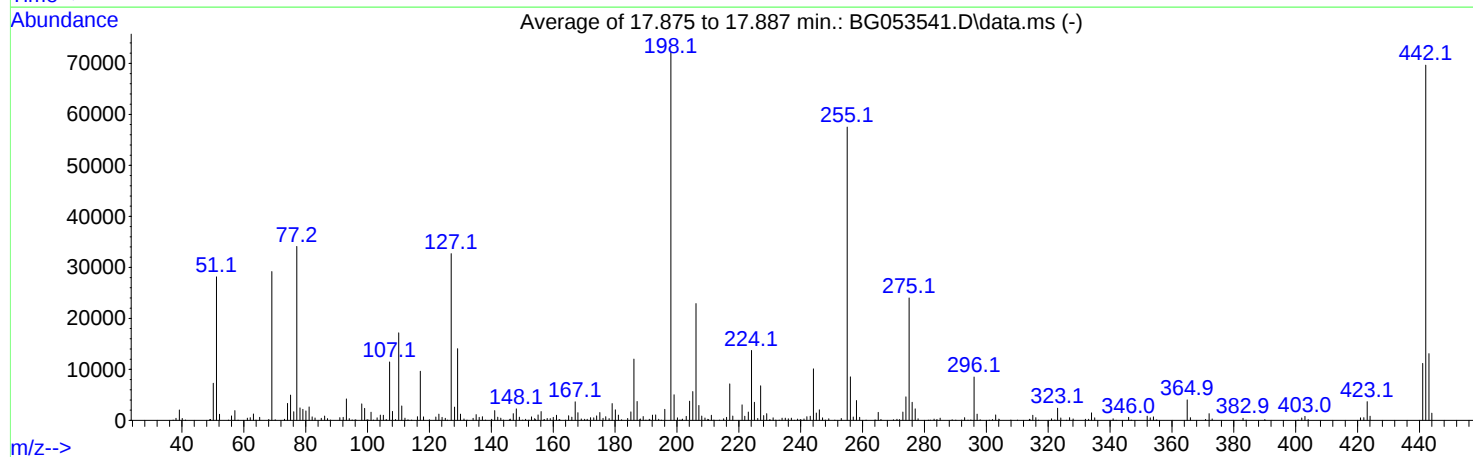


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051322\
 Data File : BG053541.D
 Acq On : 13 May 2022 13:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 11 06:00:46 2022

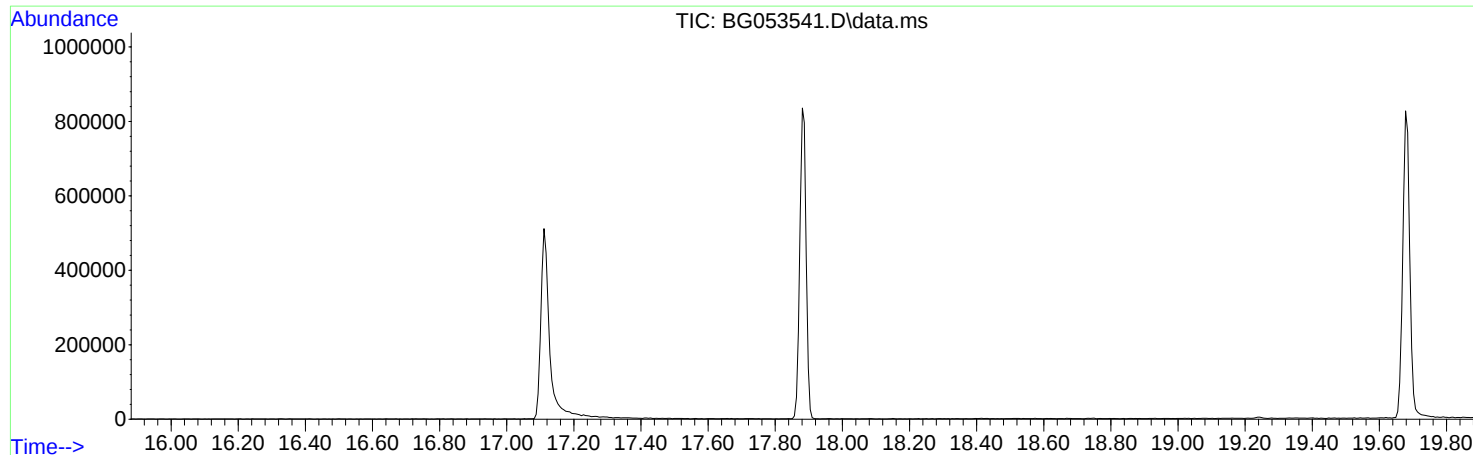




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	28157	PASS
68	69	0.00	2	0.6	181	PASS
69	198	0.00	100	40.4	29176	PASS
70	69	0.00	2	0.4	127	PASS
127	198	10	80	45.3	32693	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72131	PASS
199	198	5	9	7.0	5023	PASS
275	198	10	60	33.3	23997	PASS
365	198	1	100	5.6	4009	PASS
441	198	0.01	100	15.5	11169	PASS
442	442	50	100	100.0	69667	PASS
443	442	15	24	18.8	13074	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051322\
Data File : BG053541.D
Acq On : 13 May 2022 13:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 13 18:05:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

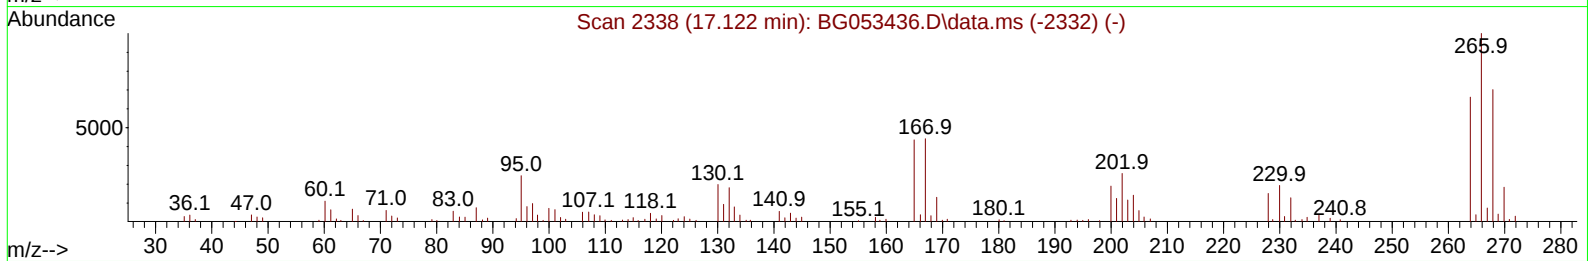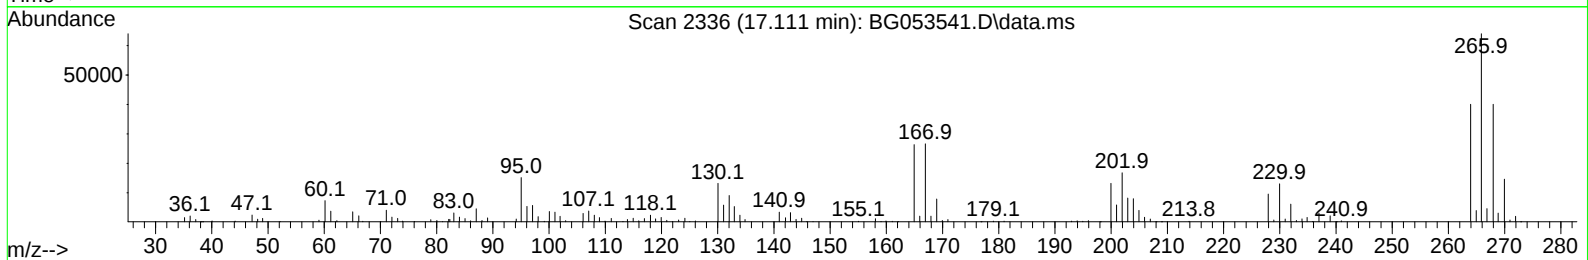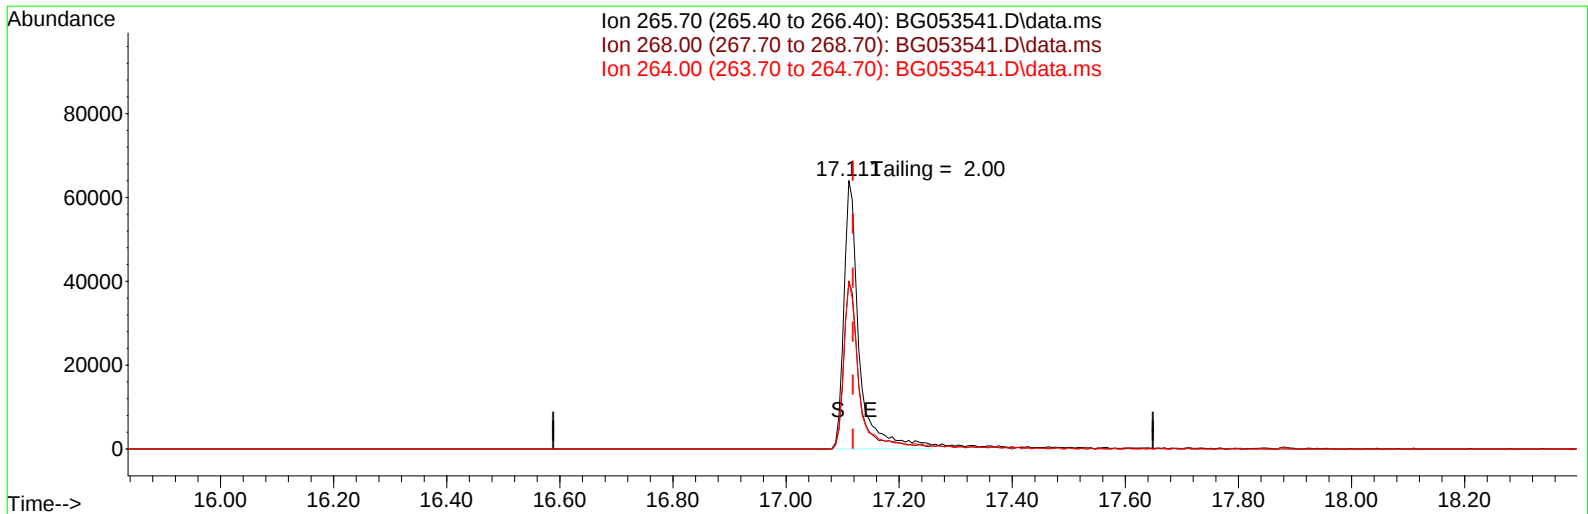

TIC: BG053541.D\data.ms

(70) Pentachlorophenol (C)

17.111min (-0.007) 31938.60 ng




response 118171

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	62.61
264.00	66.20	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051322\
Data File : BG053541.D
Acq On : 13 May 2022 13:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 13 18:05:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

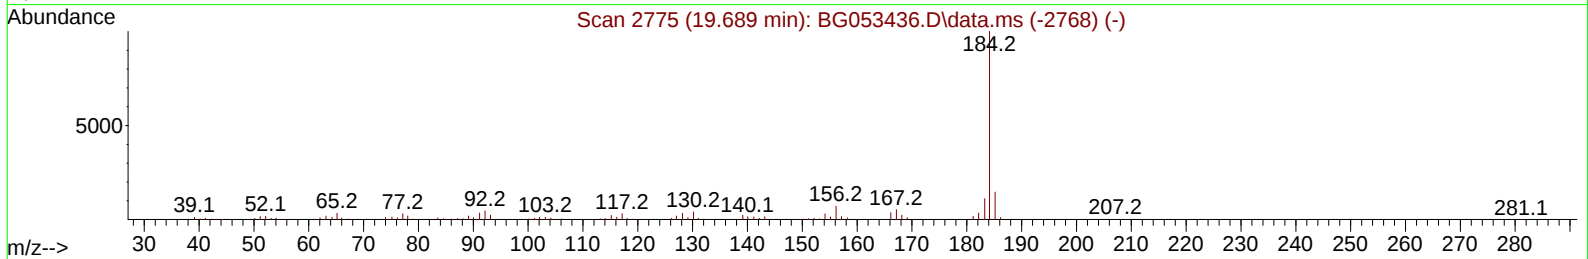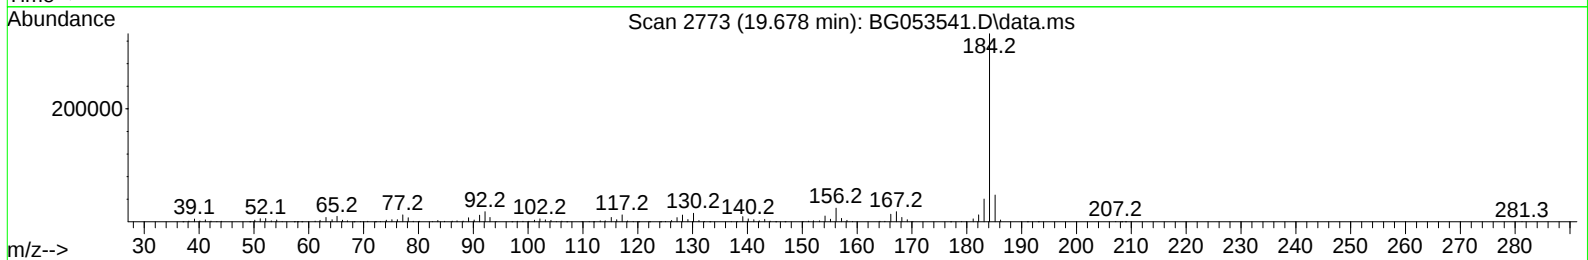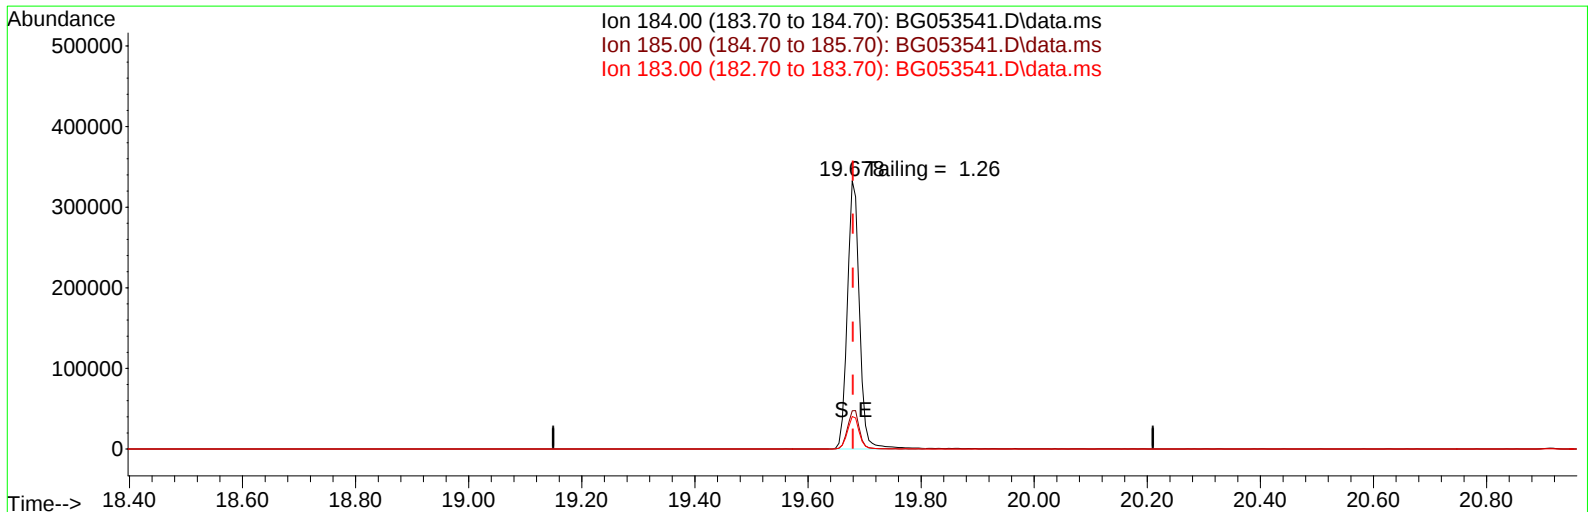

TIC: BG053541.D\data.ms

(77) Benzidine

19.678min (-0.001) 0.00 ng

response 494949

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.27
183.00	11.10	12.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/13/2022	BNA_G	<u>BG053541.D</u>
Compound Name	Response	Retention Time
DDT	258182	20.912
DDD	11783	20.471
DDE	730	19.966
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12513	270695	4.62

Instrument :
BNA_G
ClientSampleId :
DFTPP