
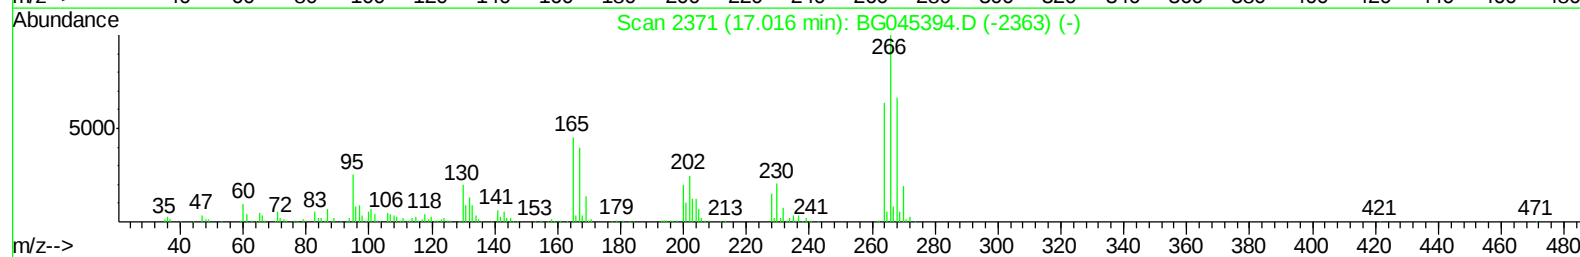
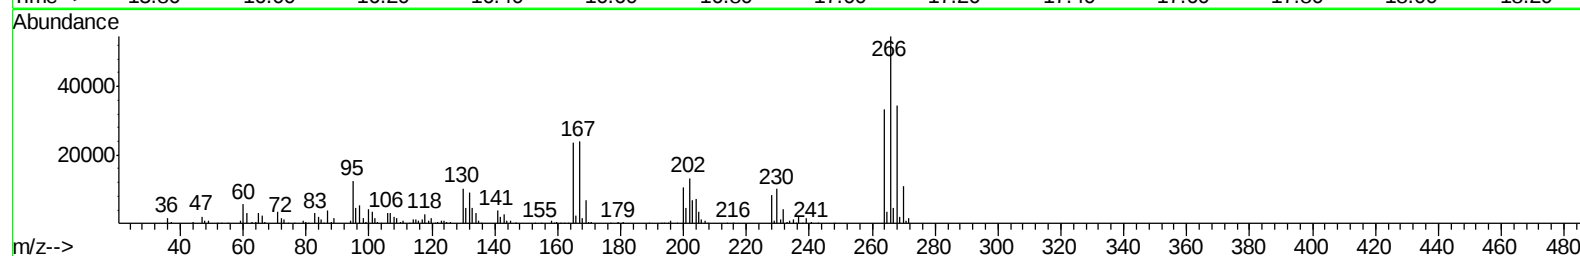


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051520\
 Data File : BG045391.D
 Acq On : 15 May 2020 10:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 01:59:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 15 15:45:48 2020
 Response via : Initial Calibration

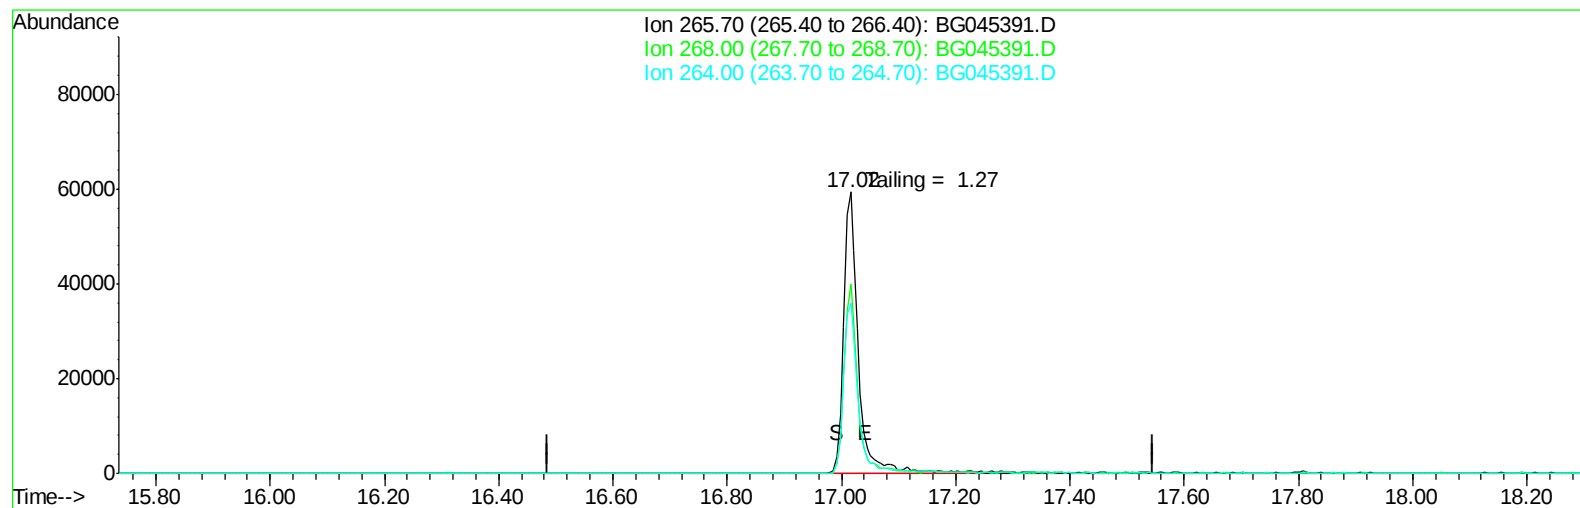

TIC: BG045391.D

(70) Pentachlorophenol (C)




17.016min (-17.016) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	66.50	0.00#
264.00	63.70	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051520\
 Data File : BG045391.D
 Acq On : 15 May 2020 10:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 01:59:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 15 15:45:48 2020
 Response via : Initial Calibration

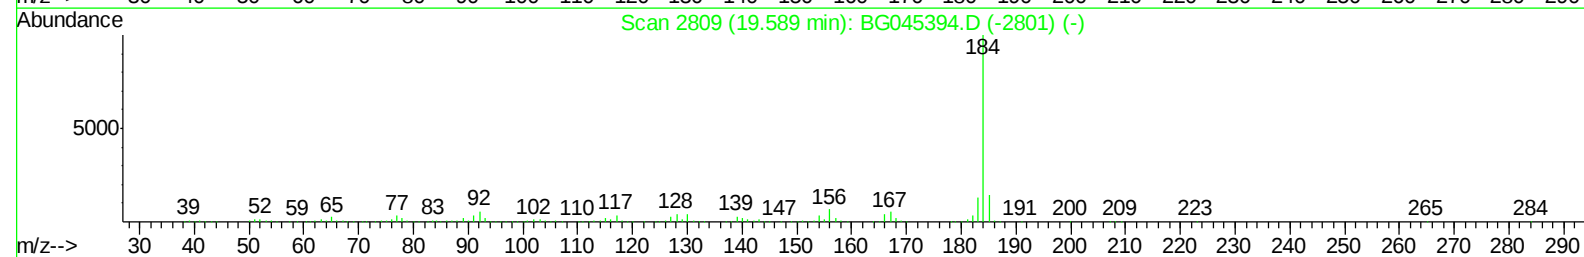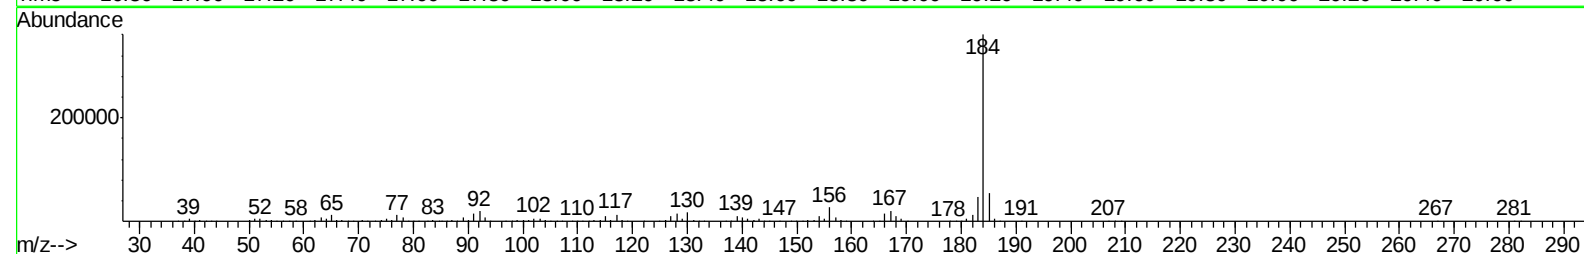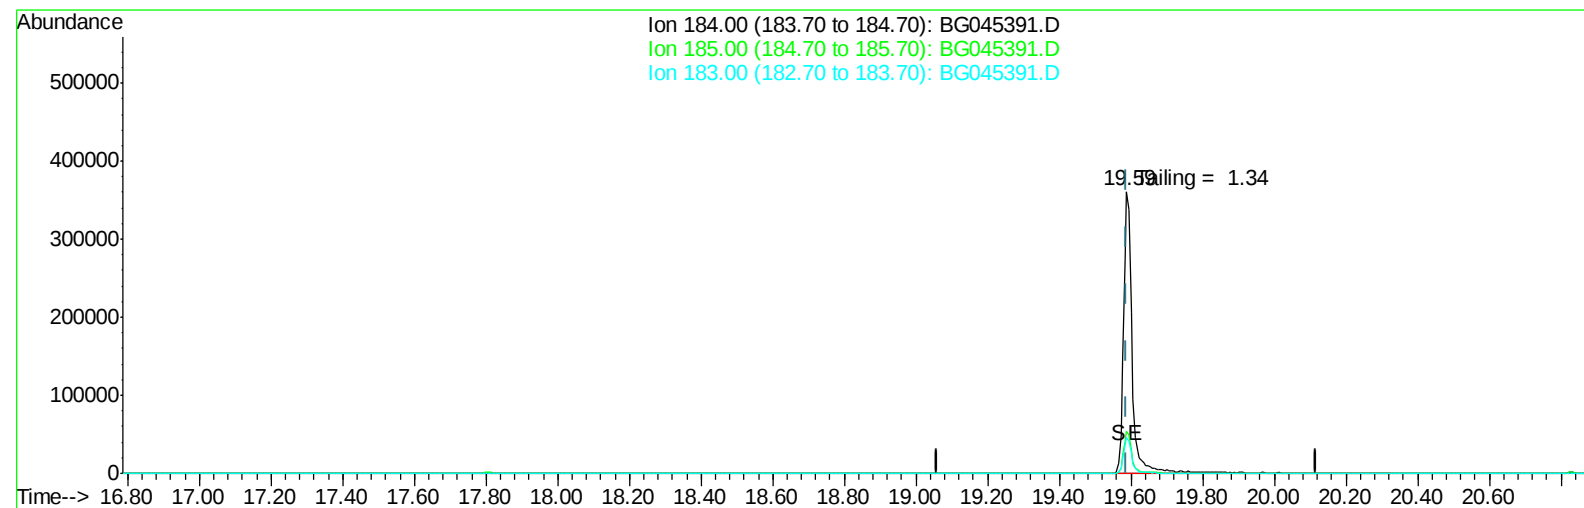

TIC: BG045391.D

(77) Benzidine

17.809min (-1.780) 266.14ng

response 441

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	449.70#
183.00	12.80	0.00#
0.00	0.00	0.00