


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG051520\
 Data File : BG045391.D
 Acq On : 15 May 2020 10:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 15 15:45:48 2020

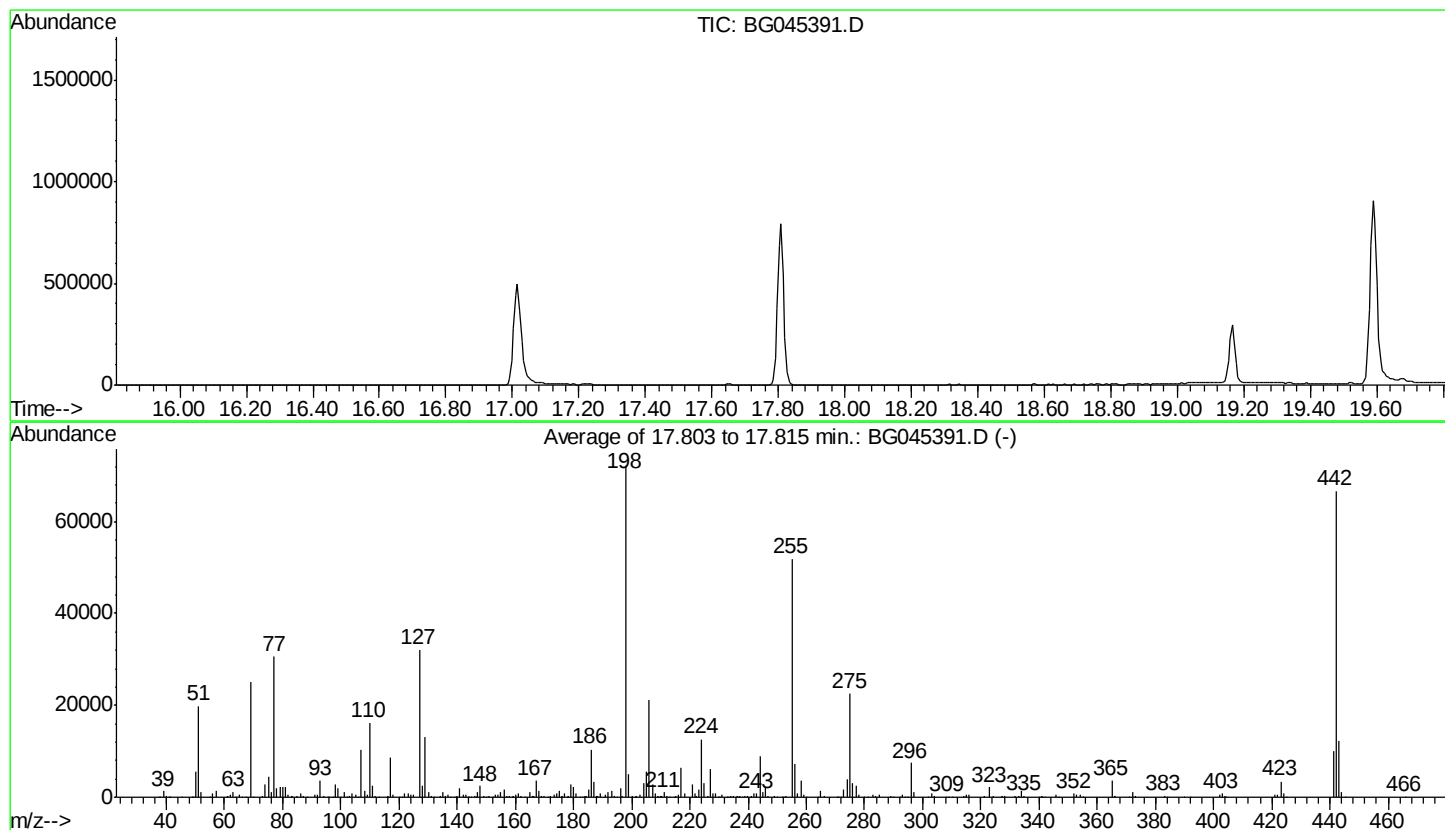

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	19836	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.7	25029	PASS
70	69	0.00	2	0.4	111	PASS
127	198	10	80	44.6	32162	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72168	PASS
199	198	5	9	6.9	4954	PASS
275	198	10	60	31.1	22464	PASS
365	198	1	100	4.9	3558	PASS
441	198	0.01	100	13.8	9989	PASS
442	198	50	100	92.4	66656	PASS
443	442	15	24	18.4	12276	PASS