
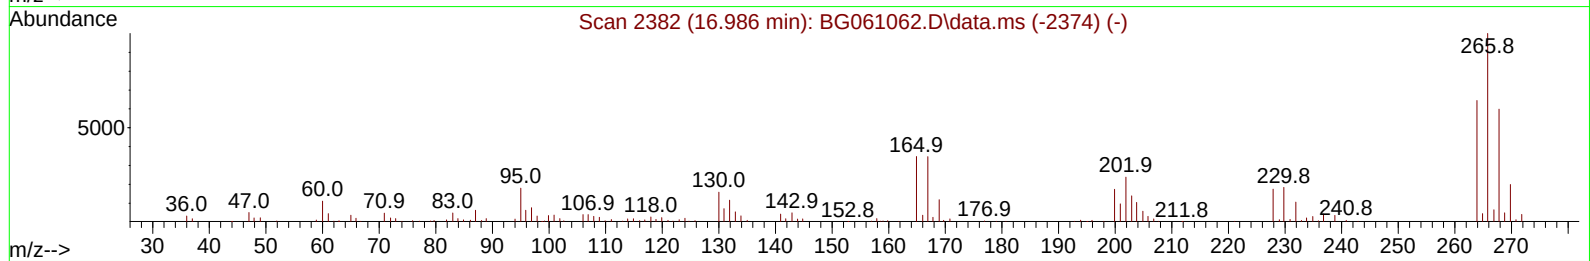
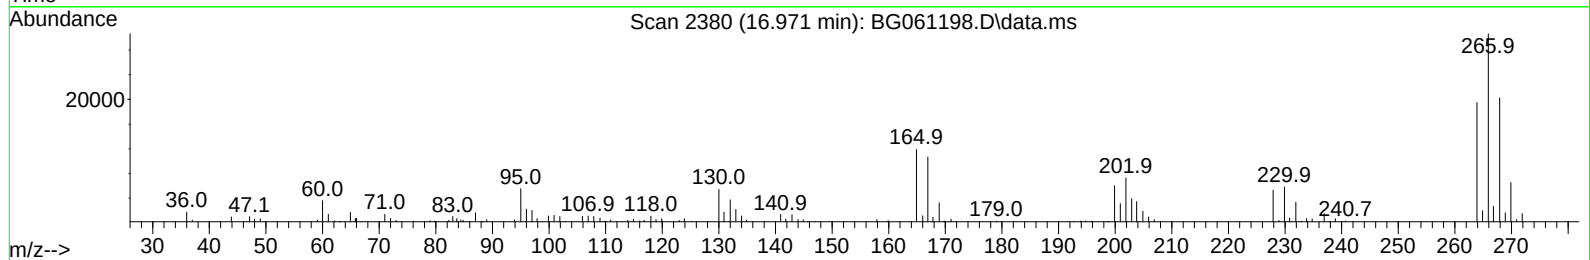


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051524\
Data File : BG061198.D
Acq On : 15 May 2024 9:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 09:54:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

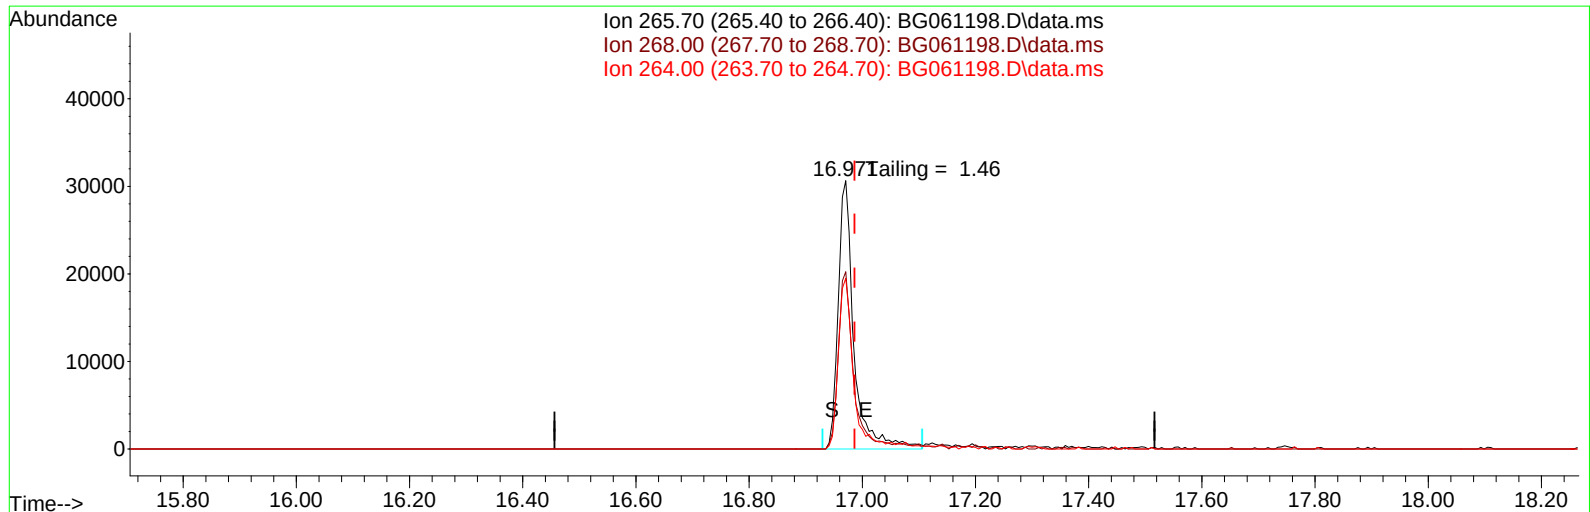

TIC: BG061198.D\data.ms

(70) Pentachlorophenol (C)




16.971min (-0.015) 19428.44 ng

response 59152

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	66.05
264.00	64.40	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051524\
Data File : BG061198.D
Acq On : 15 May 2024 9:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 09:54:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

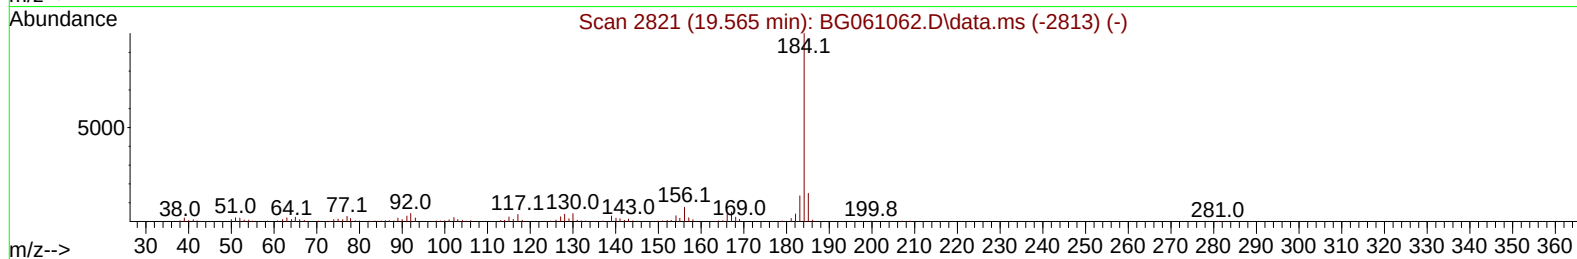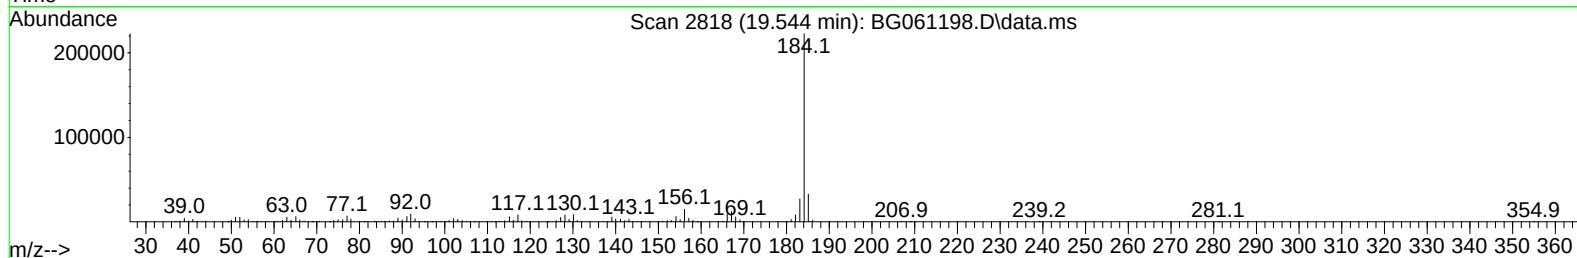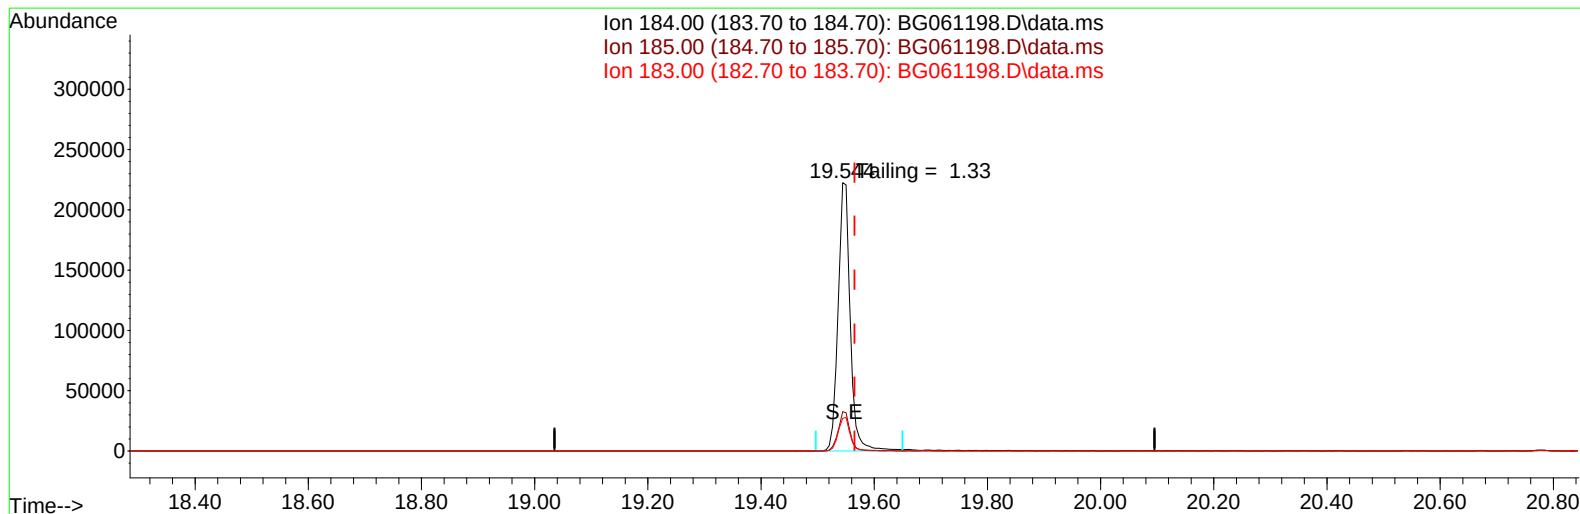

TIC: BG061198.D\data.ms

(77) Benzidine

19.544min (-0.021) 0.00 ng

response 330985

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.69
183.00	13.60	12.18
0.00	0.00	0.00