


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051524\
Data File : BG061198.D
Acq On : 15 May 2024 9:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

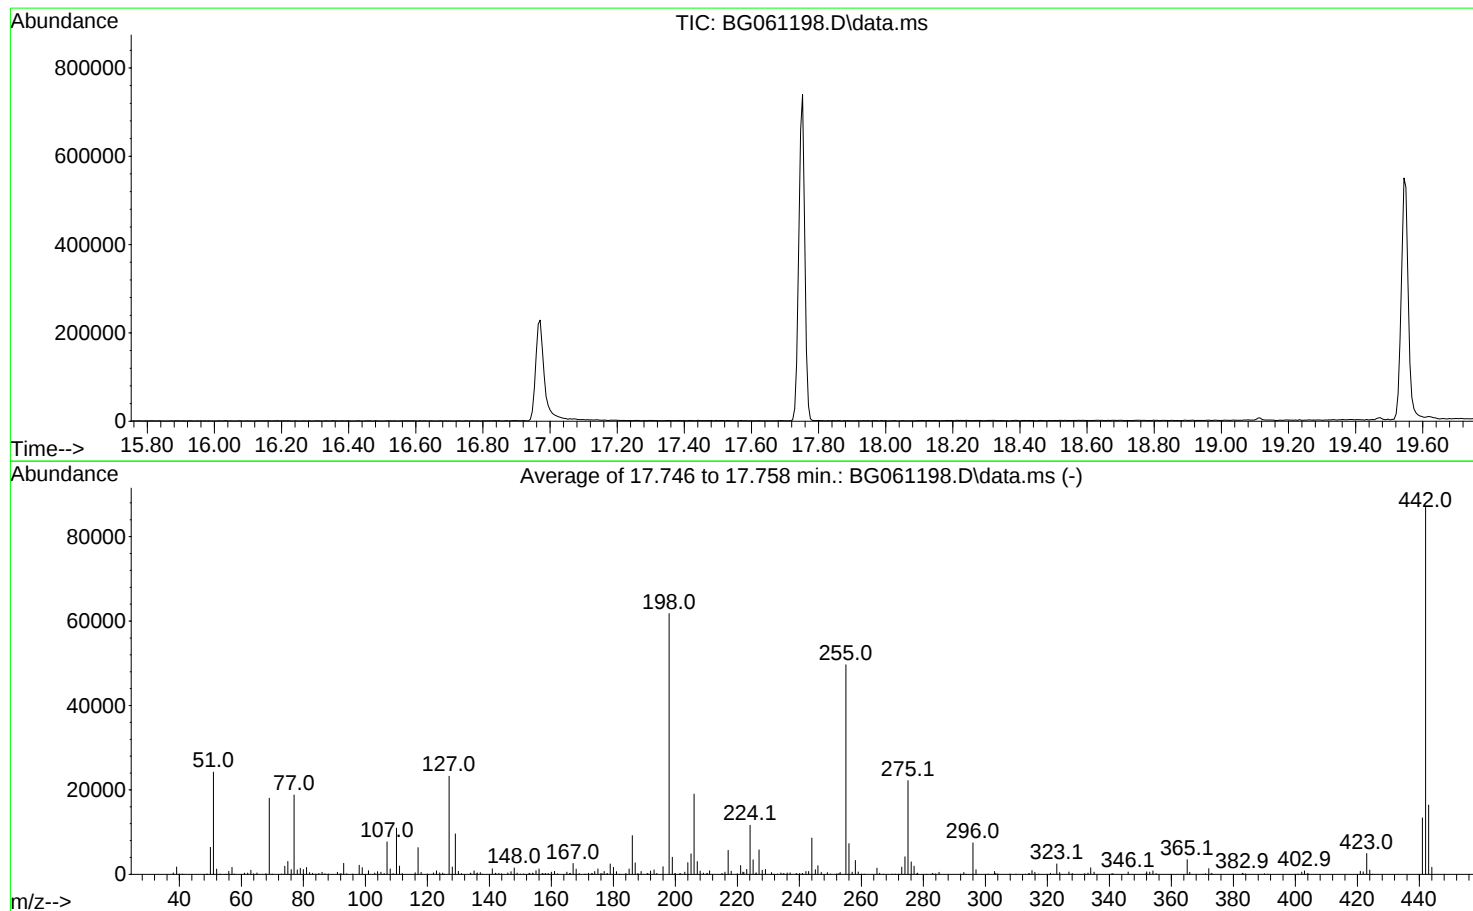

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	24228	PASS
68	69	0.00	2	0.8	140	PASS
69	198	0.00	100	29.2	18043	PASS
70	69	0.00	2	0.3	60	PASS
127	198	10	80	37.6	23221	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61768	PASS
199	198	5	9	6.6	4046	PASS
275	198	10	60	36.0	22221	PASS
365	198	1	100	5.7	3504	PASS
441	198	0.01	100	21.7	13375	PASS
442	442	50	100	100.0	87139	PASS
443	442	15	24	18.8	16424	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/15/2024	BNA_G	<u>BG061198.D</u>
Compound Name	Response	Retention Time
DDT	231011	20.778
DDD	10874	20.343
DDE	1320	19.832
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12194	243205	5.01

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051524\
Data File : BG061198.D
Acq On : 15 May 2024 9:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 15 09:54:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

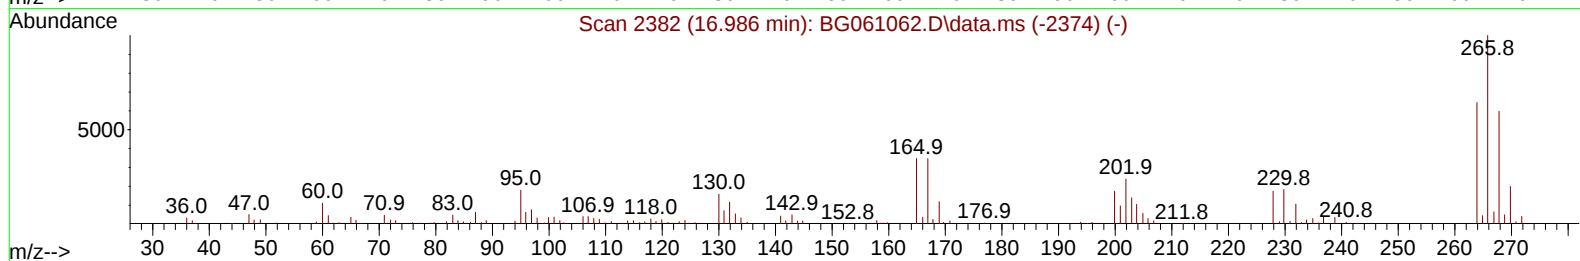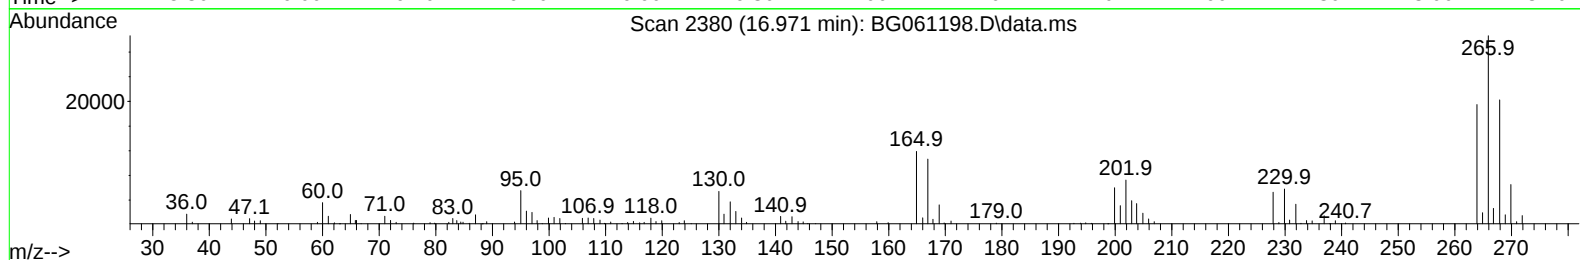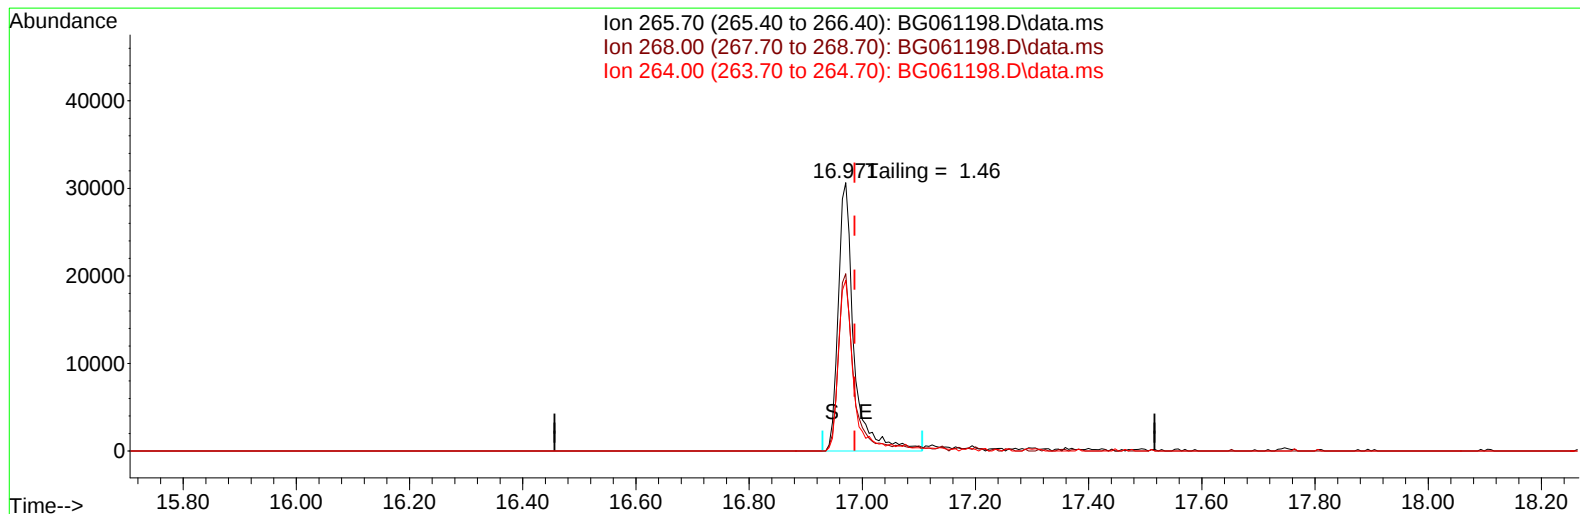

TIC: BG061198.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.015) 19428.44 ng




response 59152

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	66.05
264.00	64.40	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051524\
 Data File : BG061198.D
 Acq On : 15 May 2024 9:18
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: May 15 09:54:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 05:11:25 2024
 Response via : Initial Calibration

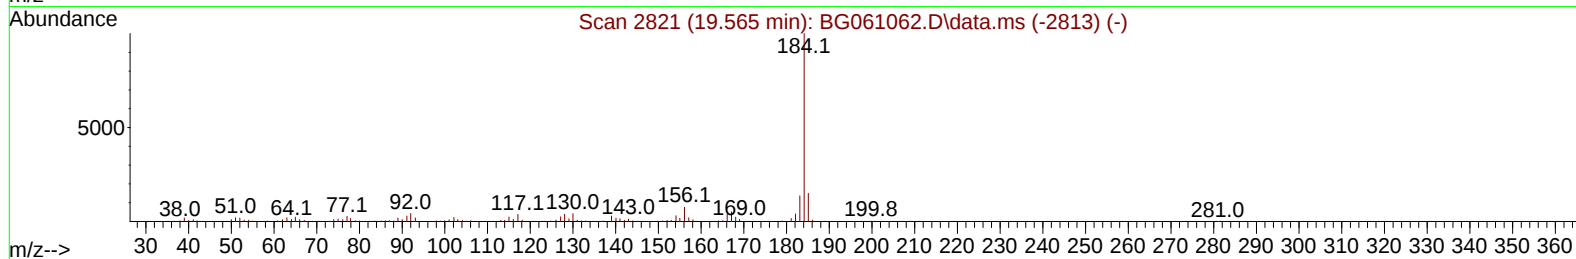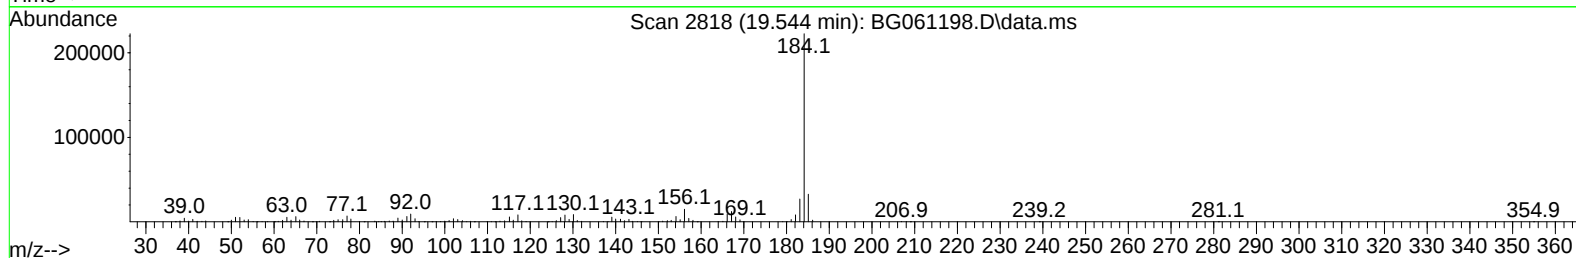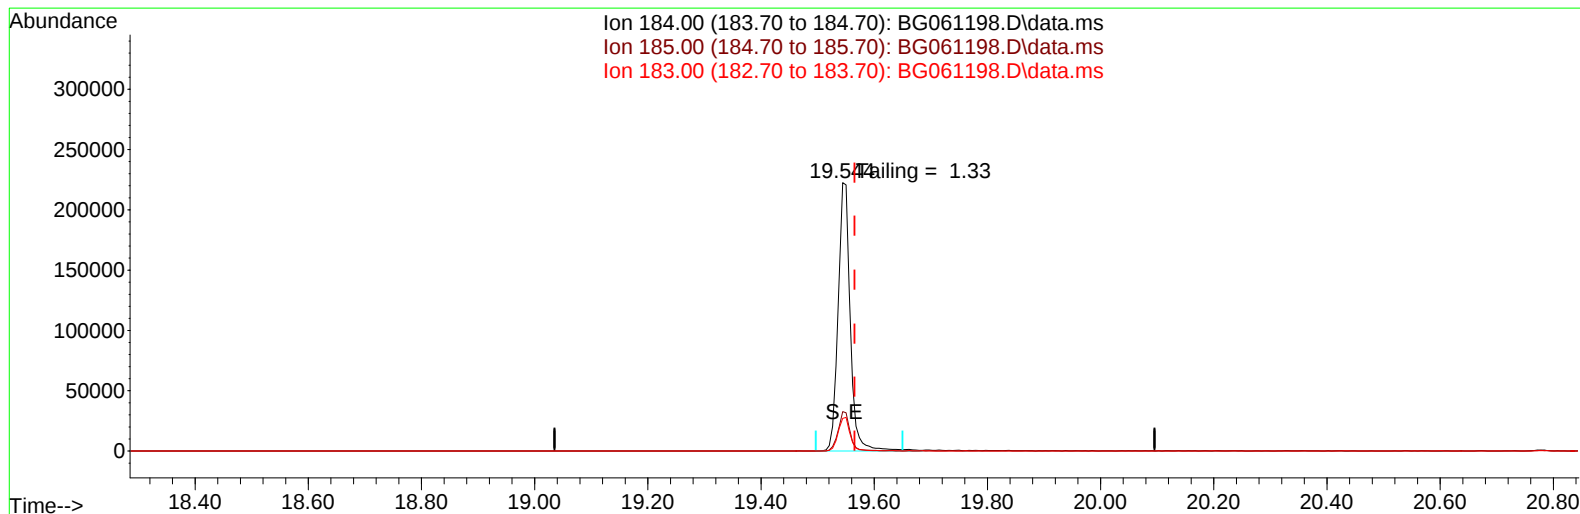

TIC: BG061198.D\data.ms

(77) Benzidine

19.544min (-0.021) 0.00 ng

response 330985

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.69
183.00	13.60	12.18
0.00	0.00	0.00