
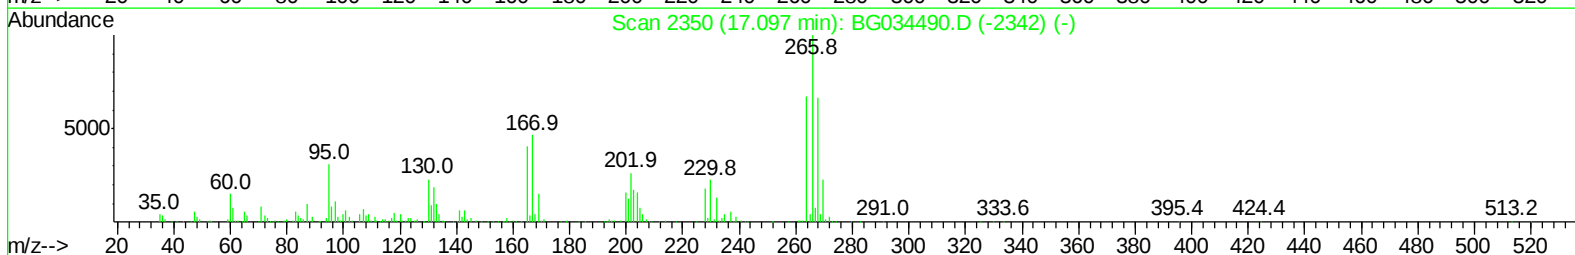
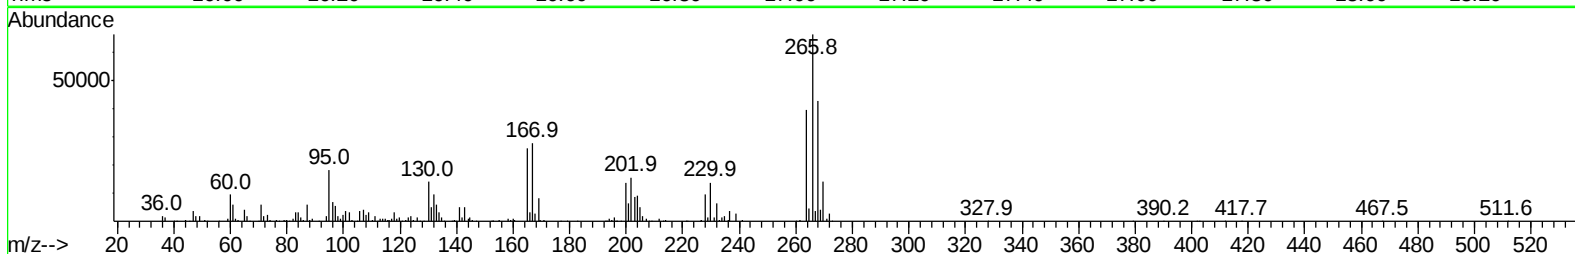


Data Path : Z:\HPCHEM1\BNA G\DATA\BG051618\
Data File : BG034486.D
Acq On : 16 May 2018 13:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 18:54:48 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 16 21:44:43 2018
Response via : Initial Calibration

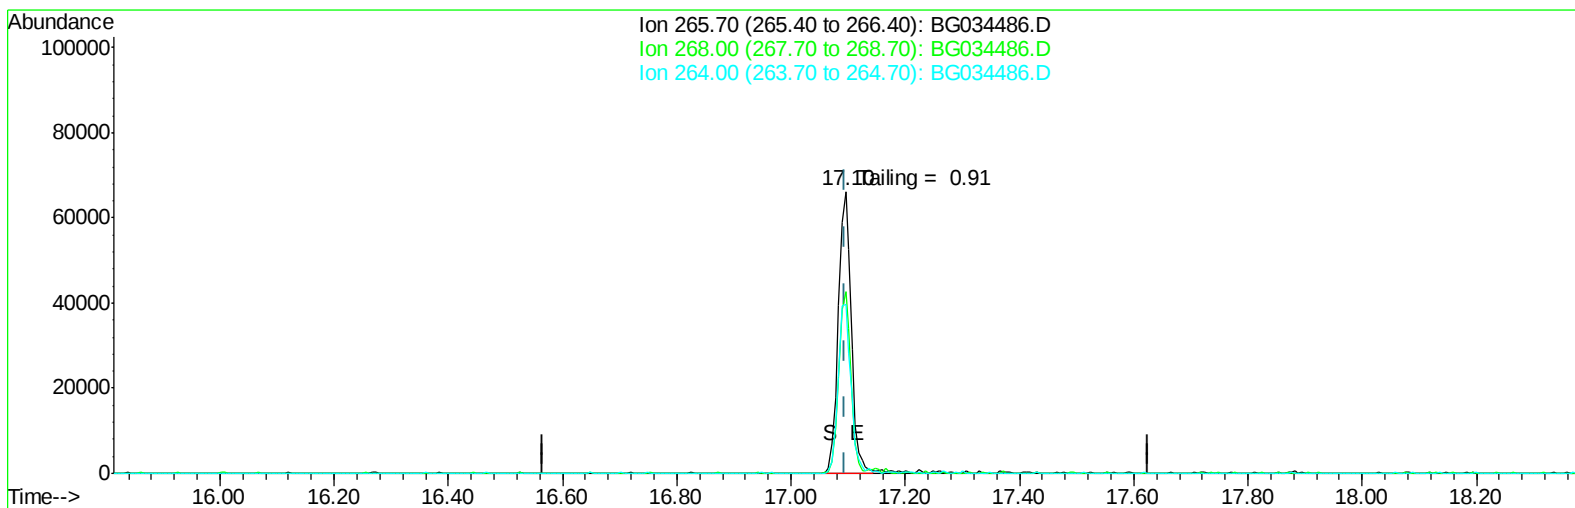

TIC: BG034486.D

(69) Pentachlorophenol (C)




17.095min (-0.001) 134835.49ng

response 104062

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.52
264.00	62.00	59.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051618\
Data File : BG034486.D
Acq On : 16 May 2018 13:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 18:54:48 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 16 21:44:43 2018
Response via : Initial Calibration

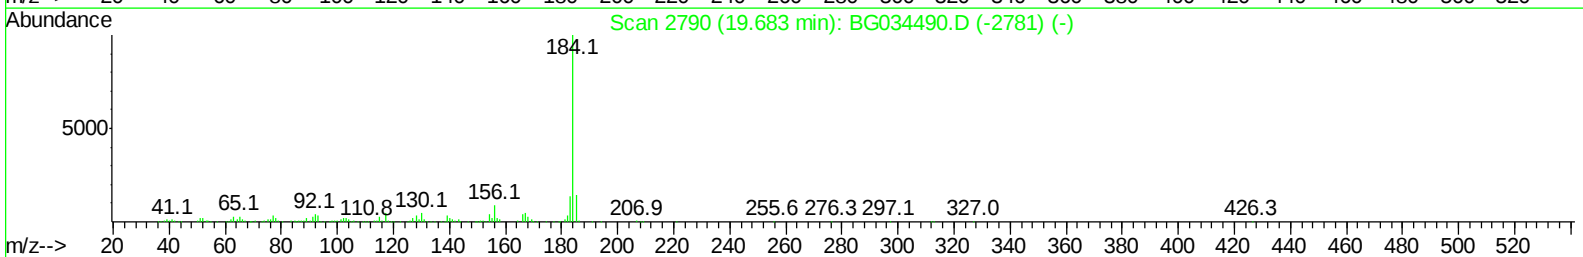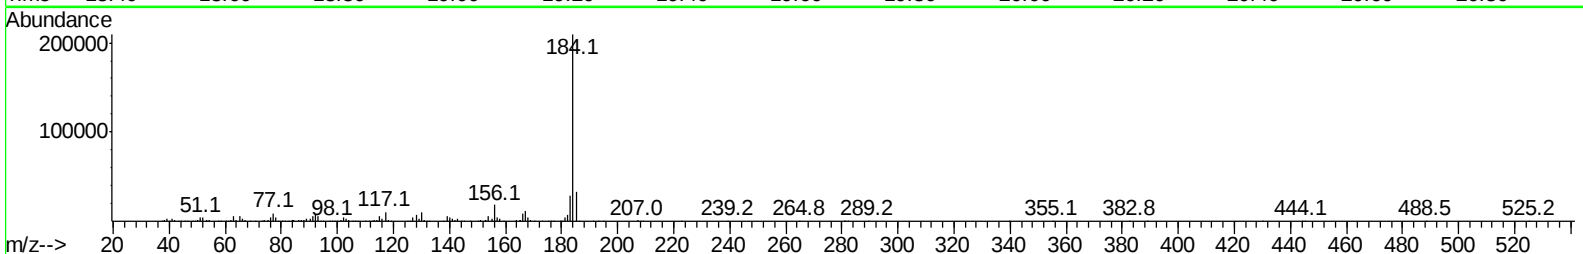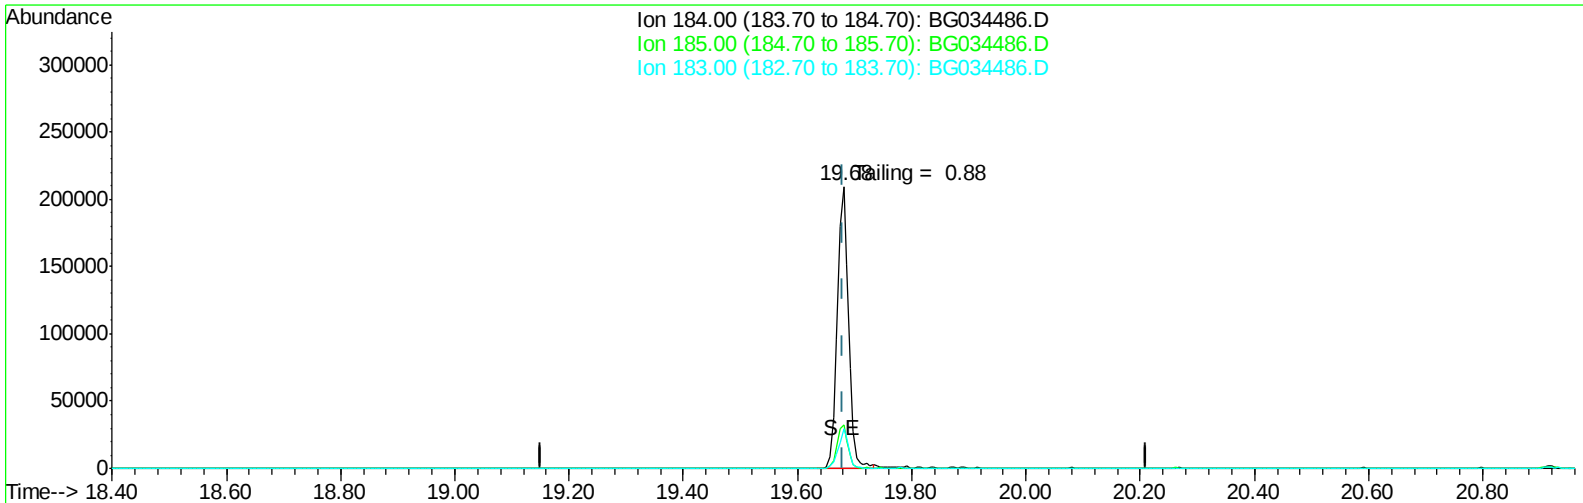

TIC: BG034486.D

(76) Benzidine

19.710min (+0.029) 2389.94ng m

response 4528

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.05
183.00	13.30	15.77
0.00	0.00	0.00