


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051618\
 Data File : BG034486.D
 Acq On : 16 May 2018 13:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 05 15:48:31 2018

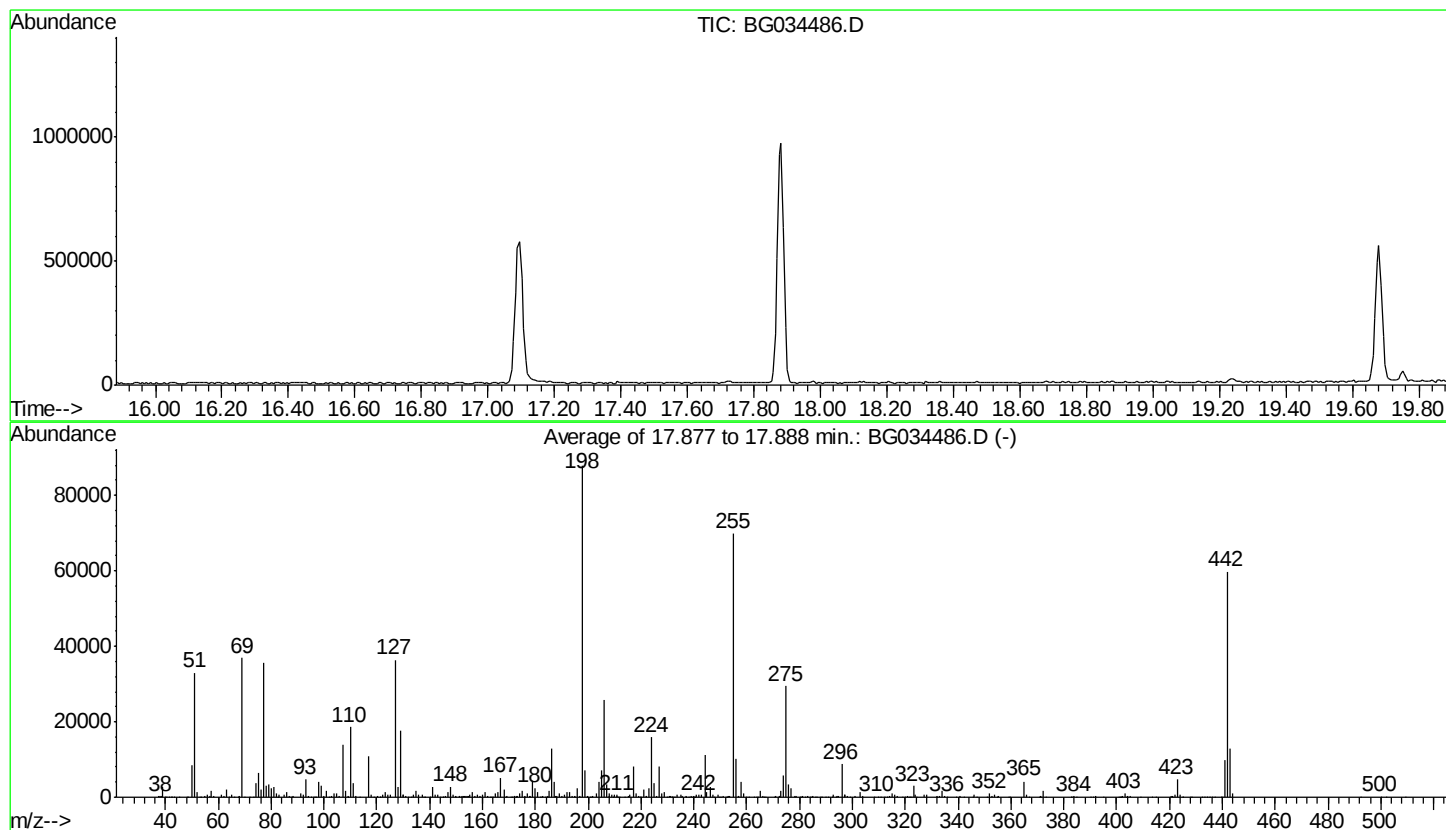

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	33056	PASS
68	69	0.00	2	1.0	355	PASS
69	198	0.00	100	42.0	36920	PASS
70	69	0.00	2	0.4	164	PASS
127	198	10	80	41.4	36408	PASS
197	198	0.00	2	0.5	427	PASS
198	198	100	100	100.0	87893	PASS
199	198	5	9	8.0	6996	PASS
275	198	10	60	33.5	29477	PASS
365	198	1	100	4.8	4230	PASS
441	198	0.01	100	11.1	9728	PASS
442	198	50	100	68.1	59898	PASS
443	442	15	24	21.5	12876	PASS