
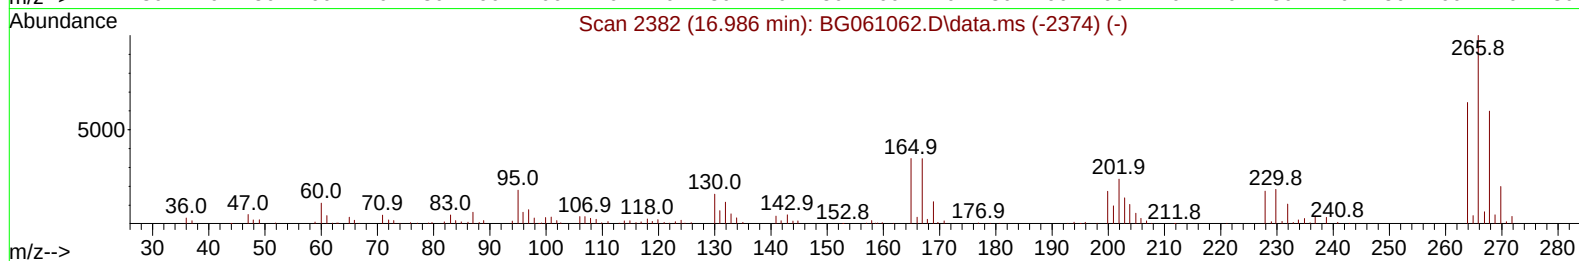
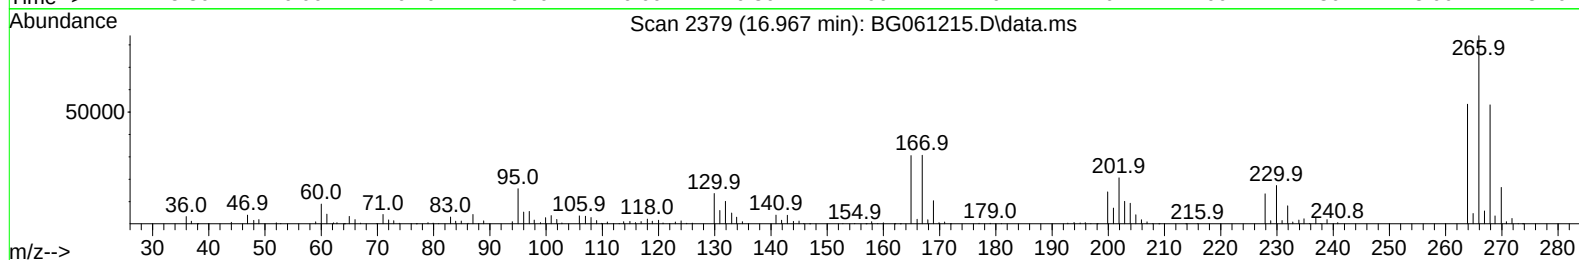


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051624\
Data File : BG061215.D
Acq On : 16 May 2024 10:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 10:43:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

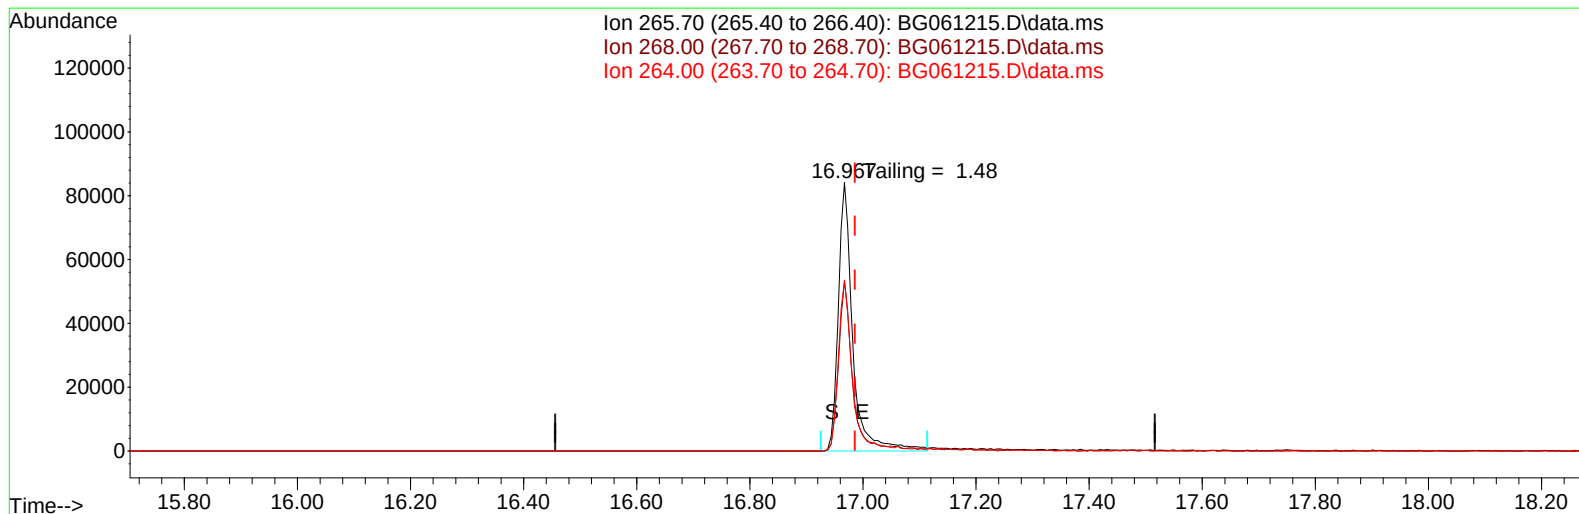

TIC: BG061215.D\data.ms

(70) Pentachlorophenol (C)




16.967min (-0.019) 32196.12 ng

response 149647

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	63.26
264.00	64.40	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051624\
Data File : BG061215.D
Acq On : 16 May 2024 10:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 10:43:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

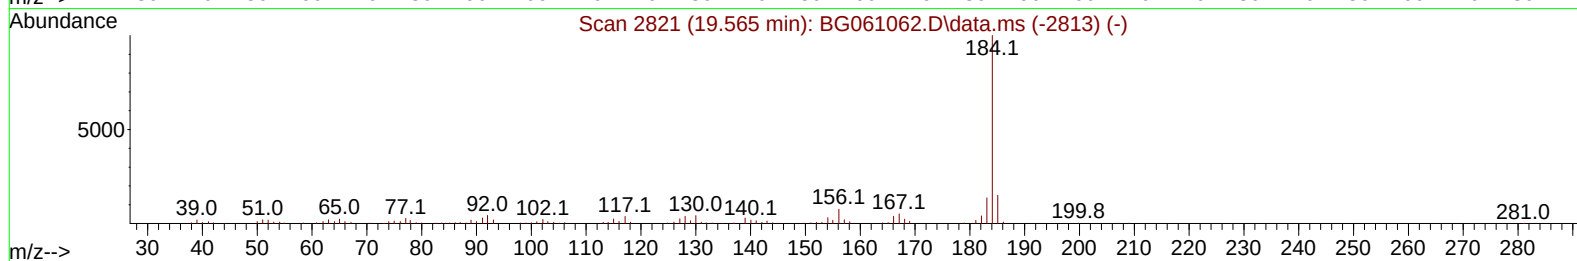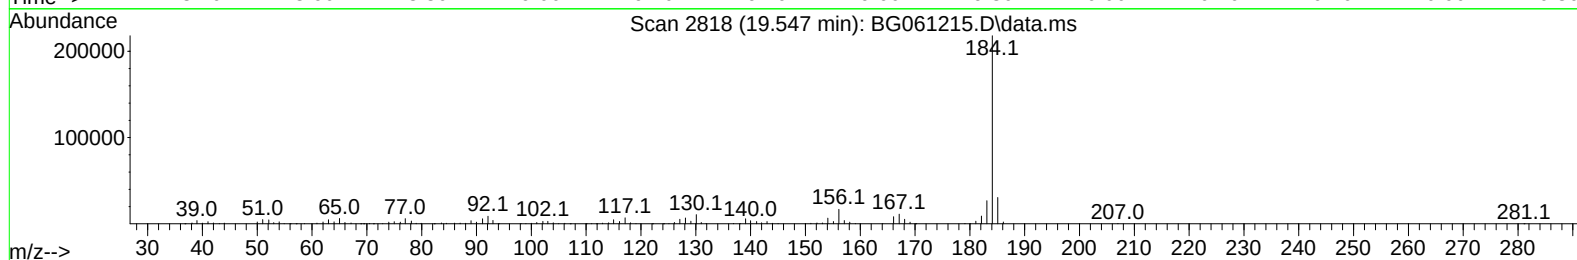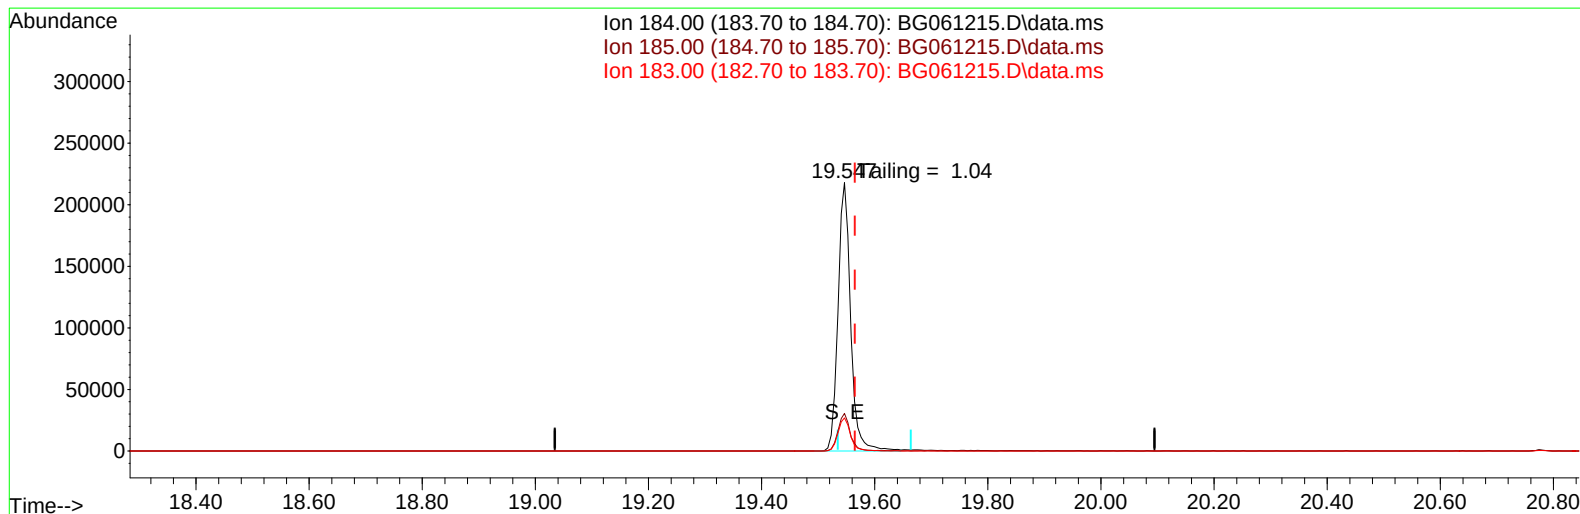

TIC: BG061215.D\data.ms

(77) Benzidine

19.547min (-0.018) 202853.03 ng

response 270519

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.02
183.00	13.60	12.33
0.00	0.00	0.00