

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051624\
Data File : BG061217.D
Acq On : 16 May 2024 12:15
Operator : MA/JU
Sample : PB160933BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160933BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG061217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.523	425	431	442	rBV	444274	687798	28.47%	8.193%
2	7.110	693	701	718	rBV	436999	747254	30.94%	8.901%
3	7.926	835	840	847	rVB	73846	124303	5.15%	1.481%
4	9.084	1029	1037	1047	rBV	266982	483554	20.02%	5.760%
5	10.723	1309	1316	1323	rBV	94260	164453	6.81%	1.959%
6	13.179	1727	1734	1746	rBV	747086	1126887	46.65%	13.424%
7	14.560	1962	1969	1979	rBV	159931	253807	10.51%	3.023%
8	16.052	2216	2223	2243	rBV	657313	1097921	45.45%	13.079%
9	17.309	2430	2437	2448	rBV	238450	370977	15.36%	4.419%
10	19.930	2876	2883	2891	rBV	1788385	2415476	100.00%	28.774%
11	21.569	3155	3162	3173	rBV	271347	459986	19.04%	5.479%
12	24.695	3684	3694	3707	rBV	147789	462376	19.14%	5.508%




Sum of corrected areas: 8394792

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051624\
Data File : BG061217.D
Acq On : 16 May 2024 12:15
Operator : MA/JU
Sample : PB160933BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160933BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

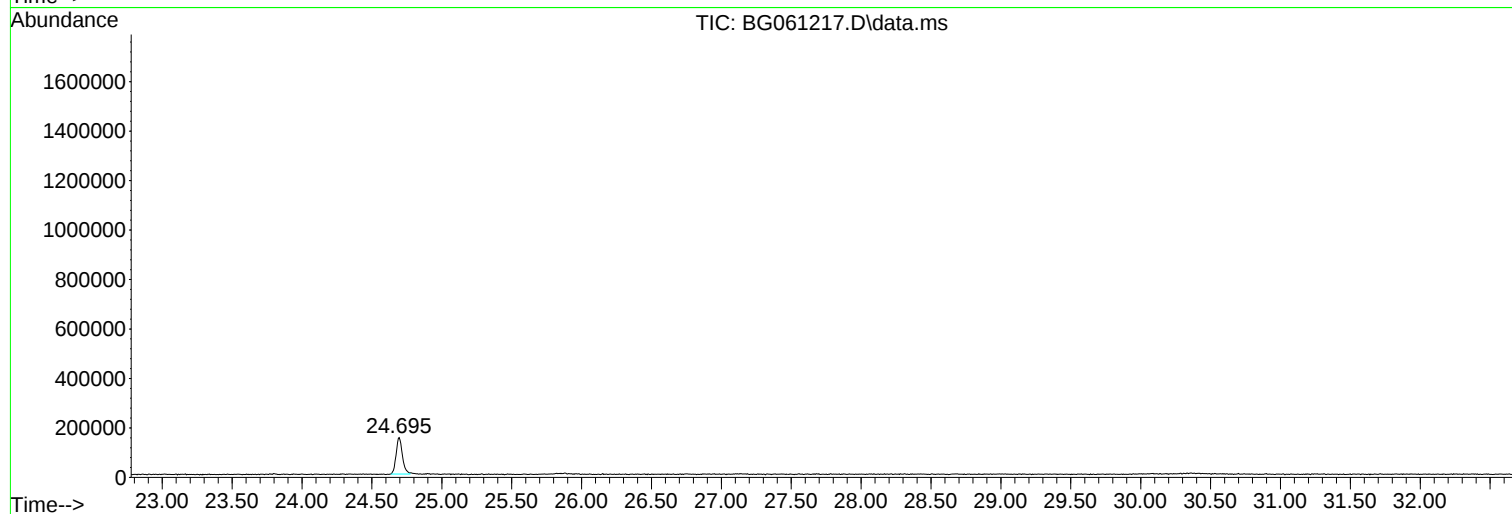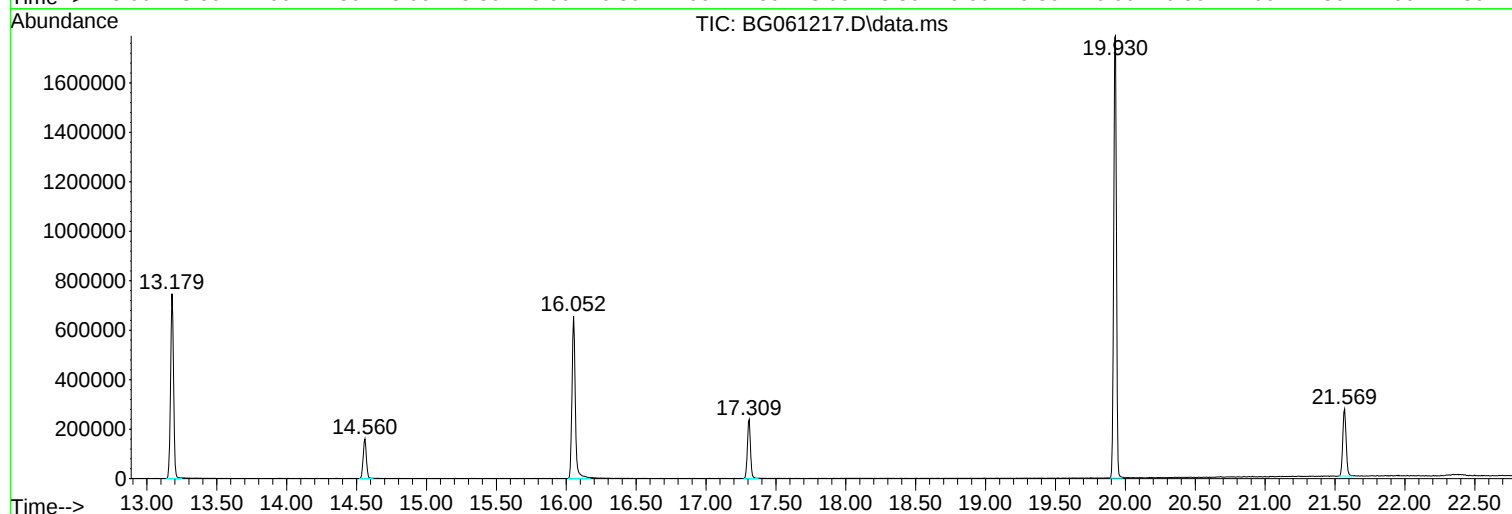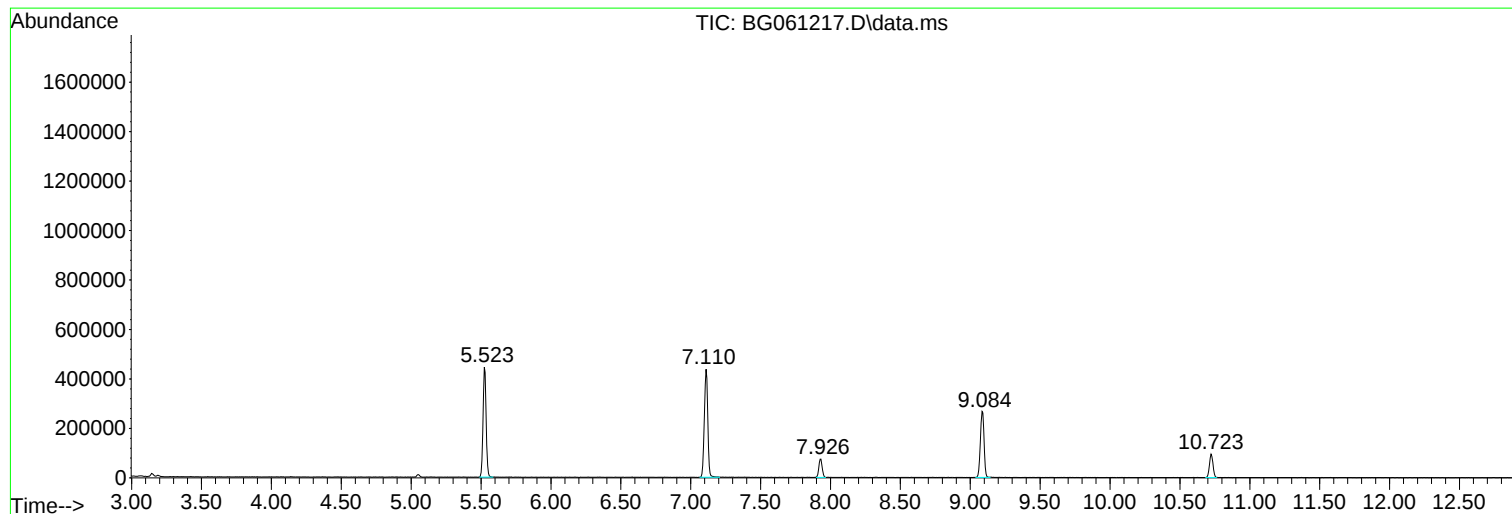

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051624\
Data File : BG061217.D
Acq On : 16 May 2024 12:15
Operator : MA/JU
Sample : PB160933BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160933BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051624\
Data File : BG061217.D
Acq On : 16 May 2024 12:15
Operator : MA/JU
Sample : PB160933BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160933BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------