
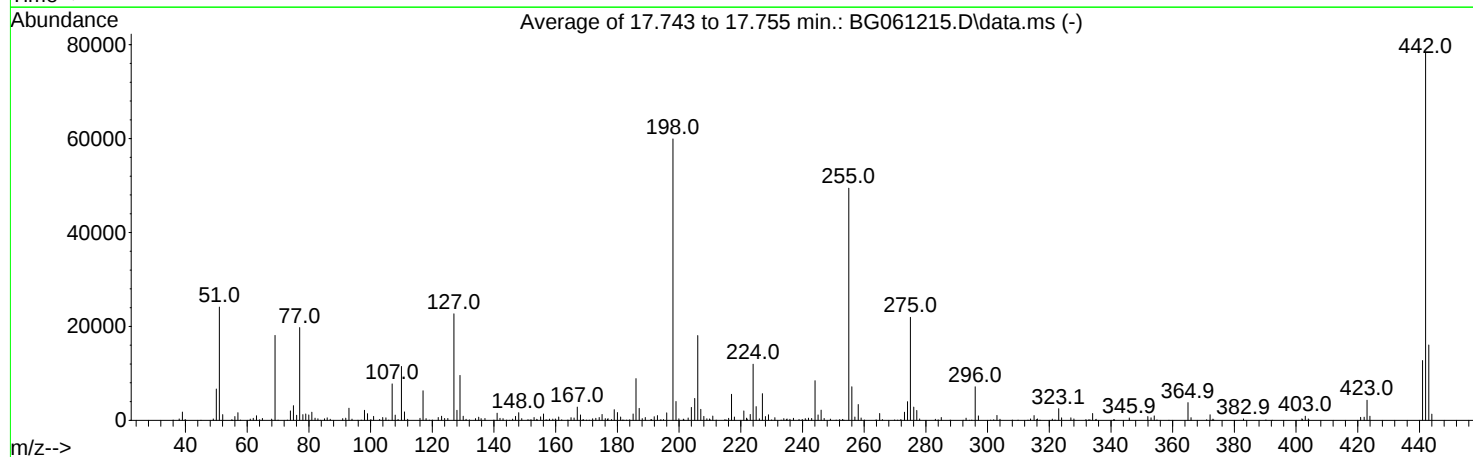


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051624\
Data File : BG061215.D
Acq On : 16 May 2024 10:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

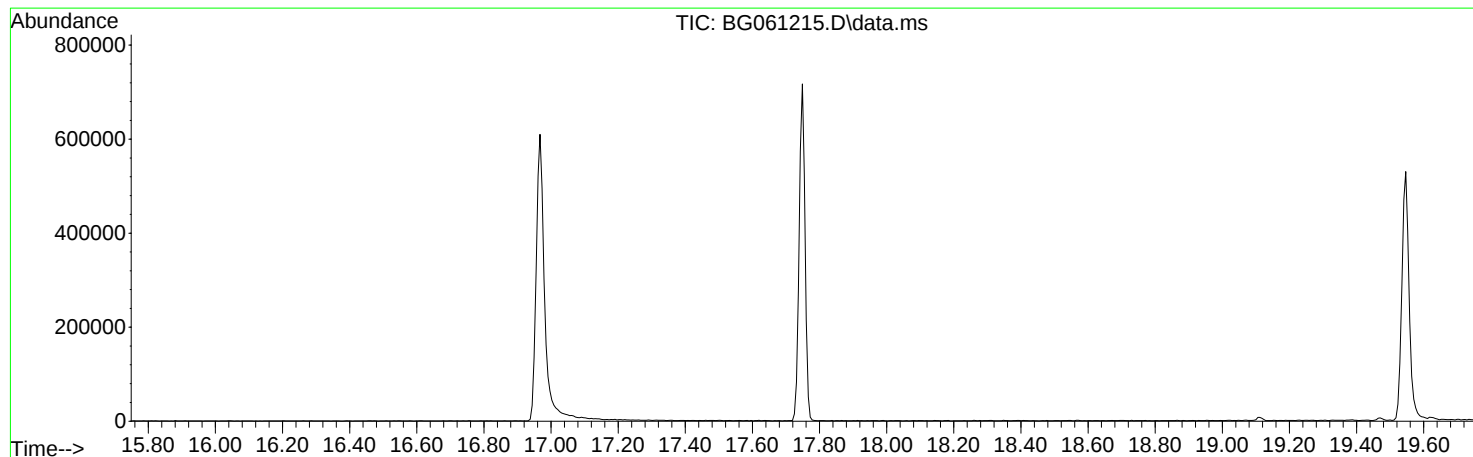

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	24115	PASS
68	69	0.00	2	1.6	289	PASS
69	198	0.00	100	30.2	18081	PASS
70	69	0.00	2	0.4	65	PASS
127	198	10	80	37.9	22685	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59928	PASS
199	198	5	9	6.7	4029	PASS
275	198	10	60	36.6	21957	PASS
365	198	1	100	6.3	3772	PASS
441	198	0.01	100	21.2	12733	PASS
442	442	50	100	100.0	78328	PASS
443	442	15	24	20.5	16040	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/16/2024	BNA_G	<u>BG061215.D</u>
Compound Name	Response	Retention Time
DDT	223282	20.78
DDD	7363	20.34
DDE	816	19.834
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8179	231461	3.53

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051624\
Data File : BG061215.D
Acq On : 16 May 2024 10:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 16 10:43:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

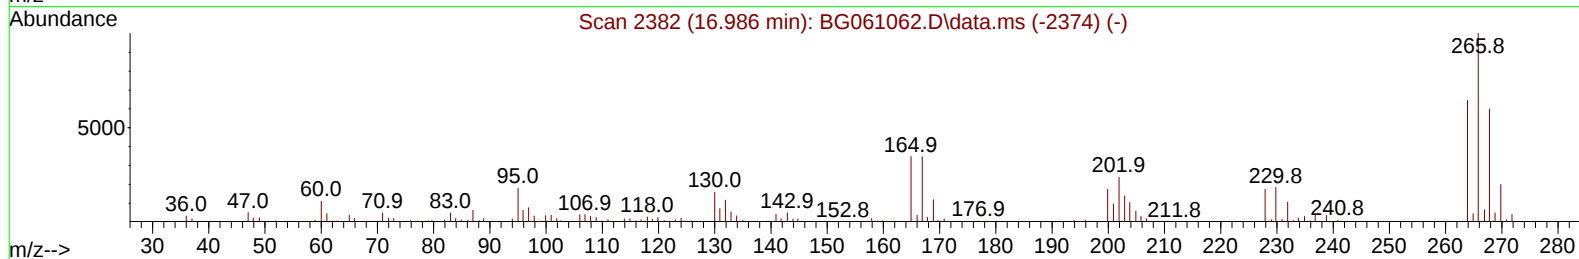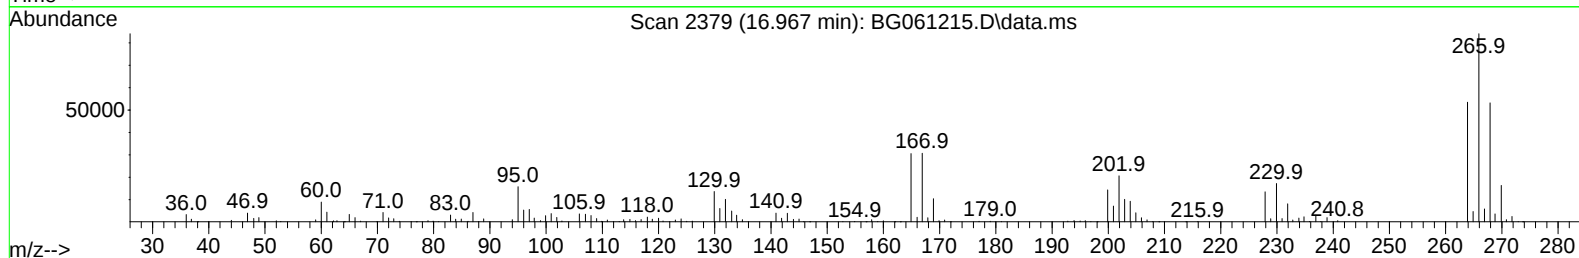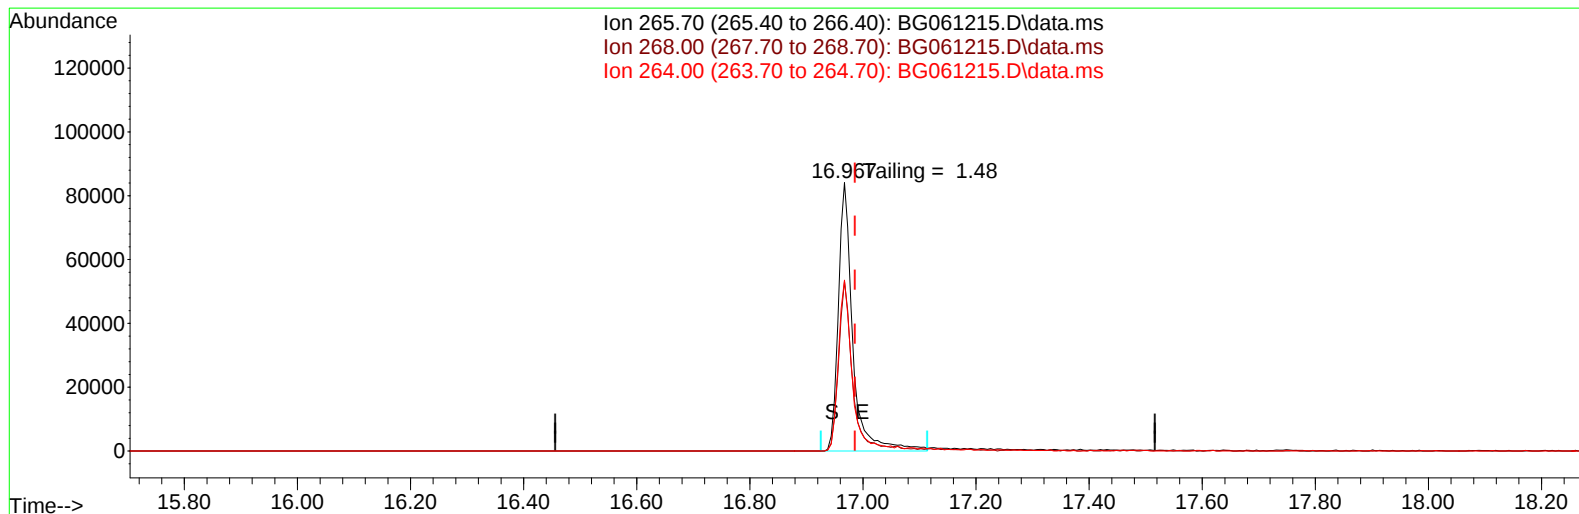

TIC: BG061215.D\data.ms

(70) Pentachlorophenol (C)

16.967min (-0.019) 32196.12 ng




response 149647

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	63.26
264.00	64.40	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051624\
Data File : BG061215.D
Acq On : 16 May 2024 10:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 16 10:43:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

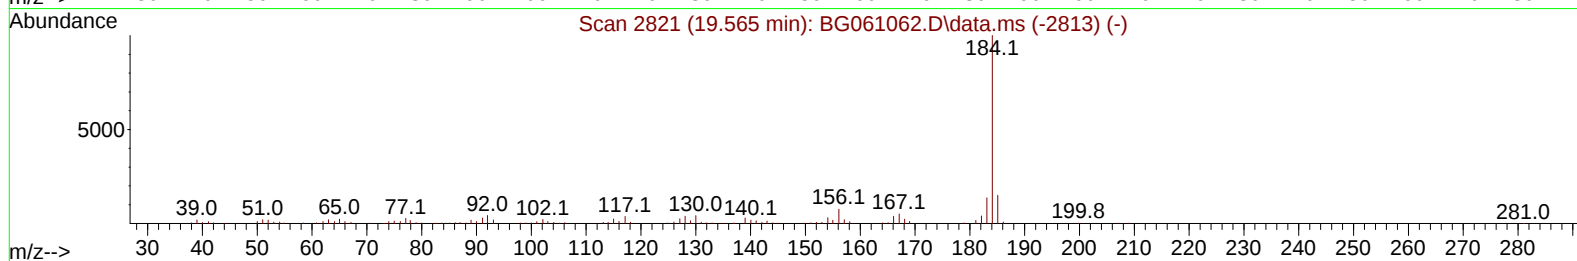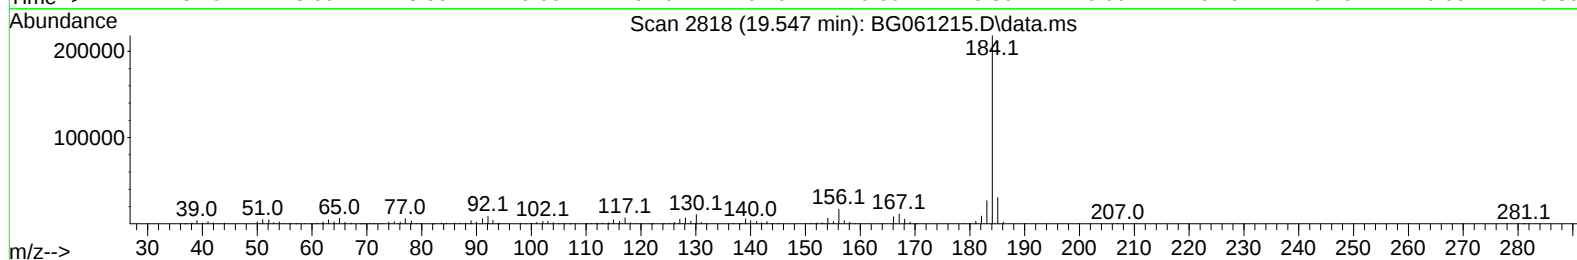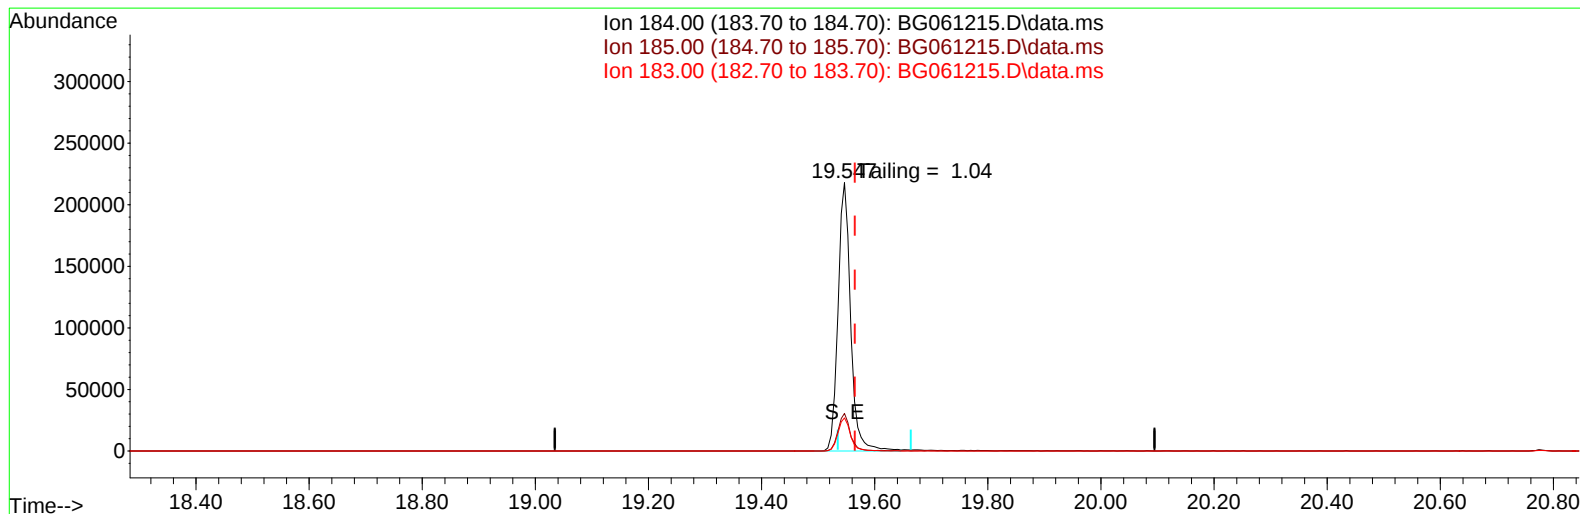

TIC: BG061215.D\data.ms

(77) Benzidine

19.547min (-0.018) 202853.03 ng

response 270519

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.02
183.00	13.60	12.33
0.00	0.00	0.00