
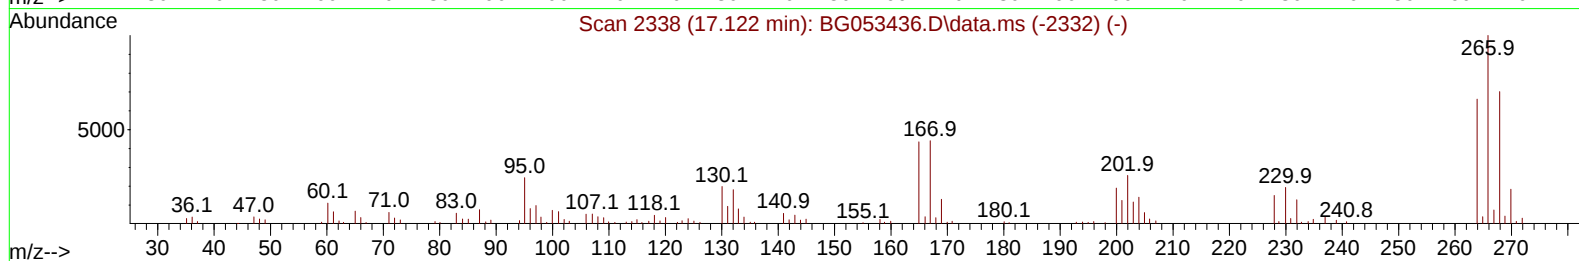
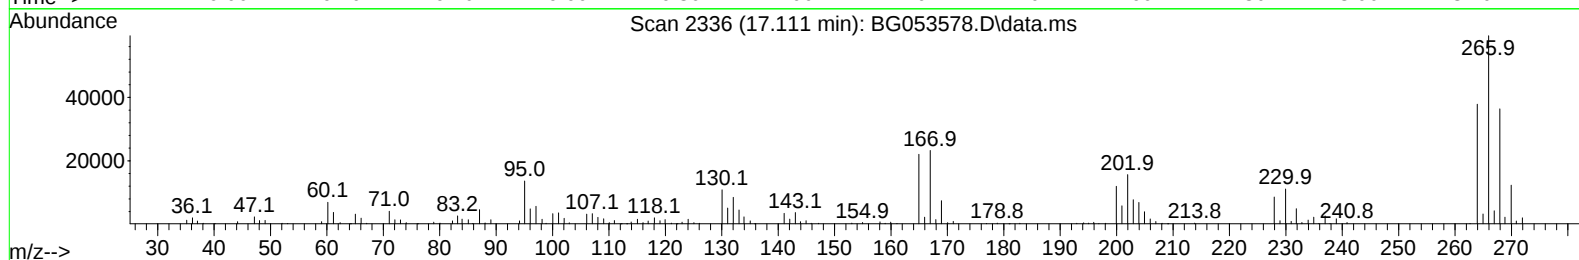


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
Data File : BG053578.D
Acq On : 17 May 2022 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 04:46:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

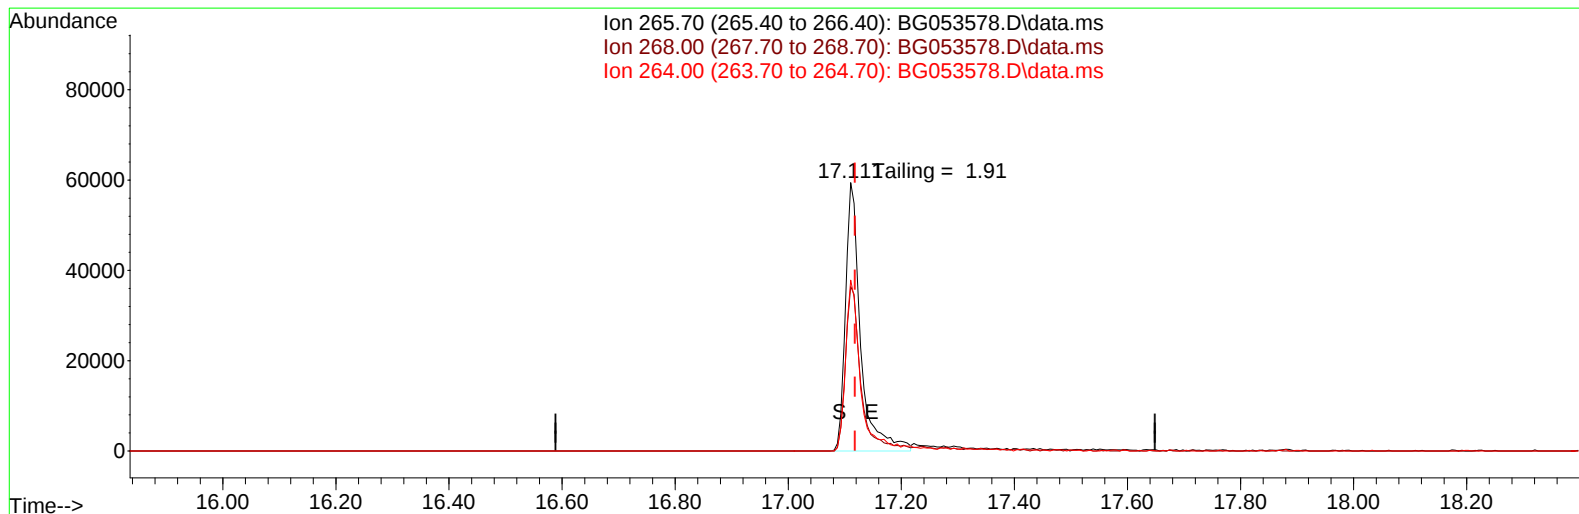

TIC: BG053578.D\data.ms

(70) Pentachlorophenol (C)




17.111min (-0.008) 28260.74 ng

response 108694

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.25
264.00	66.20	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
Data File : BG053578.D
Acq On : 17 May 2022 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 04:46:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

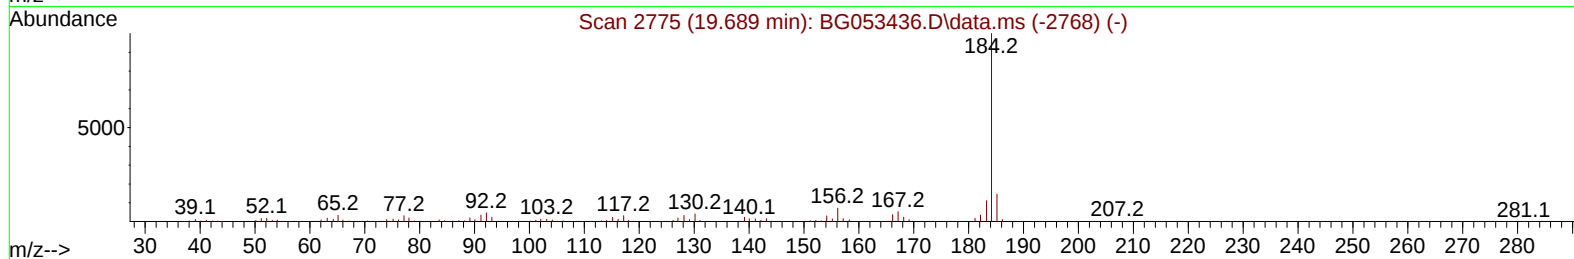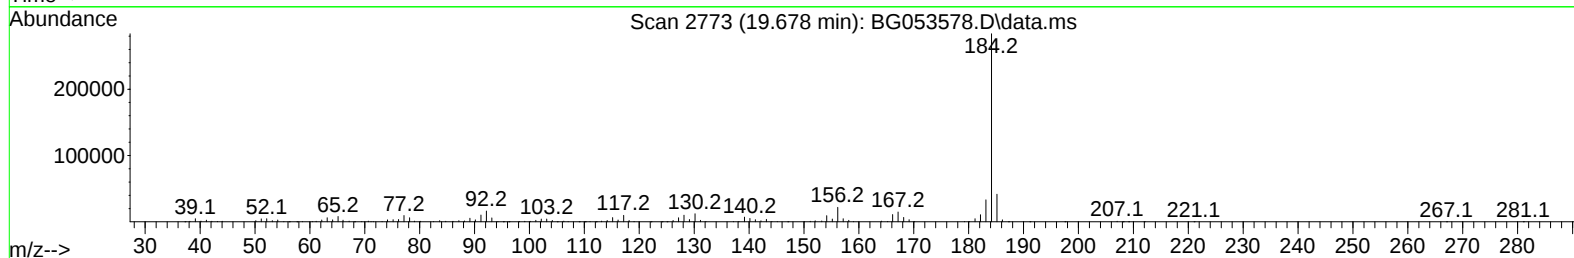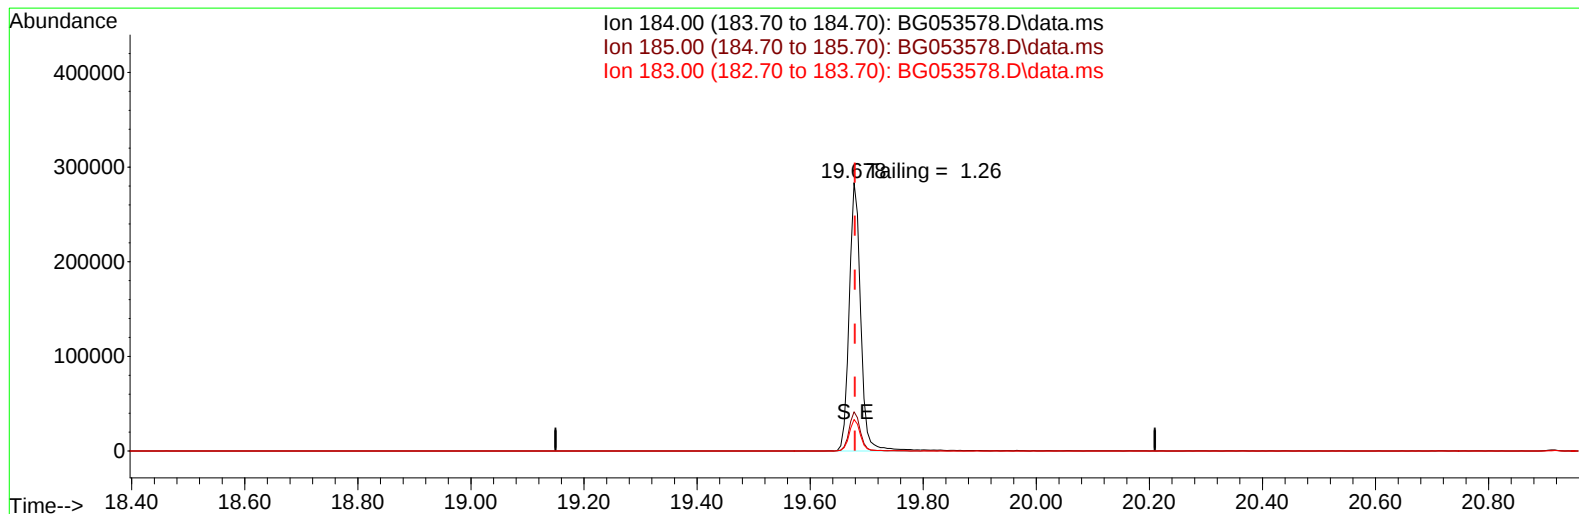

TIC: BG053578.D\data.ms

(77) Benzidine**19.678min (-0.002) 118293.91 ng****response 402848**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.64
183.00	11.10	11.75
0.00	0.00	0.00