

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
 Data File : BG053590.D
 Acq On : 17 May 2022 19:05
 Operator : CG/JU
 Sample : N2863-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P003-SS003-1824-01

Quant Time: May 18 03:14:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 11 06:00:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.082	152	25023	20.000	ng	0.00
21) Naphthalene-d8	10.890	136	107838	20.000	ng	0.00
39) Acenaphthene-d10	14.708	164	93551	20.000	ng	0.00
64) Phenanthrene-d10	17.452	188	249600	20.000	ng	0.00
76) Chrysene-d12	21.734	240	215295	20.000	ng	0.00
86) Perylene-d12	25.012	264	193952	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.650	112	159803	108.383	ng	0.00
7) Phenol-d6	7.242	99	245676	109.791	ng	0.00
23) Nitrobenzene-d5	9.245	82	174182	68.757	ng	0.00
42) 2,4,6-Tribromophenol	16.195	330	143800	104.220	ng	0.00
45) 2-Fluorobiphenyl	13.328	172	398123	62.187	ng	0.00
79) Terphenyl-d14	20.054	244	846216	73.204	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
Data File : BG053590.D
Acq On : 17 May 2022 19:05
Operator : CG/JU
Sample : N2863-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P003-SS003-1824-01

Quant Time: May 18 03:14:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration




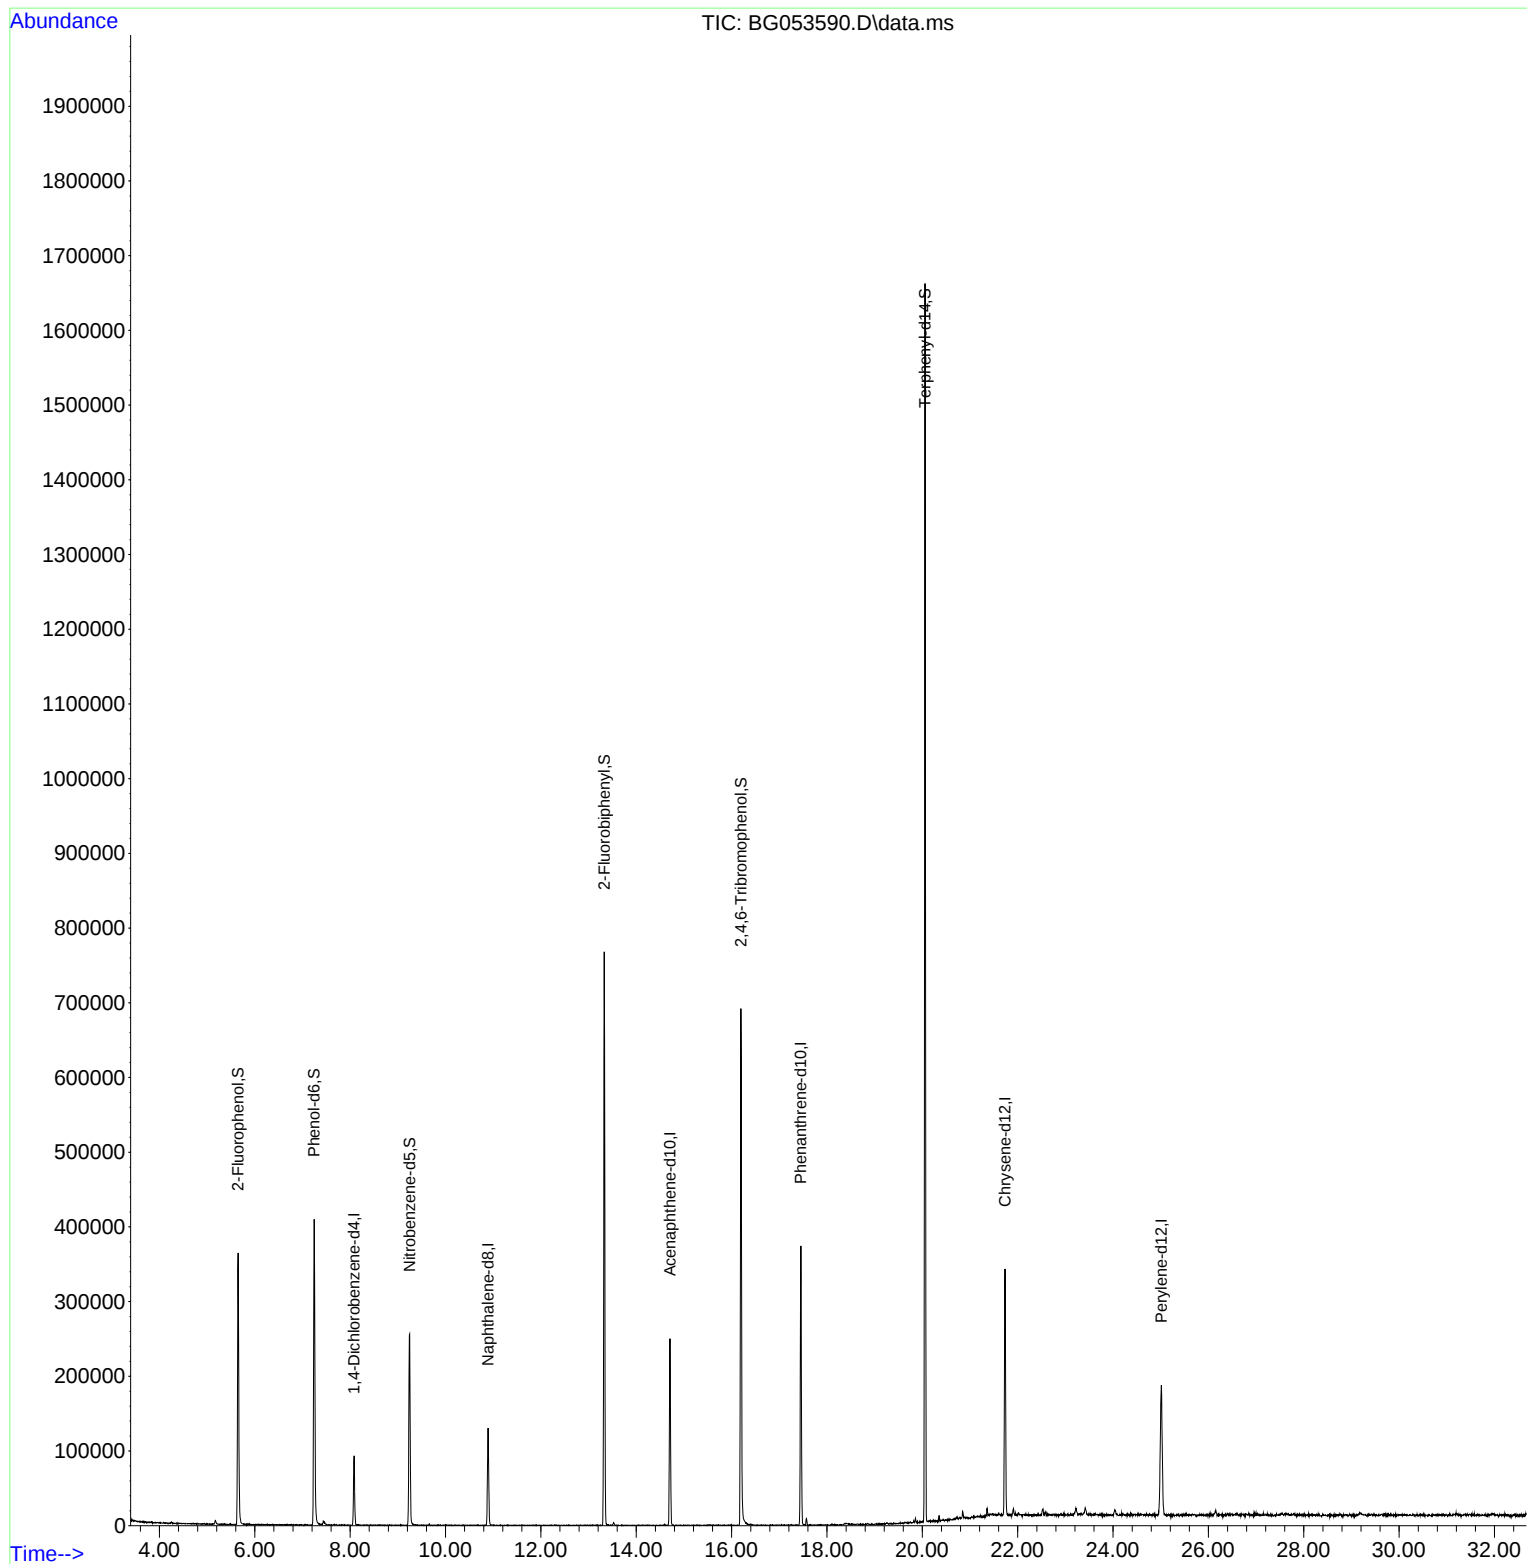




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.082 min Scan# 79
Delta R.T. -0.007 min
Lab File: BG053590.D
Acq: 17 May 2022 19:05




Instrument :
BNA_G
ClientSampleId :
P003-SS003-1824-01


Tgt Ion:152 Resp: 25023
Ion Ratio Lower Upper
152 100
150 147.0 131.6 197.4
115 59.7 50.9 76.3

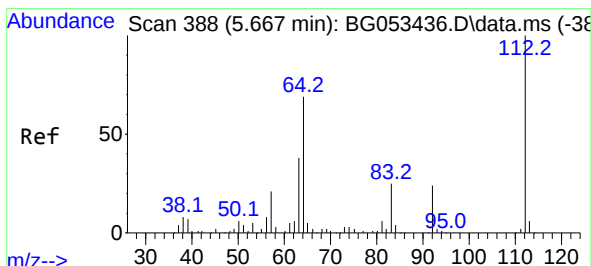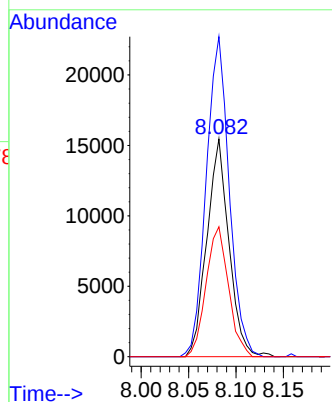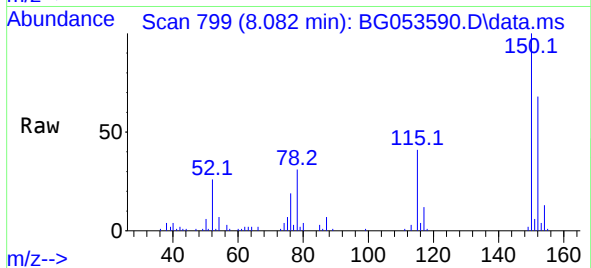

#5
2-Fluorophenol
Concen: 108.383 ng
RT: 5.650 min Scan# 385
Delta R.T. -0.002 min
Lab File: BG053590.D
Acq: 17 May 2022 19:05

Tgt Ion:112 Resp: 159803
Ion Ratio Lower Upper
112 100
64 69.5 55.1 82.7
63 40.5 30.4 45.6


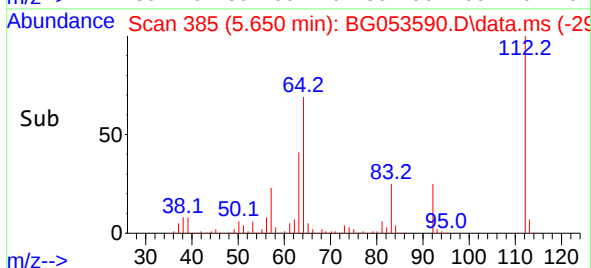
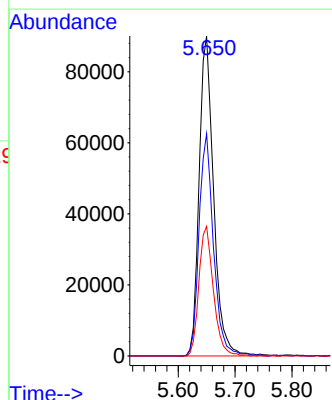



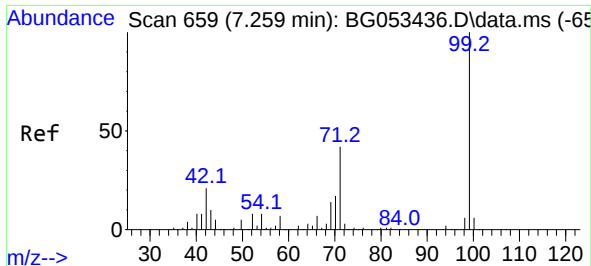

#7
Phenol-d6
Concen: 109.791 ng
RT: 7.242 min Scan# 61
Delta R.T. -0.007 min
Lab File: BG053590.D
Acq: 17 May 2022 19:05




Instrument :
BNA_G
ClientSampleId :
P003-SS003-1824-01

Tgt Ion: 99 Resp: 245676
Ion Ratio Lower Upper
99 100
42 22.5 17.0 25.6
71 43.3 33.8 50.8

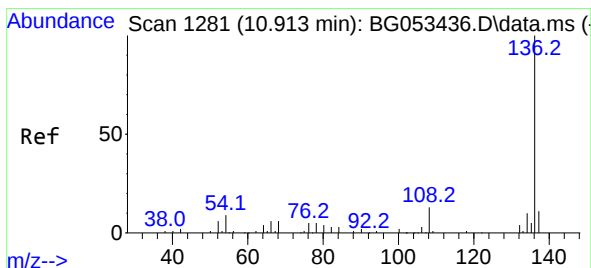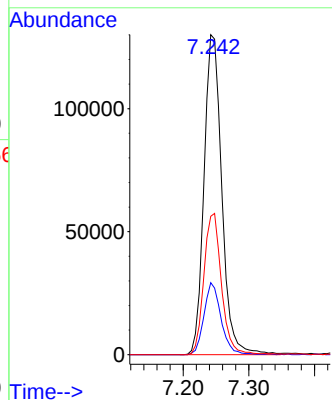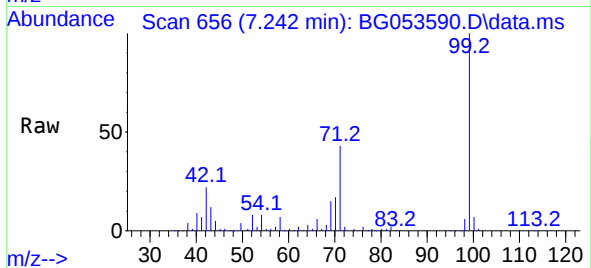

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.890 min Scan# 1277
Delta R.T. -0.007 min
Lab File: BG053590.D
Acq: 17 May 2022 19:05

Tgt Ion:136 Resp: 107838
Ion Ratio Lower Upper
136 100
137 11.6 8.5 12.7
54 9.4 7.4 11.2
68 6.7 4.9 7.3


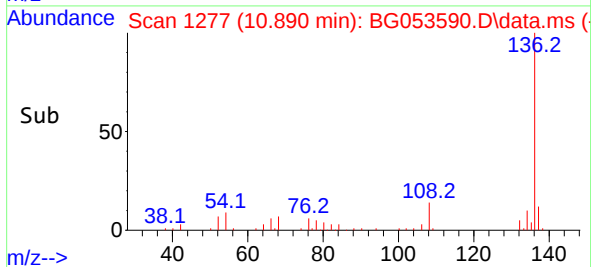
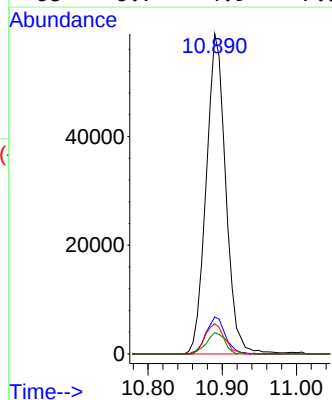
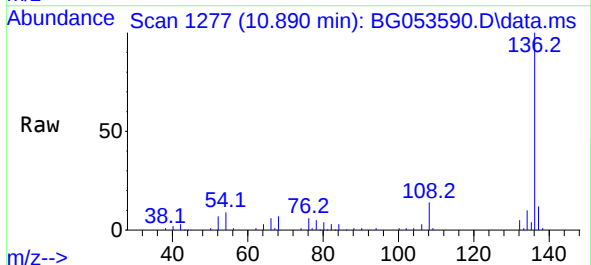




#23
Nitrobenzene-d5
Concen: 68.757 ng
RT: 9.245 min Scan# 91
Delta R.T. -0.007 min
Lab File: BG053590.D
Acq: 17 May 2022 19:05




Instrument :
BNA_G
ClientSampleId :
P003-SS003-1824-01

Tgt Ion: 82 Resp: 174182
Ion Ratio Lower Upper
82 100
128 35.3 27.9 41.9
54 51.3 41.2 61.8

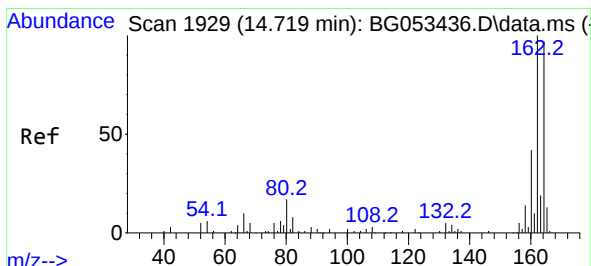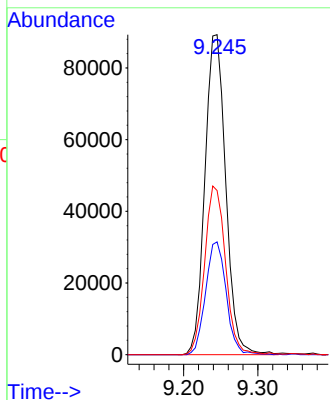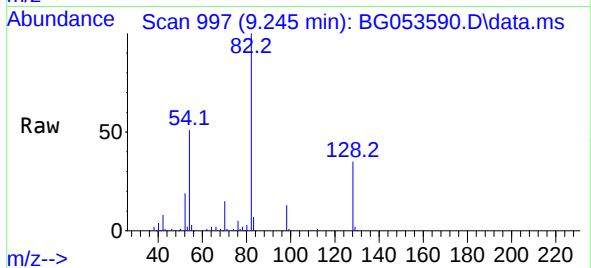

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.708 min Scan# 1927
Delta R.T. -0.007 min
Lab File: BG053590.D
Acq: 17 May 2022 19:05

Tgt Ion: 164 Resp: 93551
Ion Ratio Lower Upper
164 100
162 102.2 82.3 123.5
160 43.7 34.2 51.2

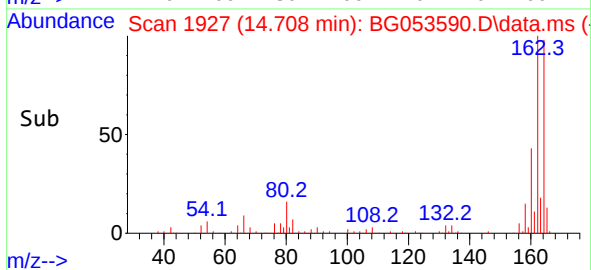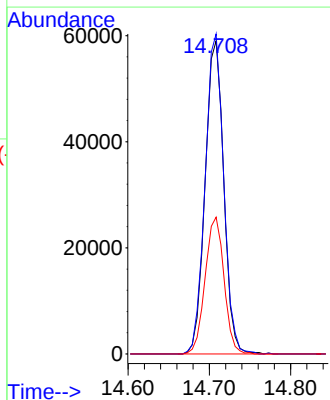



#42

2,4,6-Tribromophenol

Concen: 104.220 ng

RT: 16.195 min Scan# 21

Delta R.T. -0.007 min

Lab File: BG053590.D


Acq: 17 May 2022 19:05

Instrument :

BNA_G

ClientSampleId :

P003-SS003-1824-01

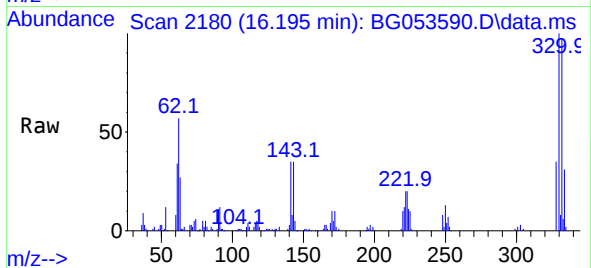




Tgt Ion:330 Resp: 143800

Ion Ratio Lower Upper

330 100

332 95.3 76.0 114.0

141 33.5 27.1 40.7

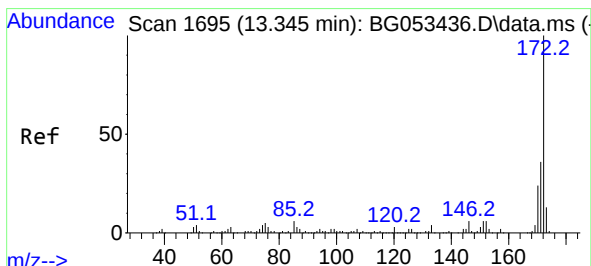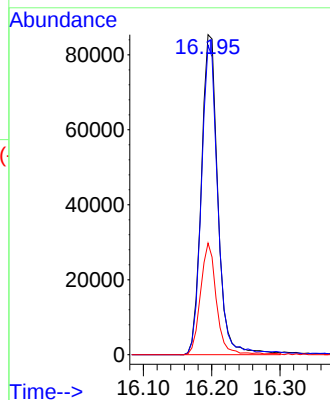

#45

2-Fluorobiphenyl

Concen: 62.187 ng

RT: 13.328 min Scan# 1692

Delta R.T. -0.007 min

Lab File: BG053590.D

Acq: 17 May 2022 19:05




Tgt Ion:172 Resp: 398123


Ion Ratio Lower Upper

172 100

171 34.4 28.5 42.7

170 23.5 18.9 28.3


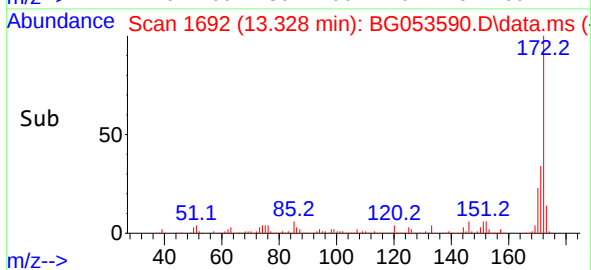

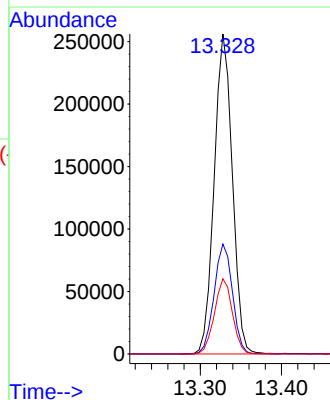


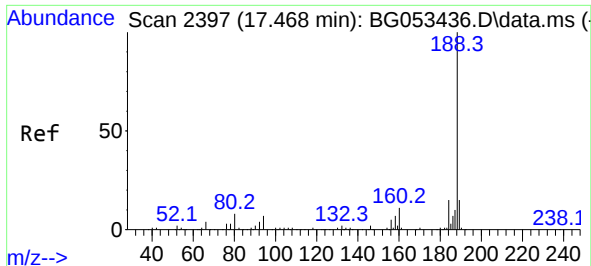

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.452 min Scan# 21
Delta R.T. -0.007 min
Lab File: BG053590.D
Acq: 17 May 2022 19:05




Instrument :
BNA_G
ClientSampleId :
P003-SS003-1824-01


Tgt Ion:188 Resp: 249600
Ion Ratio Lower Upper
188 100
94 6.6 5.4 8.0
80 7.9 6.8 10.2

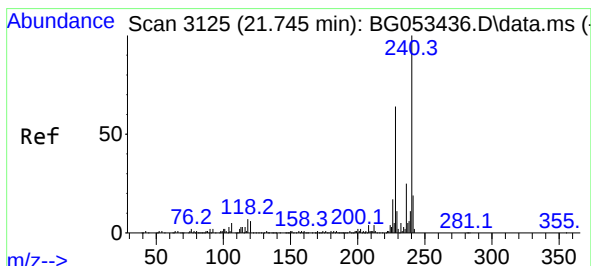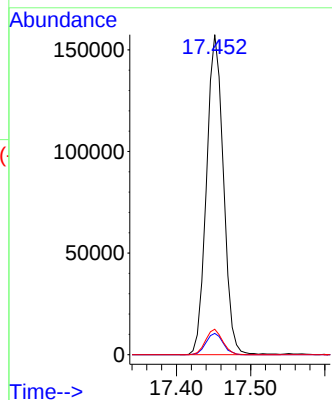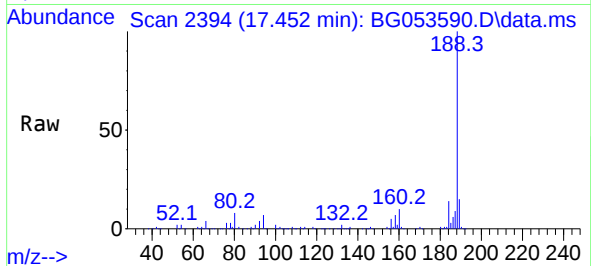

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.734 min Scan# 3123
Delta R.T. -0.007 min
Lab File: BG053590.D
Acq: 17 May 2022 19:05

Tgt Ion:240 Resp: 215295
Ion Ratio Lower Upper
240 100
120 5.9 4.6 7.0
236 24.2 20.2 30.4


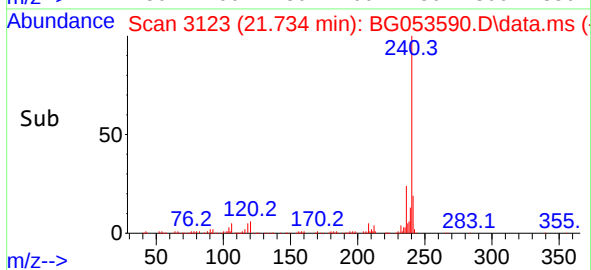
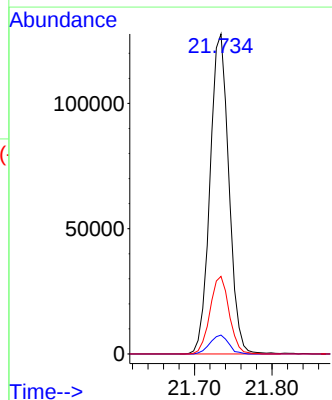





#79
Terphenyl-d14
Concen: 73.204 ng
RT: 20.054 min Scan# 21
Delta R.T. -0.007 min
Lab File: BG053590.D
Acq: 17 May 2022 19:05

Instrument :
BNA_G
ClientSampleId :
P003-SS003-1824-01

Tgt Ion:244 Resp: 846216
Ion Ratio Lower Upper
244 100
212 7.8 6.5 9.7
122 6.3 5.0 7.4

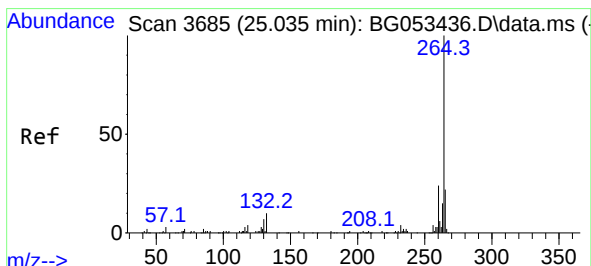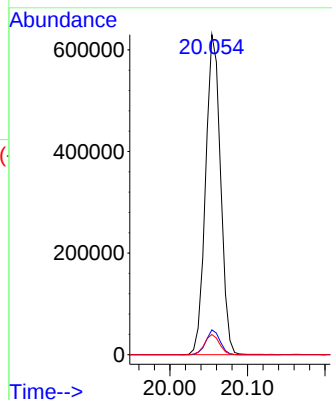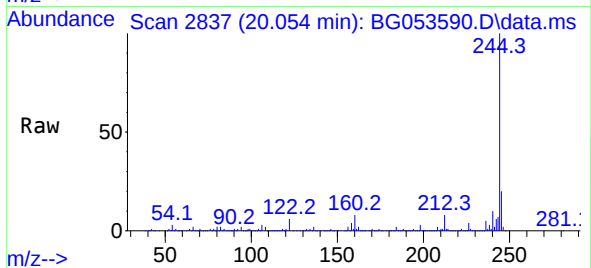

#86
Perylene-d12
Concen: 20.000 ng
RT: 25.012 min Scan# 3681
Delta R.T. -0.007 min
Lab File: BG053590.D
Acq: 17 May 2022 19:05

Tgt Ion:264 Resp: 193952
Ion Ratio Lower Upper
264 100
260 22.7 19.0 28.6
265 21.5 17.4 26.2

