

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
 Data File : BG053592.D
 Acq On : 17 May 2022 20:23
 Operator : CG/JU
 Sample : N2863-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P003-SS003-0612-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.650	379	385	399	rBV	235505	436994	28.55%	6.121%
2	7.242	646	656	671	rBV	283135	545287	35.63%	7.637%
3	8.082	792	799	808	rBV	93408	162682	10.63%	2.279%
4	9.245	989	997	1007	rBV	183813	359017	23.46%	5.028%
5	10.890	1270	1277	1286	rBV	145581	264387	17.28%	3.703%
6	13.327	1685	1692	1703	rBV	587667	904218	59.08%	12.665%
7	14.708	1919	1927	1935	rBV	280269	444528	29.05%	6.226%
8	16.194	2174	2180	2191	rBV	497908	791546	51.72%	11.087%
9	17.451	2387	2394	2403	rBV	401176	610306	39.88%	8.548%
10	20.054	2831	2837	2845	rVB	1218662	1530443	100.00%	21.436%
11	21.358	3056	3059	3063	rBV5	12884	22479	1.47%	0.315%
12	21.734	3116	3123	3130	rBV	289328	503965	32.93%	7.059%
13	22.515	3254	3256	3263	rVB4	13074	26379	1.72%	0.369%
14	25.012	3672	3681	3695	rVB2	177598	502922	32.86%	7.044%
15	26.140	3870	3873	3886	rVB2	12060	34503	2.25%	0.483%




Sum of corrected areas: 7139656

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
Data File : BG053592.D
Acq On : 17 May 2022 20:23
Operator : CG/JU
Sample : N2863-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P003-SS003-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

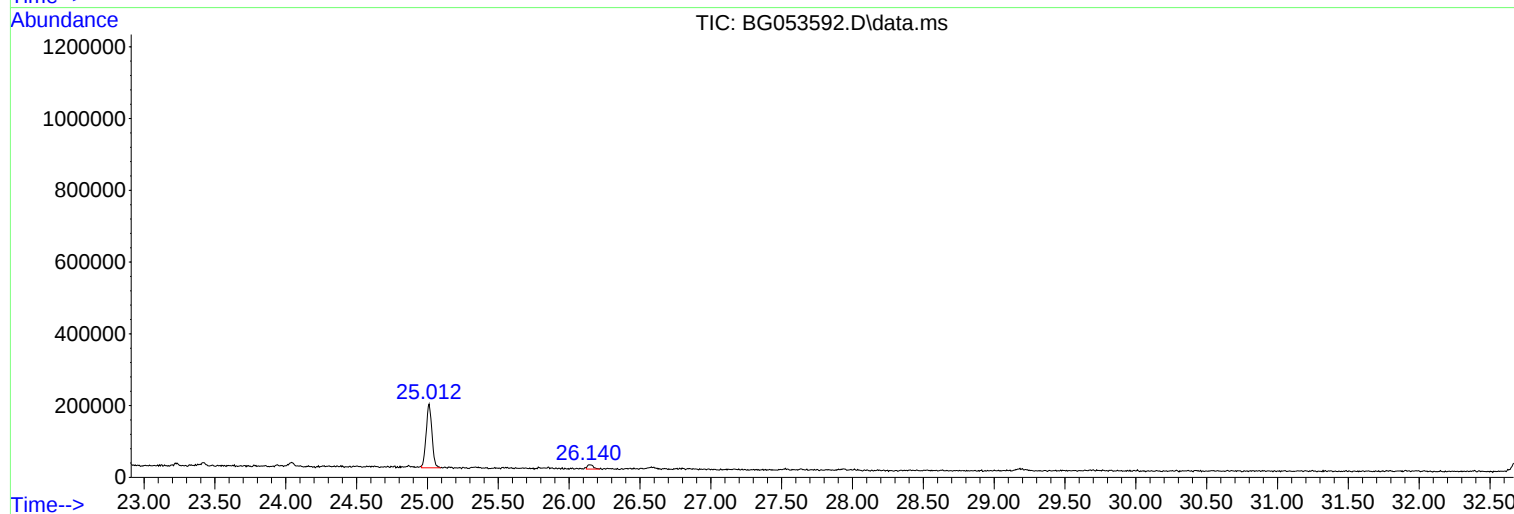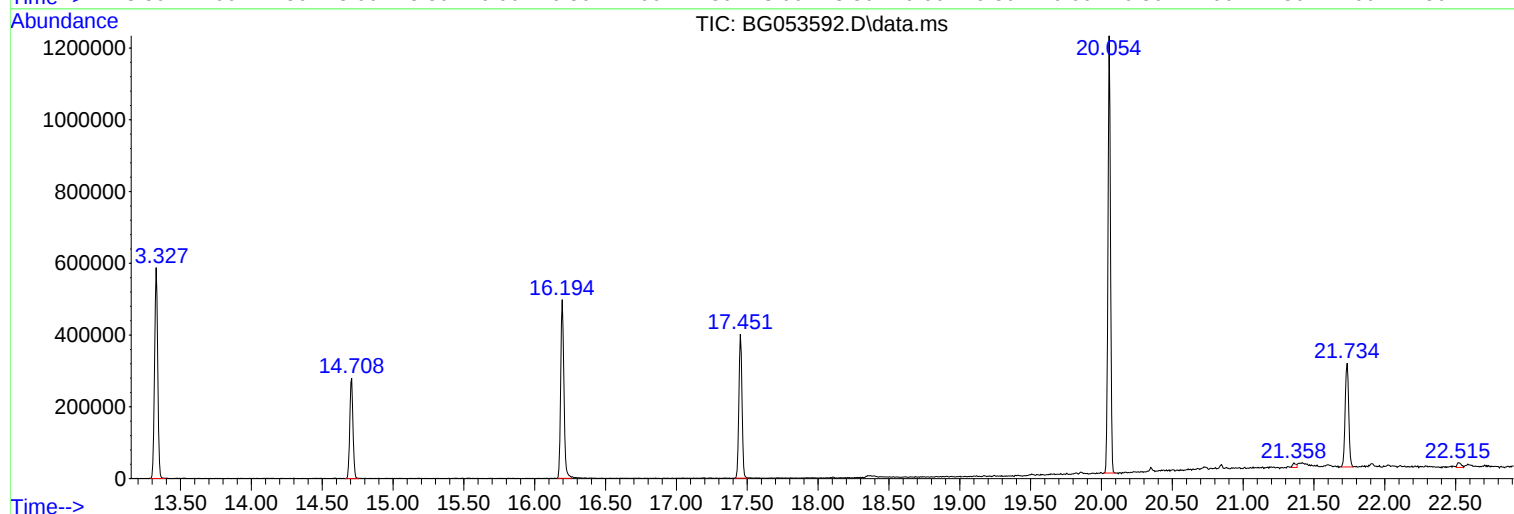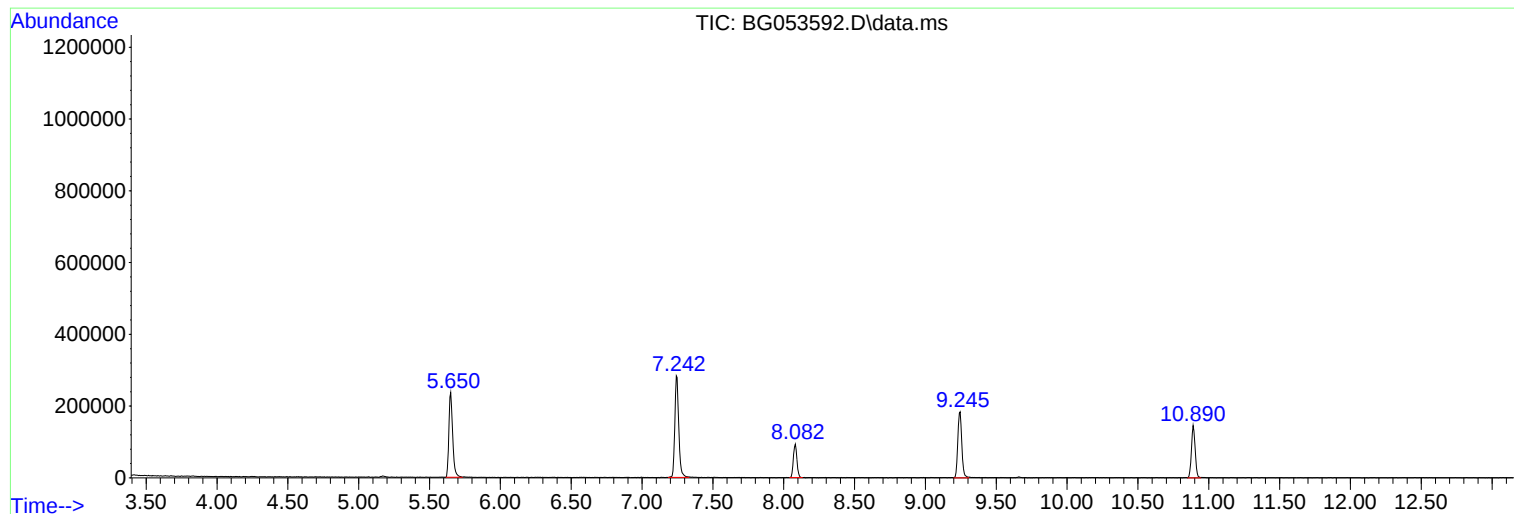

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
Data File : BG053592.D
Acq On : 17 May 2022 20:23
Operator : CG/JU
Sample : N2863-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P003-SS003-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
Data File : BG053592.D
Acq On : 17 May 2022 20:23
Operator : CG/JU
Sample : N2863-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P003-SS003-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------