
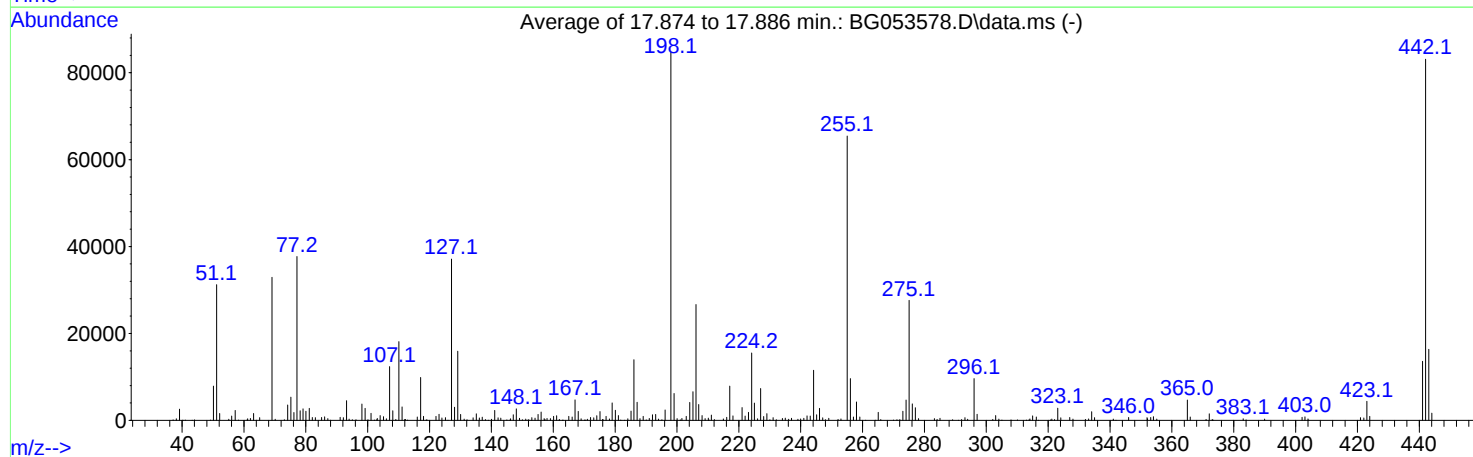


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
 Data File : BG053578.D
 Acq On : 17 May 2022 11:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 11 06:00:46 2022

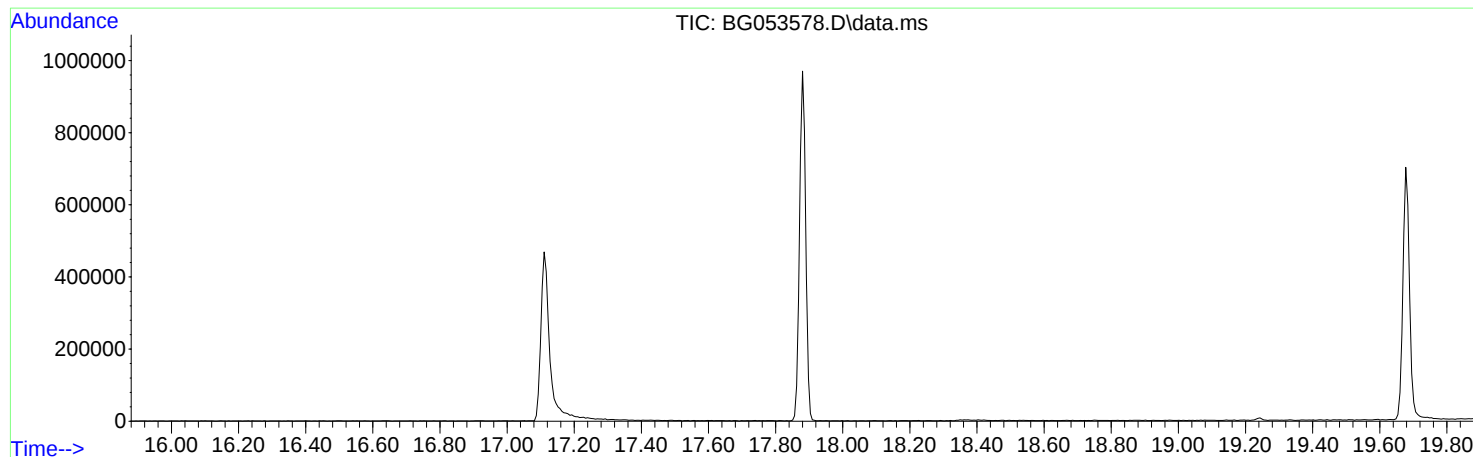




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	31243	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.9	32933	PASS
70	69	0.00	2	0.8	265	PASS
127	198	10	80	43.8	37109	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84656	PASS
199	198	5	9	7.3	6186	PASS
275	198	10	60	32.6	27611	PASS
365	198	1	100	5.5	4665	PASS
441	198	0.01	100	16.0	13573	PASS
442	442	50	100	100.0	83104	PASS
443	442	15	24	19.7	16335	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
Data File : BG053578.D
Acq On : 17 May 2022 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 18 04:46:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

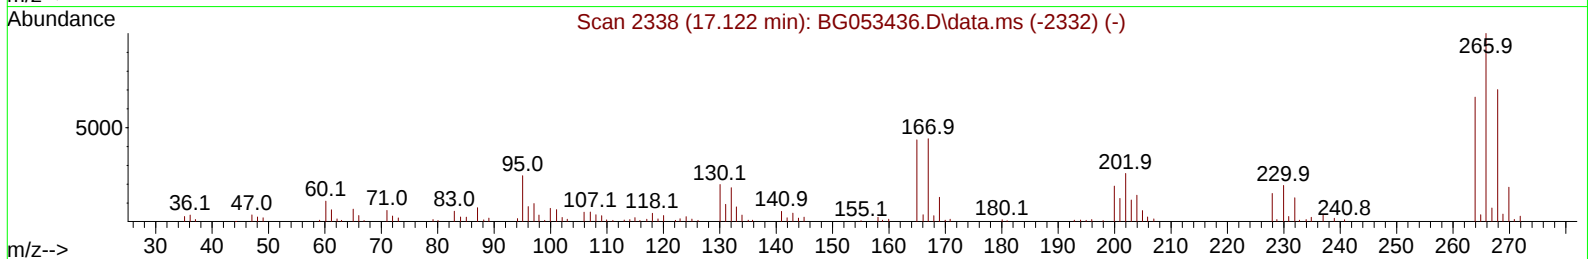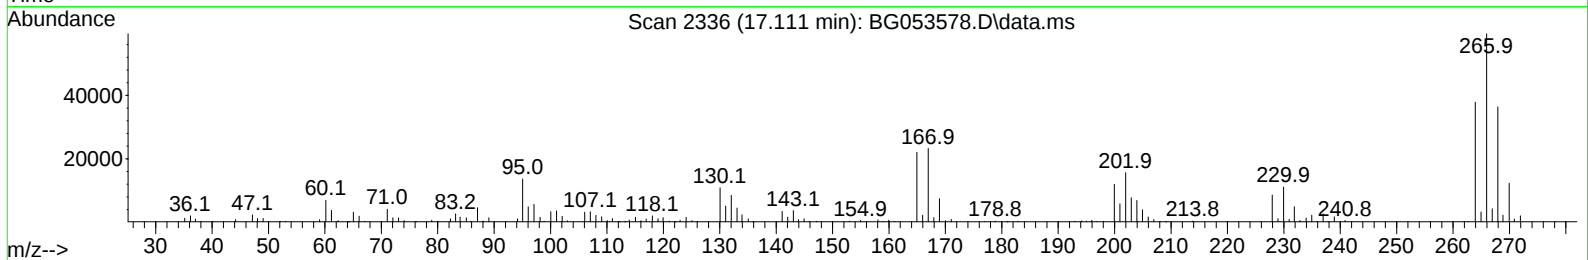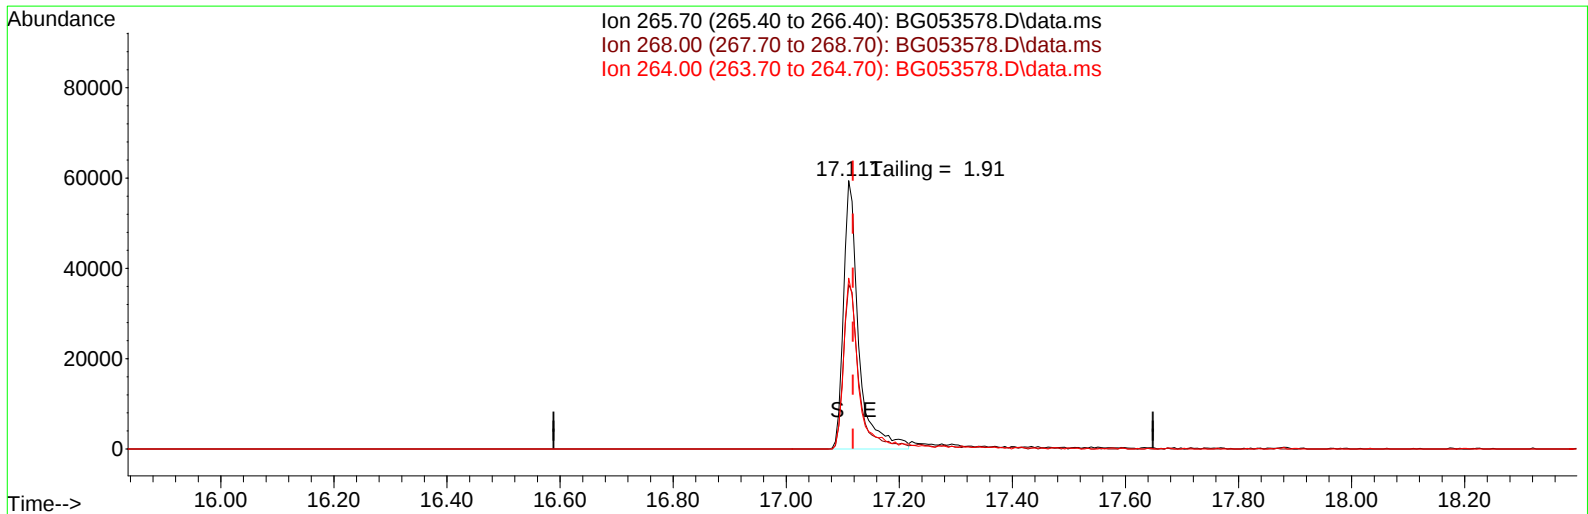

TIC: BG053578.D\data.ms

(70) Pentachlorophenol (C)

17.111min (-0.008) 28260.74 ng




response 108694

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.25
264.00	66.20	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051722\
Data File : BG053578.D
Acq On : 17 May 2022 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 18 04:46:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

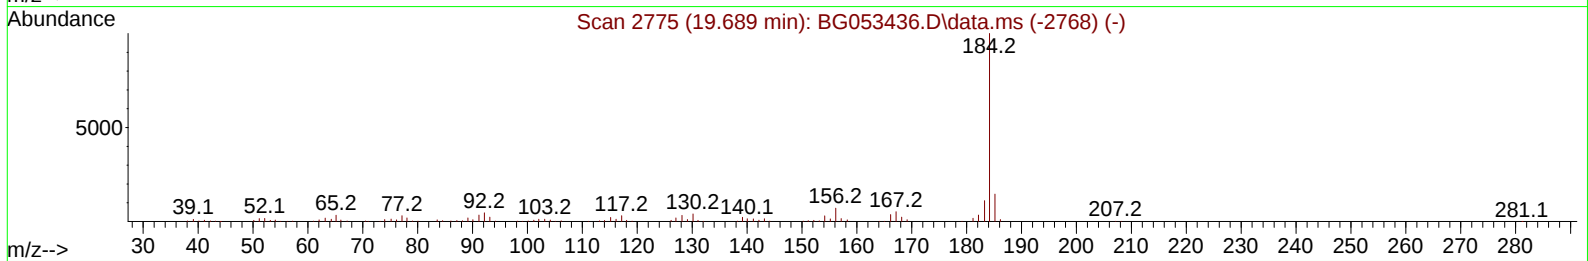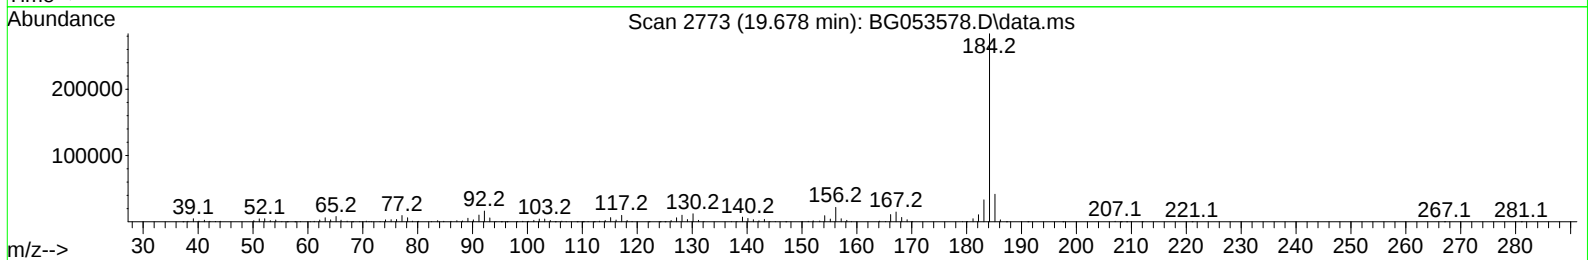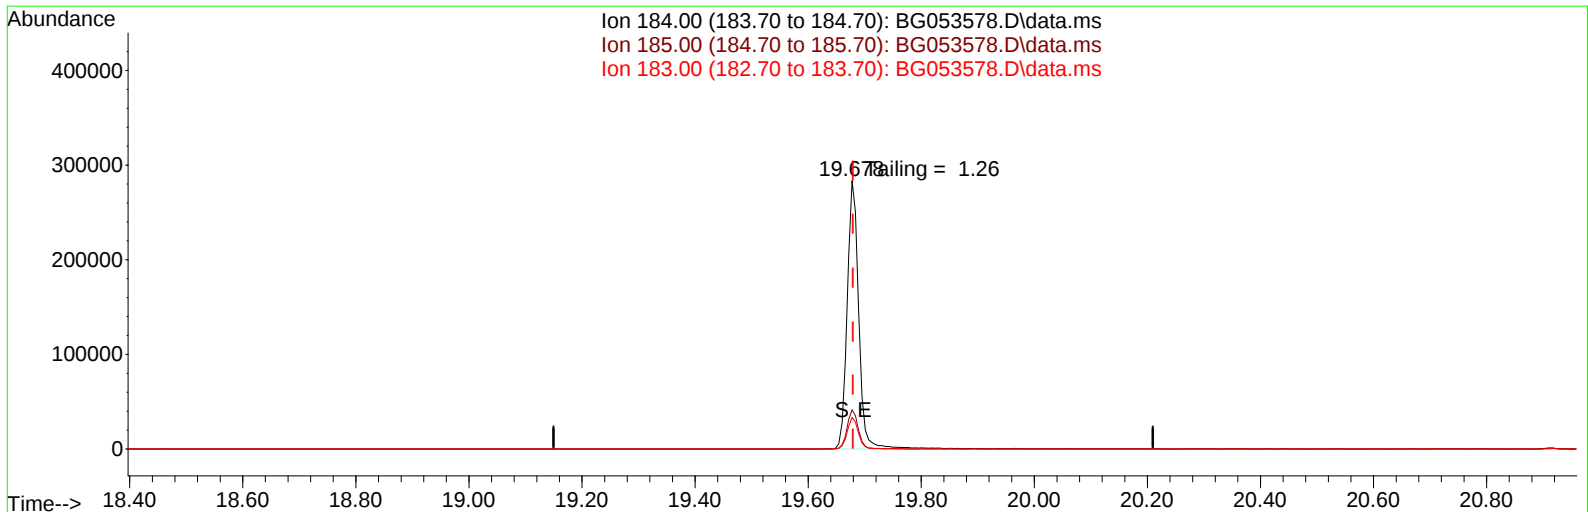

TIC: BG053578.D\data.ms

(77) Benzidine

19.678min (-0.002) 118293.91 ng

response 402848

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.64
183.00	11.10	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/17/2022	BNA_G	<u>BG053578.D</u>
Compound Name	Response	Retention Time
DDT	269225	20.911
DDD	12176	20.471
DDE	991	19.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13167	282392	4.66

Instrument :
BNA_G
ClientSampleId :
DFTPP