
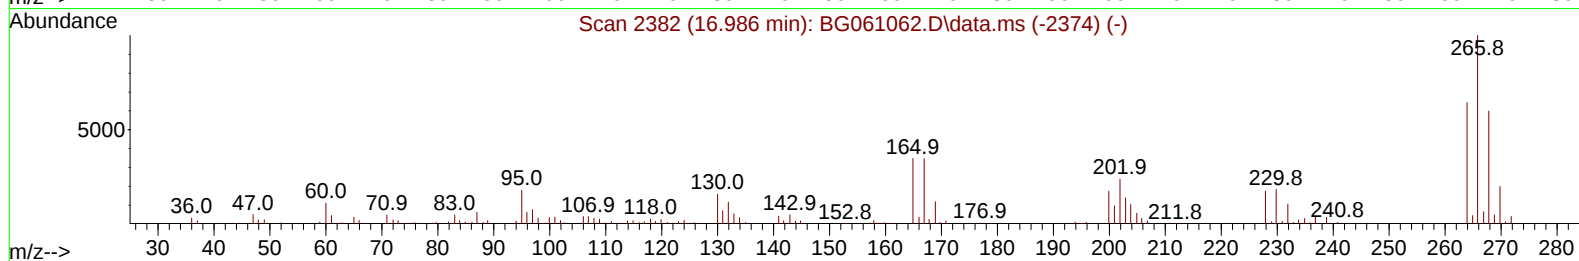
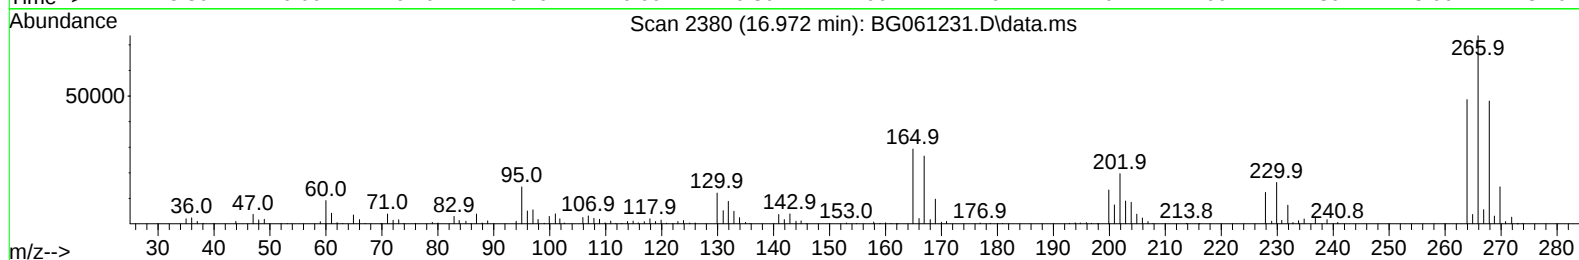


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051724\
Data File : BG061231.D
Acq On : 17 May 2024 8:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 09:32:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

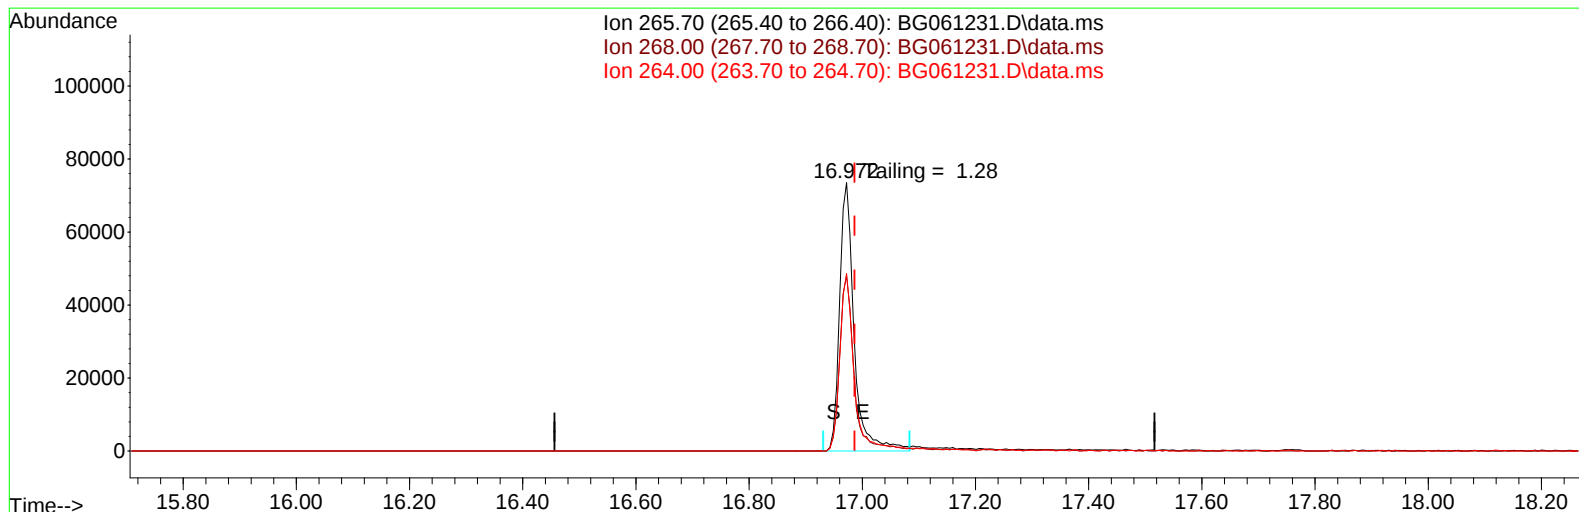

TIC: BG061231.D\data.ms

(70) Pentachlorophenol (C)




16.972min (-0.014) 38518.12 ng

response 131498

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	65.37
264.00	64.40	66.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051724\
Data File : BG061231.D
Acq On : 17 May 2024 8:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 09:32:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

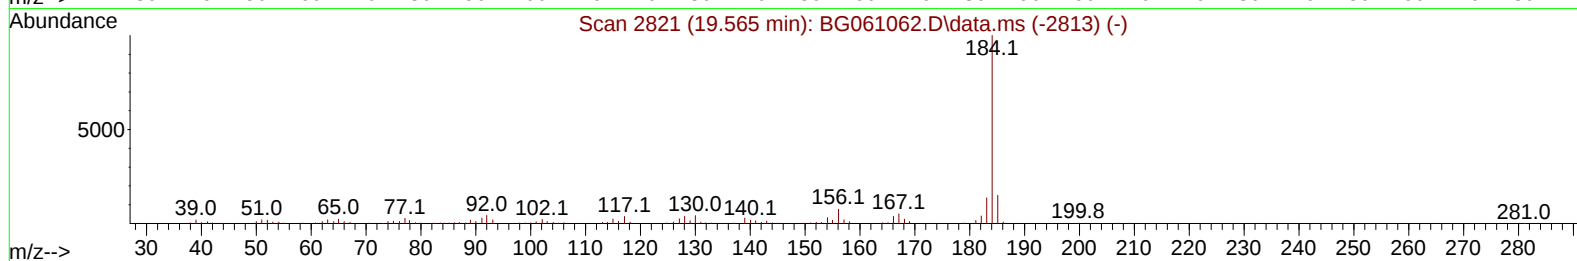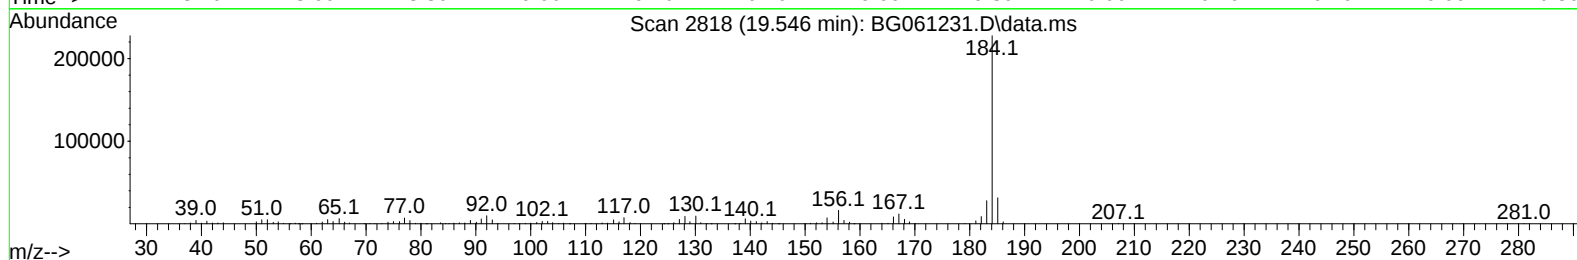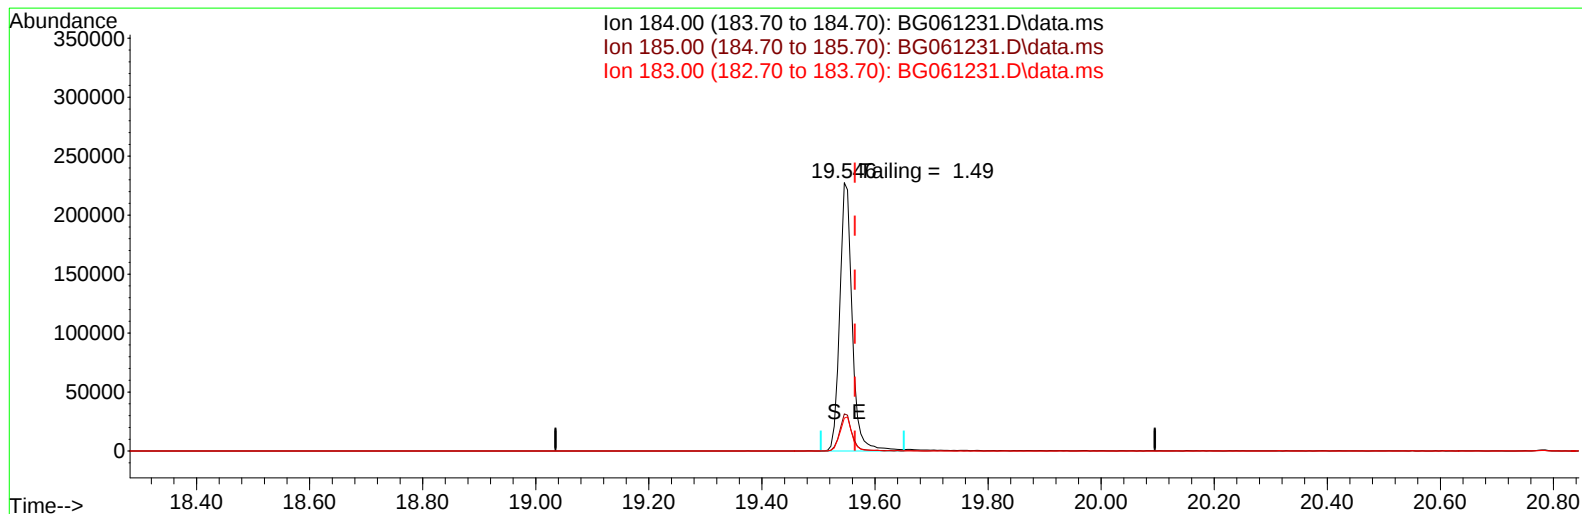

TIC: BG061231.D\data.ms

(77) Benzidine**19.546min (-0.019) 246058.16 ng****response 348024**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.84
183.00	13.60	12.30
0.00	0.00	0.00