


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051724\
Data File : BG061231.D
Acq On : 17 May 2024 8:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

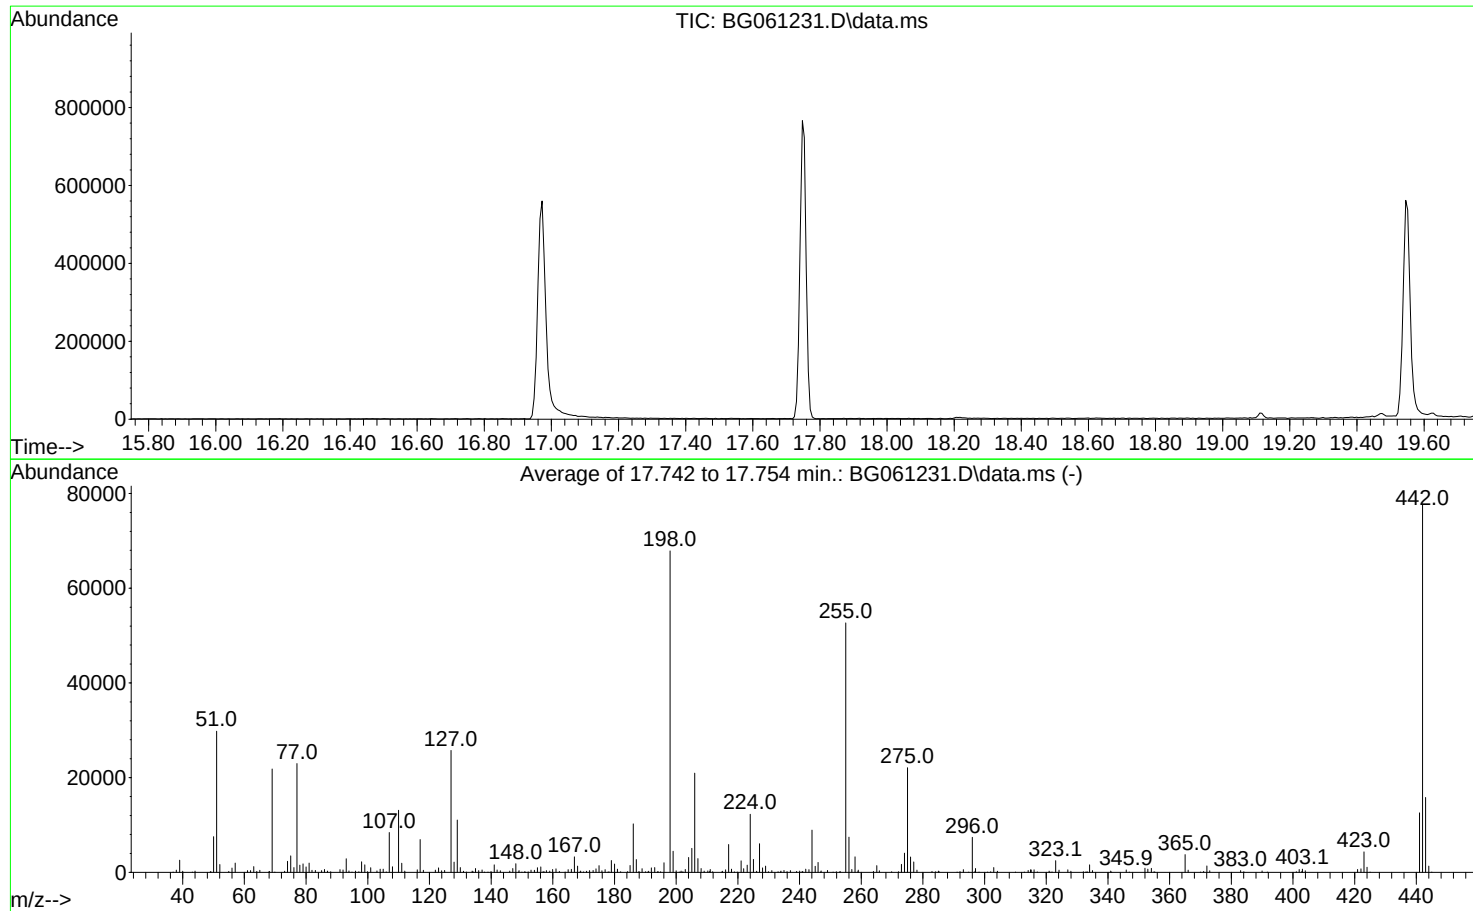

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	29811	PASS
68	69	0.00	2	0.9	203	PASS
69	198	0.00	100	32.2	21840	PASS
70	69	0.00	2	0.3	60	PASS
127	198	10	80	37.9	25739	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67888	PASS
199	198	5	9	6.5	4444	PASS
275	198	10	60	32.6	22110	PASS
365	198	1	100	5.5	3742	PASS
441	198	0.01	100	18.5	12560	PASS
442	442	50	100	100.0	77677	PASS
443	442	15	24	20.4	15825	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/17/2024	BNA_G	<u>BG061231.D</u>
Compound Name	Response	Retention Time
DDT	2527071	20.779
DDD	7284	20.339
DDE	805	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8089	2535160	0.32

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051724\
Data File : BG061231.D
Acq On : 17 May 2024 8:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 17 09:32:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

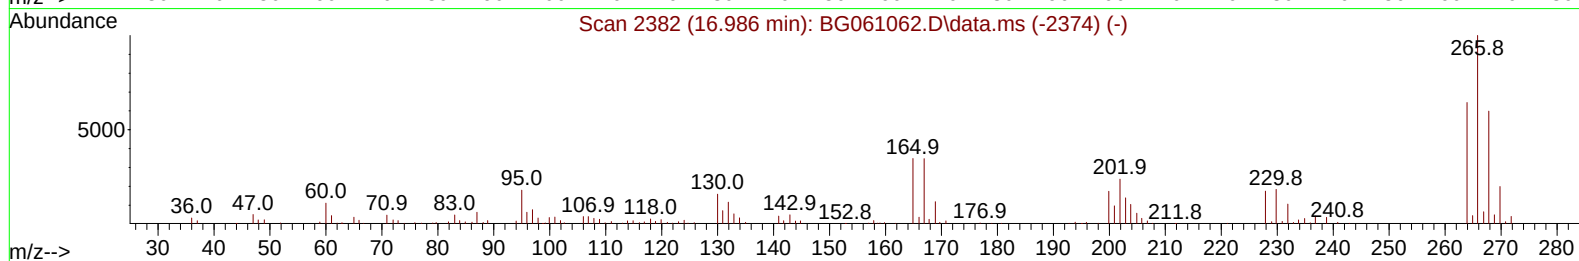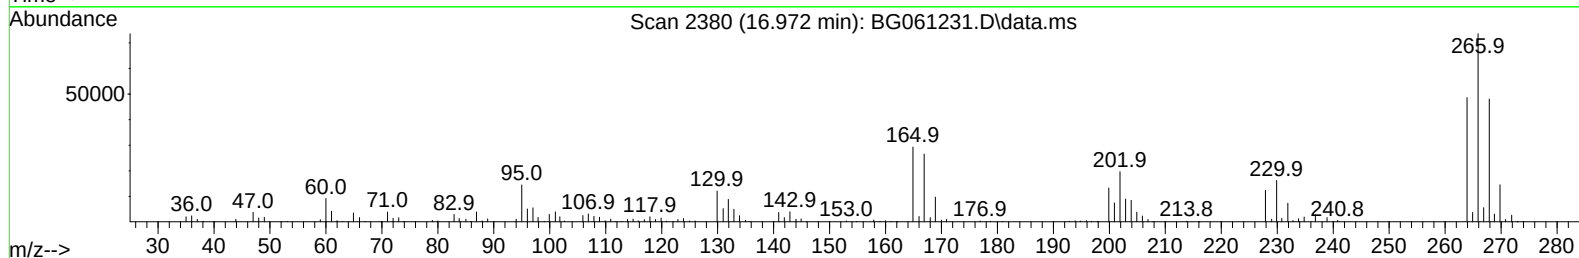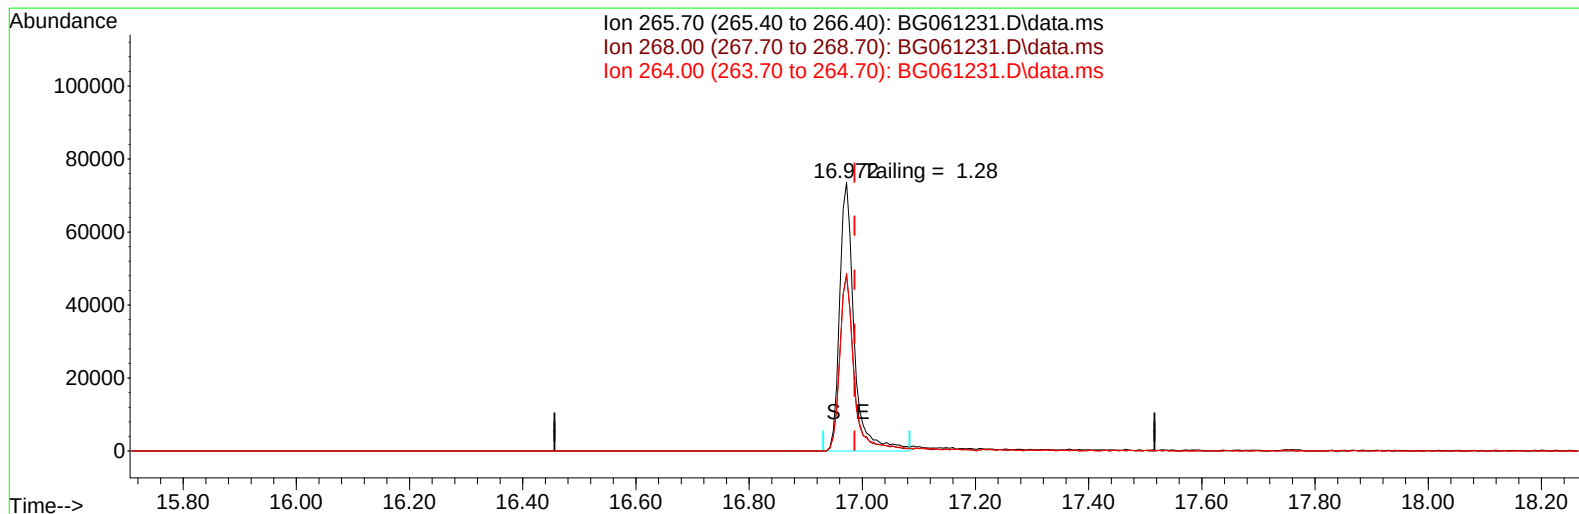

TIC: BG061231.D\data.ms

(70) Pentachlorophenol (C)

16.972min (-0.014) 38518.12 ng




response 131498

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	65.37
264.00	64.40	66.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051724\
Data File : BG061231.D
Acq On : 17 May 2024 8:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 17 09:32:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

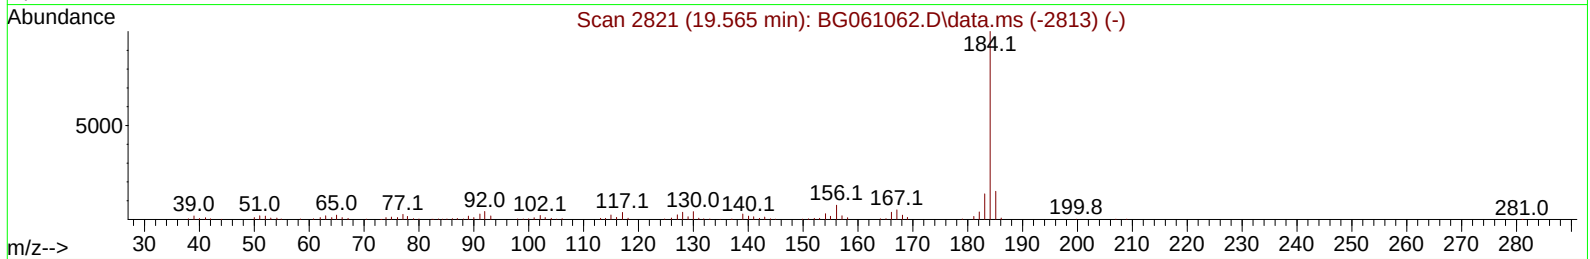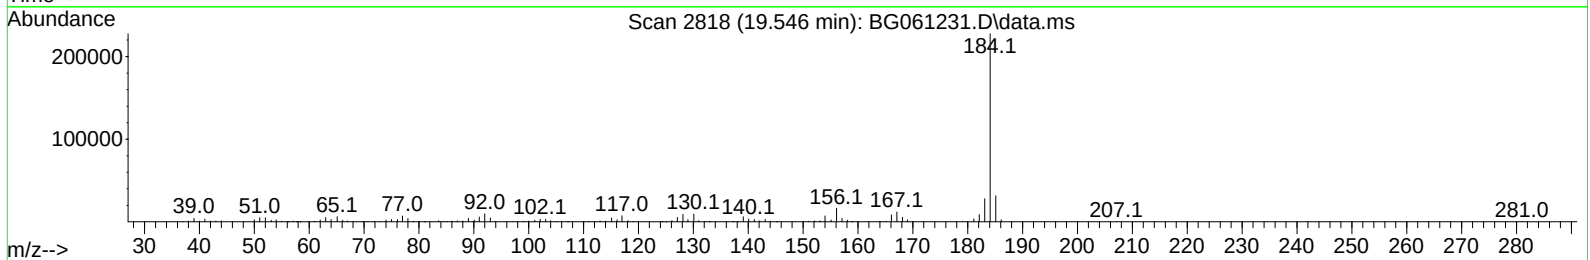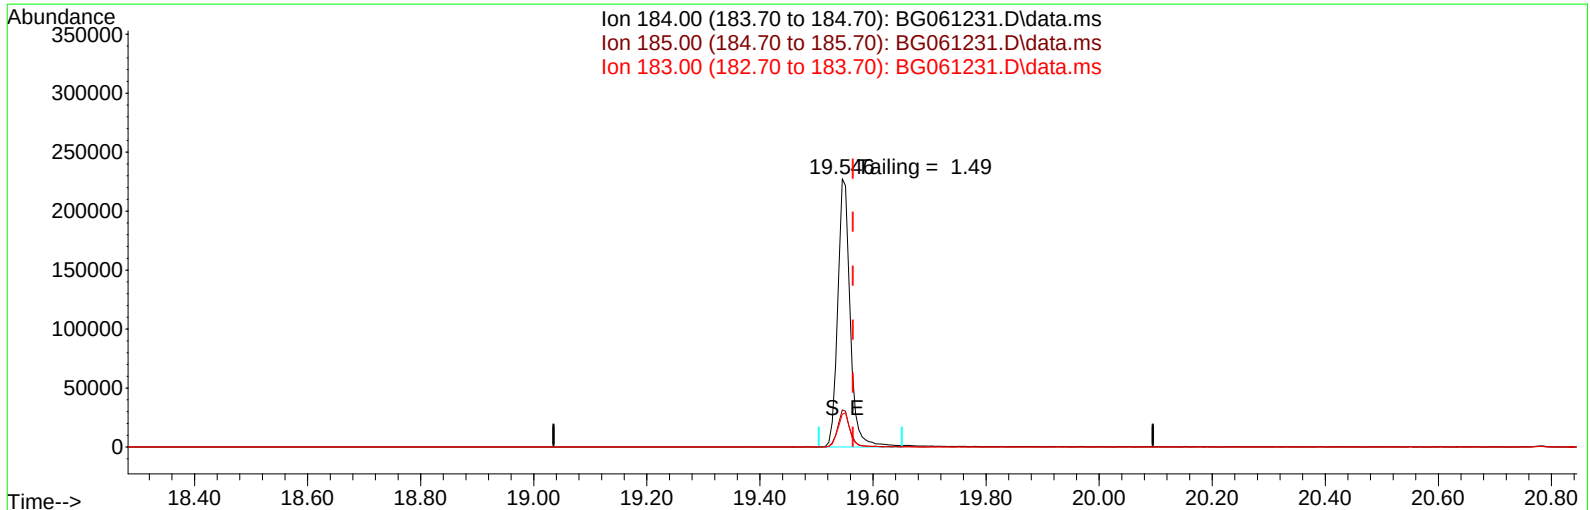

TIC: BG061231.D\data.ms

(77) Benzidine

19.546min (-0.019) 246058.16 ng

response 348024

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.84
183.00	13.60	12.30
0.00	0.00	0.00