
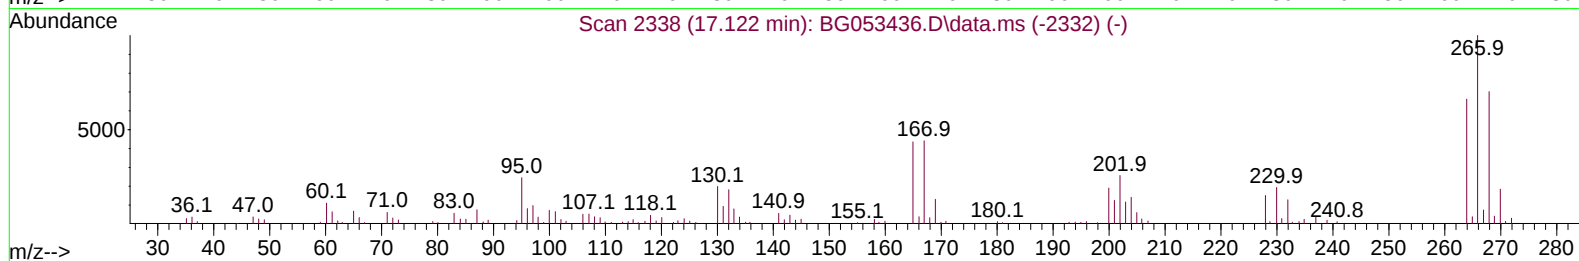
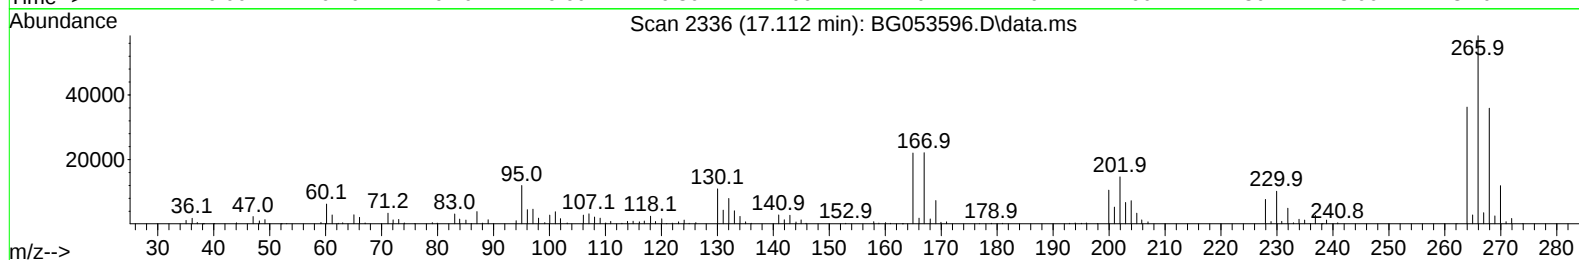


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051822\
Data File : BG053596.D
Acq On : 18 May 2022 8:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 14:28:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

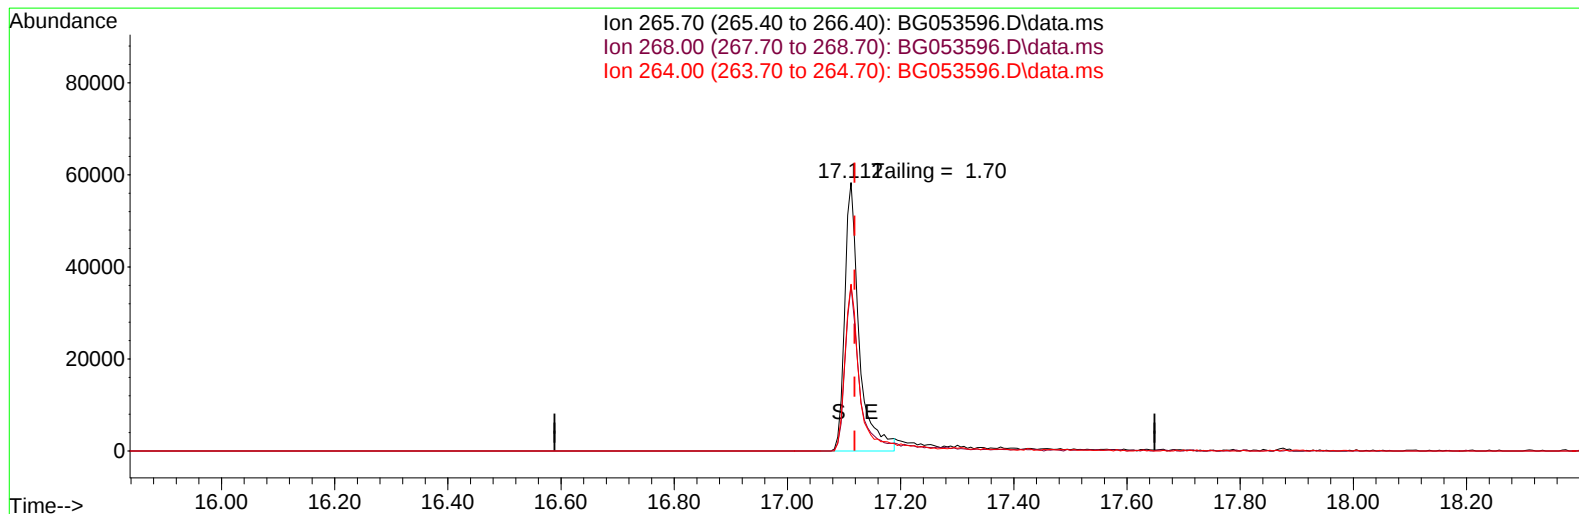

TIC: BG053596.D\data.ms

(70) Pentachlorophenol (C)




17.112min (-0.006) 30554.00 ng

response 111260

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.53
264.00	66.20	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051822\
Data File : BG053596.D
Acq On : 18 May 2022 8:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 14:28:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

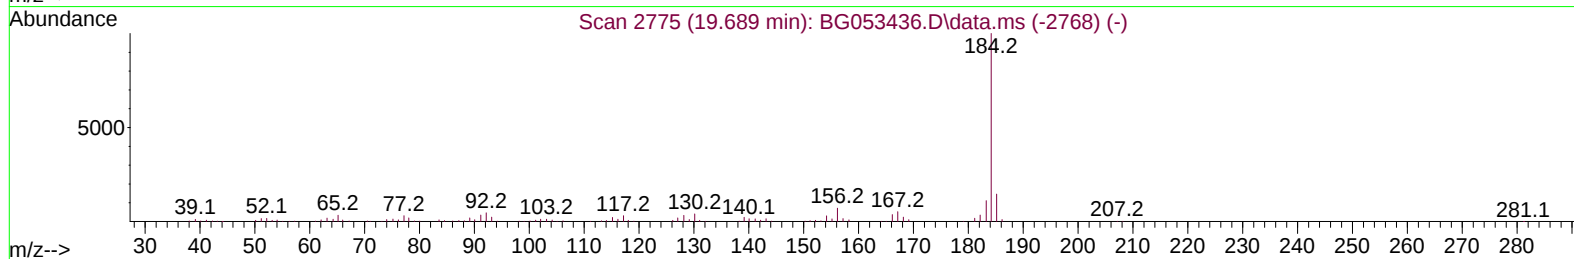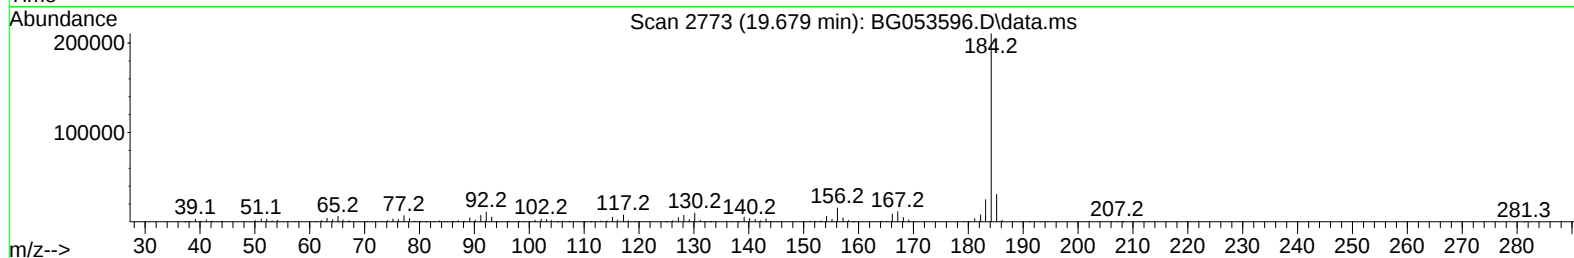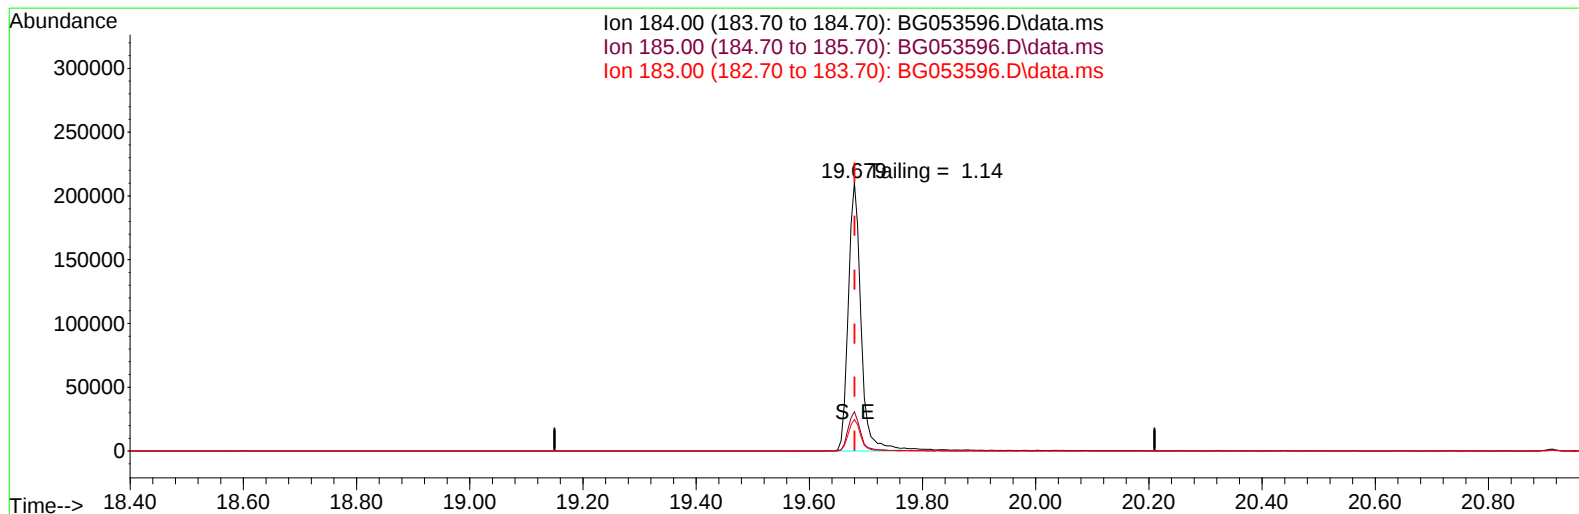

TIC: BG053596.D\data.ms

(77) Benzidine

19.679min (-0.000) 0.00 ng

response 333671

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.66
183.00	11.10	11.79
0.00	0.00	0.00