

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051822\
 Data File : BG053620.D
 Acq On : 19 May 2022 1:57
 Operator : CG/JU
 Sample : N2906-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CDF-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.644	378	384	397	rBV	334274	566463	34.04%	7.787%
2	7.242	647	656	671	rBV	350007	639998	38.45%	8.797%
3	8.076	791	798	807	rBV	86856	152985	9.19%	2.103%
4	9.239	985	996	1012	rBV	218812	416112	25.00%	5.720%
5	10.890	1269	1277	1286	rBV	114622	212500	12.77%	2.921%
6	13.328	1685	1692	1700	rVB	594943	928202	55.77%	12.759%
7	14.702	1919	1926	1934	rVB	202501	316538	19.02%	4.351%
8	16.195	2173	2180	2198	rBV	453029	760360	45.69%	10.452%
9	17.452	2386	2394	2404	rBV	290638	450224	27.05%	6.189%
10	20.054	2831	2837	2845	rVB	1276849	1664301	100.00%	22.878%
11	21.352	3054	3058	3064	rBV6	15158	32313	1.94%	0.444%
12	21.728	3113	3122	3131	rBV2	310119	549021	32.99%	7.547%
13	22.515	3254	3256	3263	rVB6	10445	18772	1.13%	0.258%
14	23.209	3368	3374	3383	rVB9	12600	31172	1.87%	0.428%
15	24.043	3512	3516	3521	rVB7	11077	19483	1.17%	0.268%
16	25.006	3671	3680	3693	rVB2	181100	516334	31.02%	7.098%




Sum of corrected areas: 7274778

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051822\
Data File : BG053620.D
Acq On : 19 May 2022 1:57
Operator : CG/JU
Sample : N2906-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CDF-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

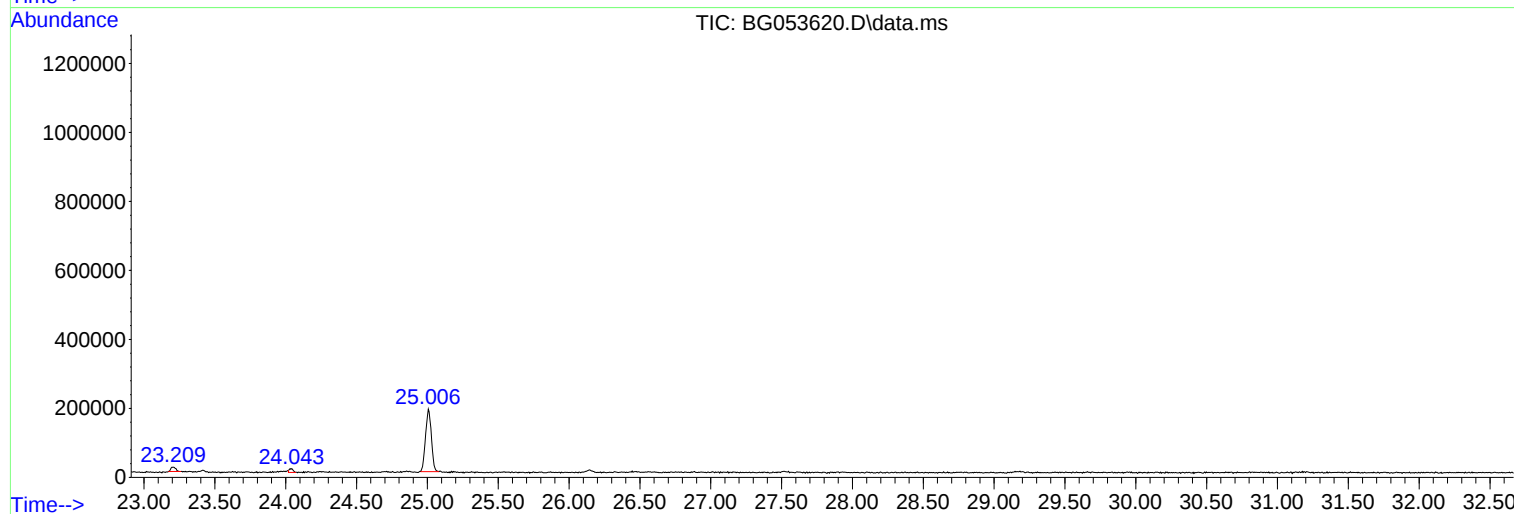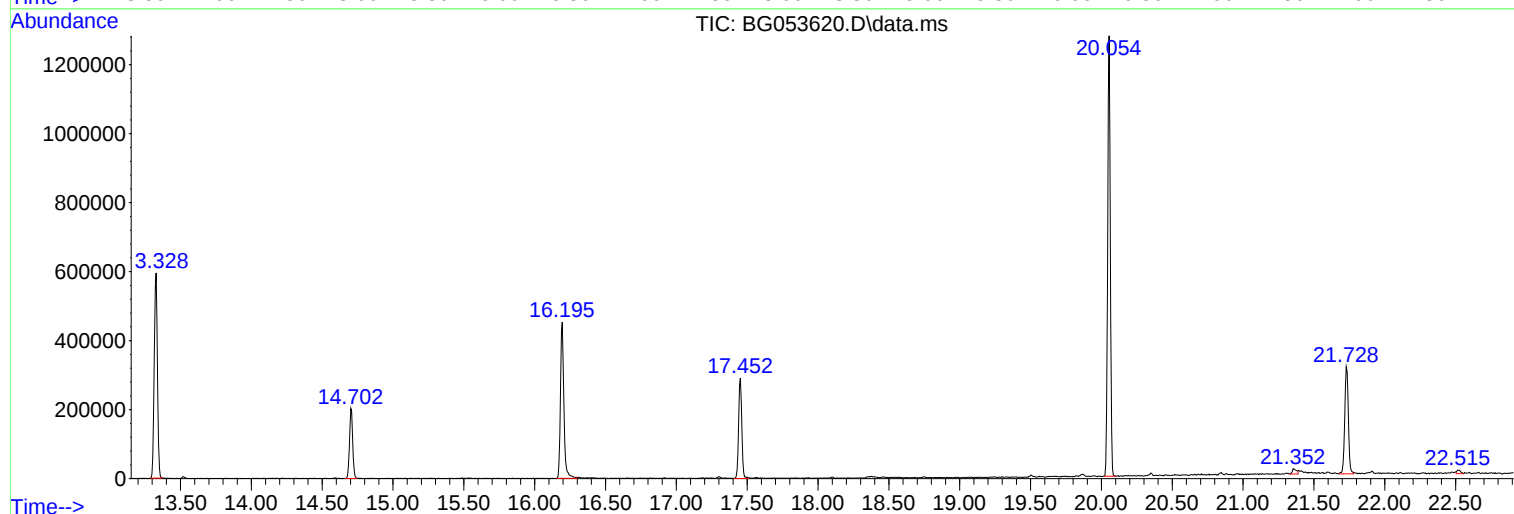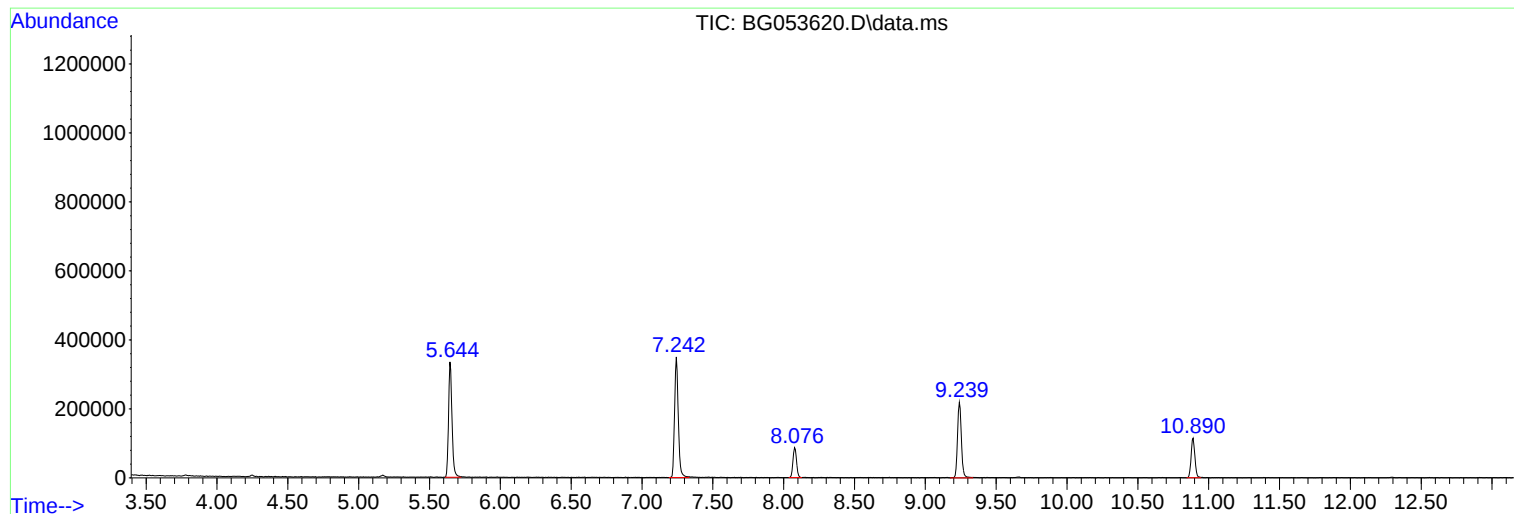

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051822\
Data File : BG053620.D
Acq On : 19 May 2022 1:57
Operator : CG/JU
Sample : N2906-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CDF-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051822\
Data File : BG053620.D
Acq On : 19 May 2022 1:57
Operator : CG/JU
Sample : N2906-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CDF-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------