
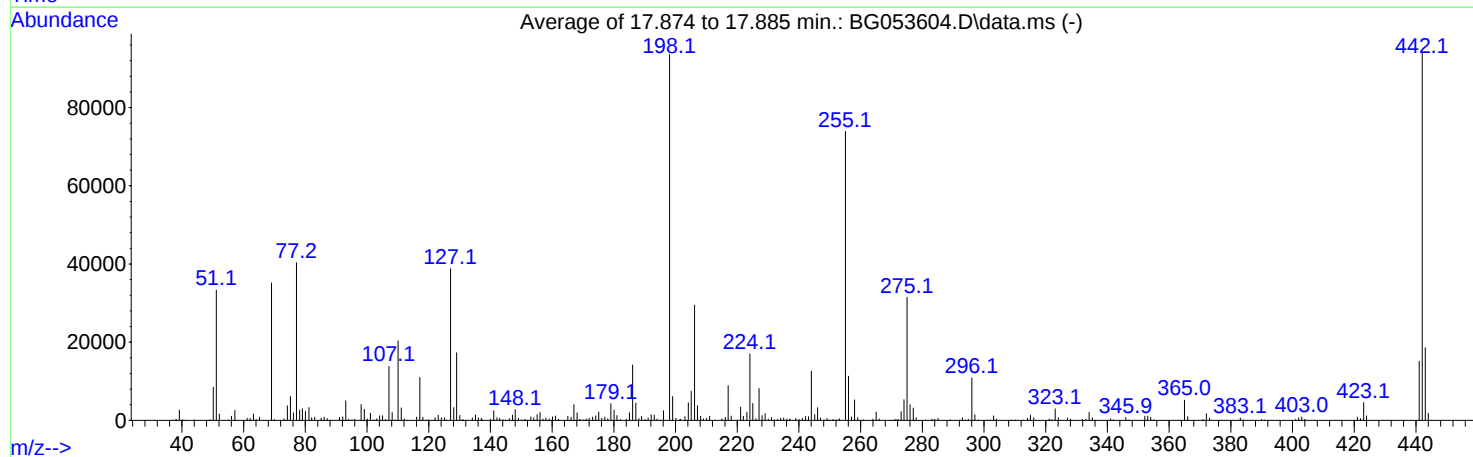


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051822\
 Data File : BG053604.D
 Acq On : 18 May 2022 14:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 11 06:00:46 2022

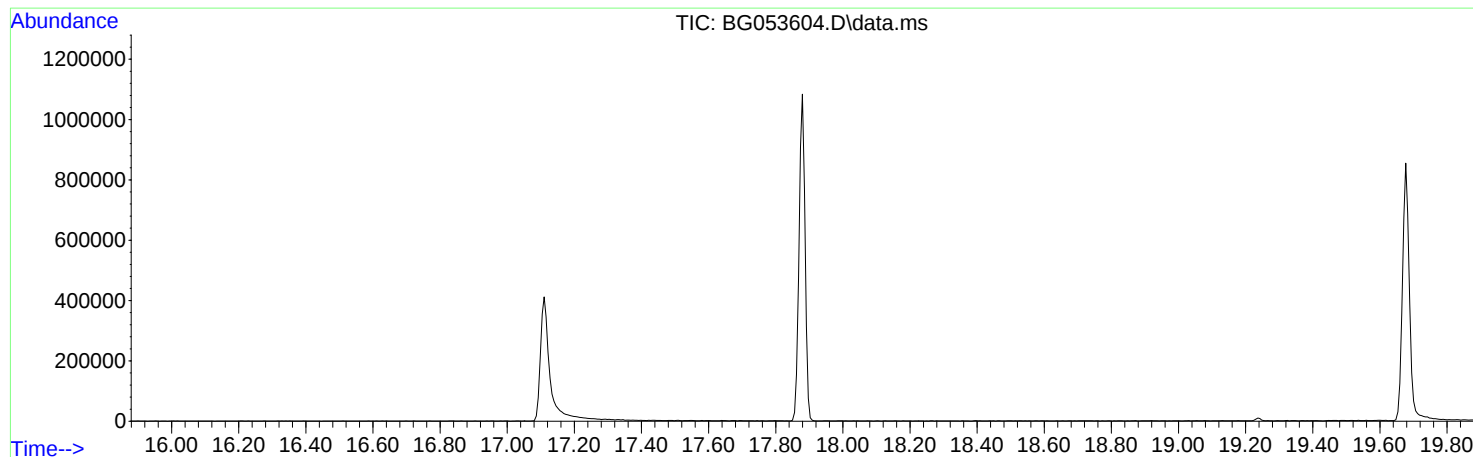




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	33331	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.6	35136	PASS
70	69	0.00	2	0.6	195	PASS
127	198	10	80	41.5	38816	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93539	PASS
199	198	5	9	6.5	6107	PASS
275	198	10	60	33.6	31469	PASS
365	198	1	100	5.5	5140	PASS
441	198	0.01	100	16.2	15120	PASS
442	442	50	100	100.0	94088	PASS
443	442	15	24	19.7	18573	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051822\
Data File : BG053604.D
Acq On : 18 May 2022 14:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 19 05:11:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

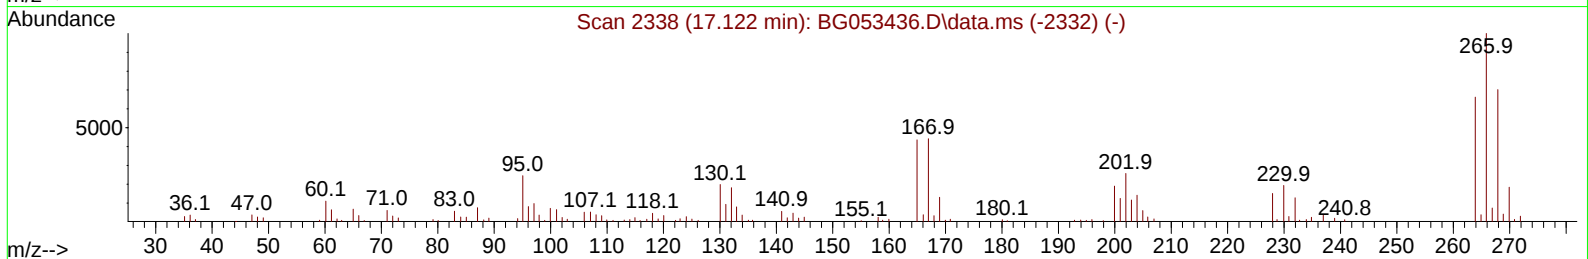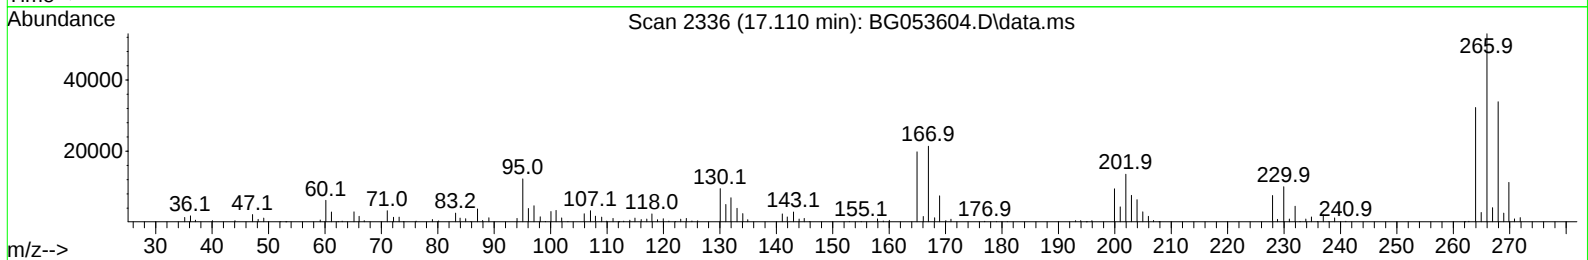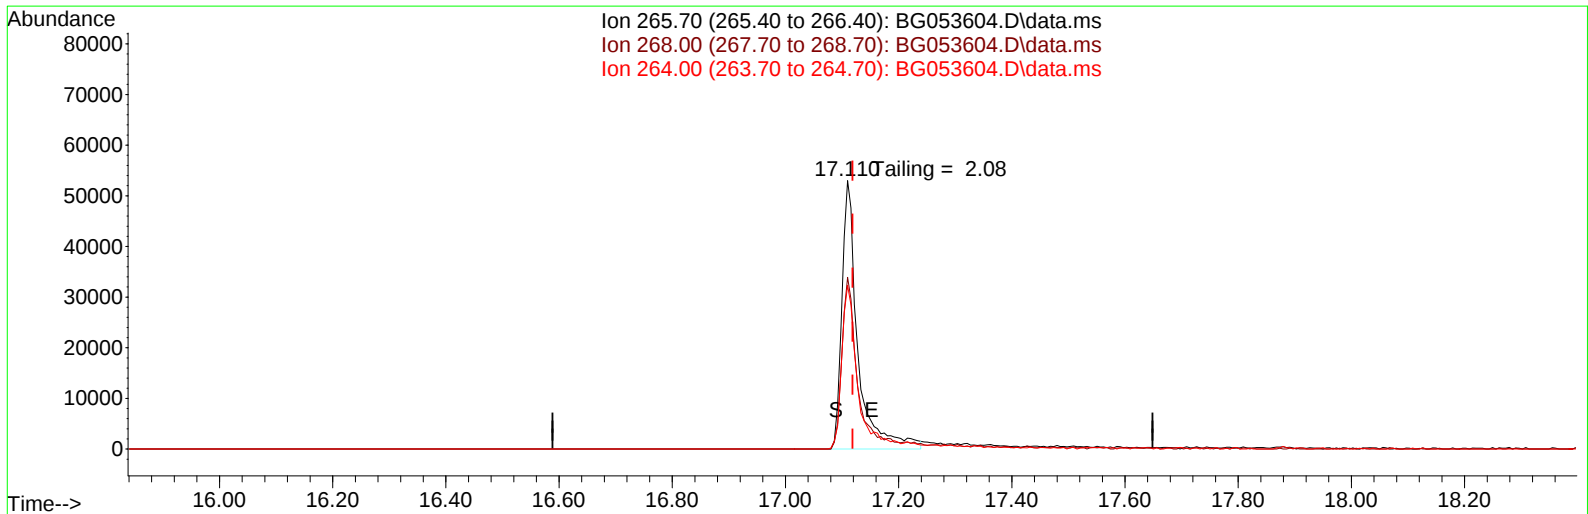

TIC: BG053604.D\data.ms

(70) Pentachlorophenol (C)

17.110min (-0.009) 23904.58 ng




response 100851

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.98
264.00	66.20	60.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051822\
Data File : BG053604.D
Acq On : 18 May 2022 14:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 19 05:11:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

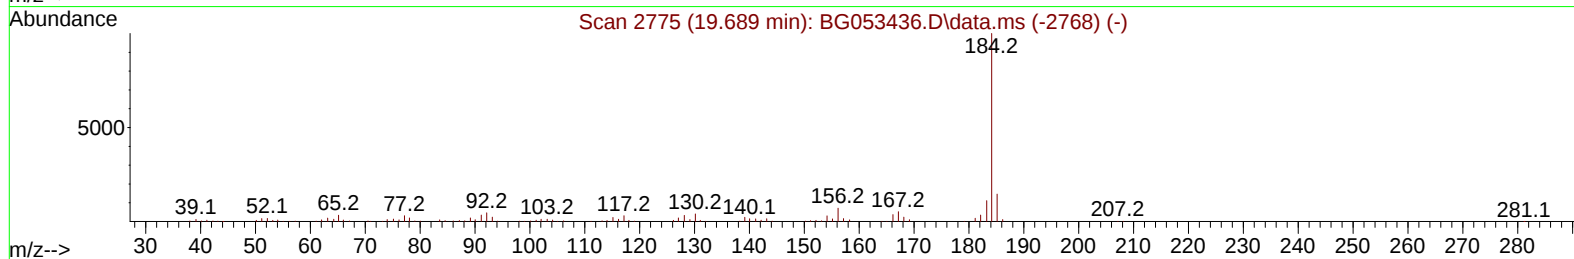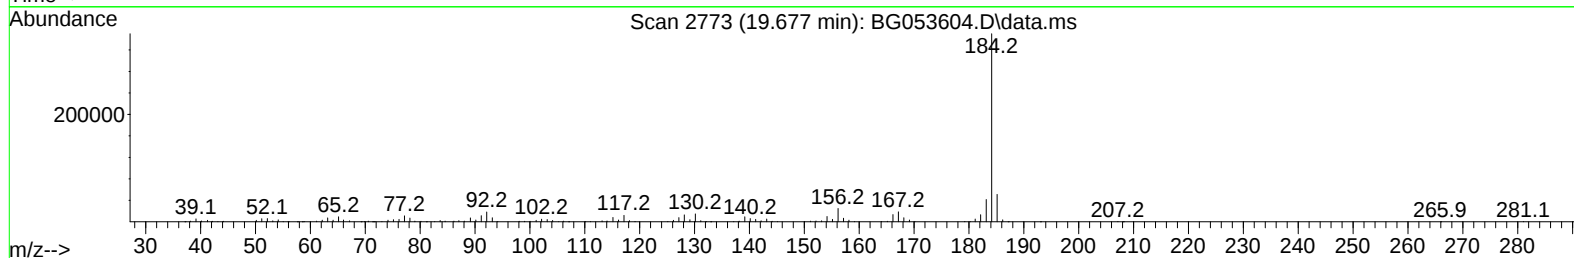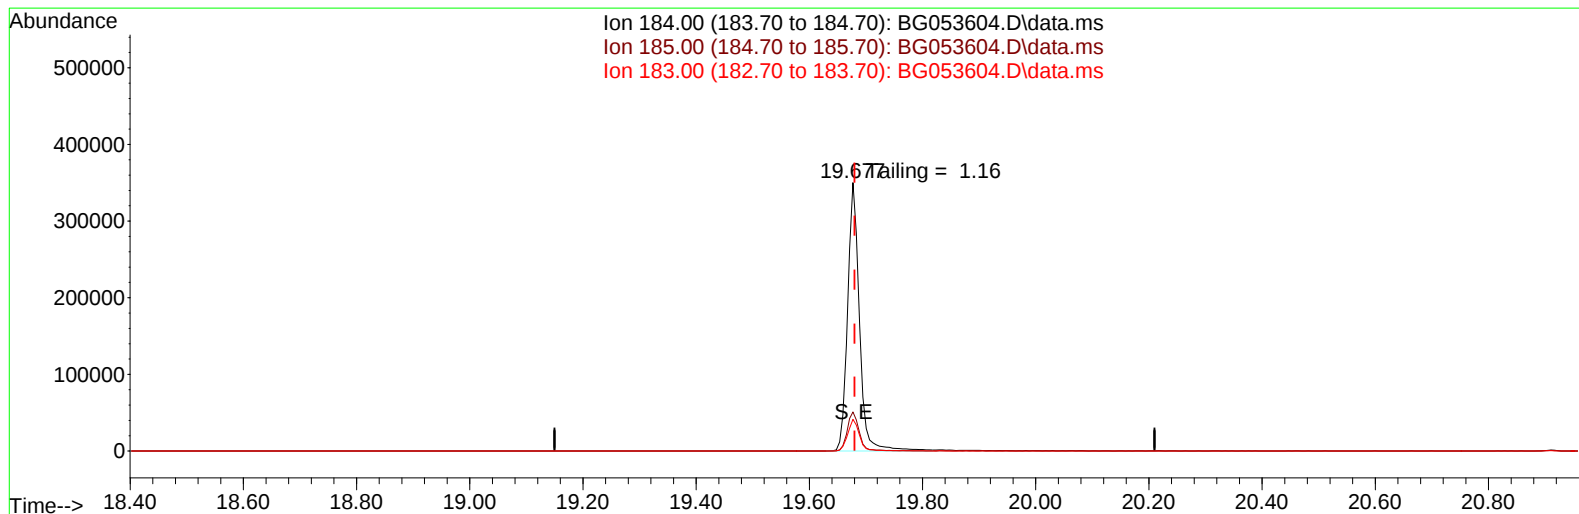

TIC: BG053604.D\data.ms

(77) Benzidine

19.677min (-0.003) 0.00 ng

response 510009

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.58
183.00	11.10	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/18/2022	BNA_G	<u>BG053604.D</u>
Compound Name	Response	Retention Time
DDT	323814	20.91
DDD	10096	20.47
DDE	788	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10884	334698	3.25

Instrument :
BNA_G
ClientSampleId :
DFTPP