
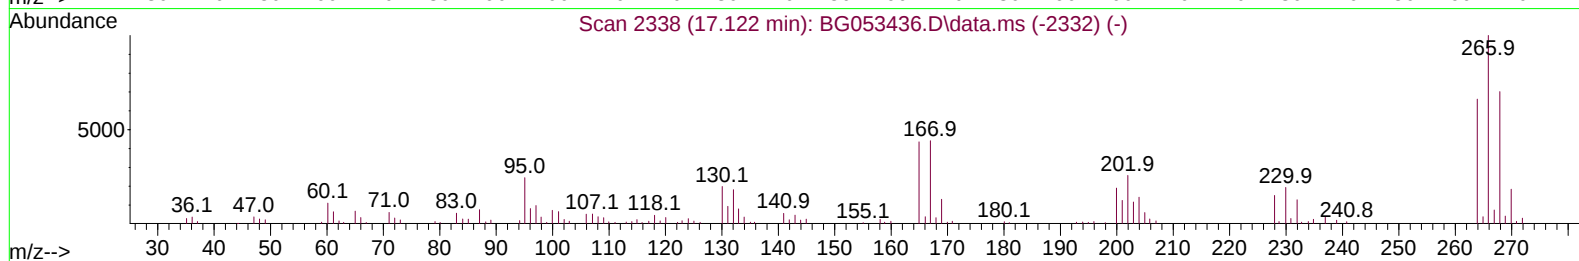
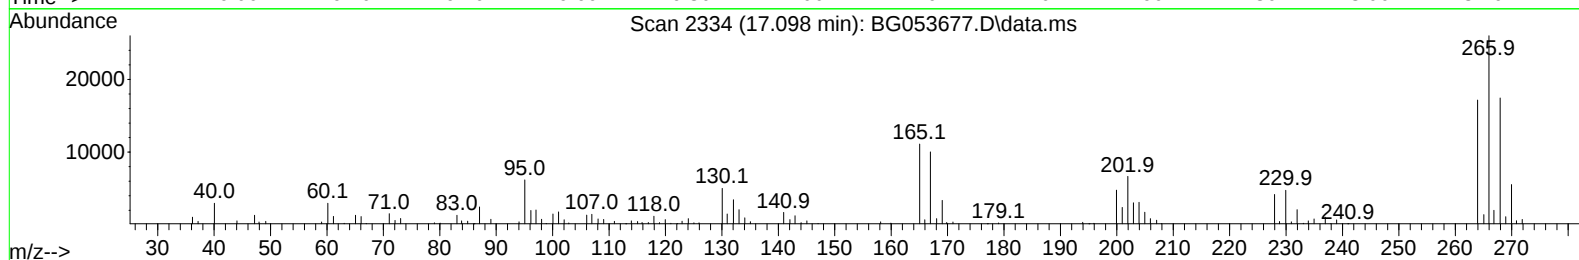


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
Data File : BG053677.D
Acq On : 24 May 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 15:08:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 24 05:05:32 2022
Response via : Initial Calibration

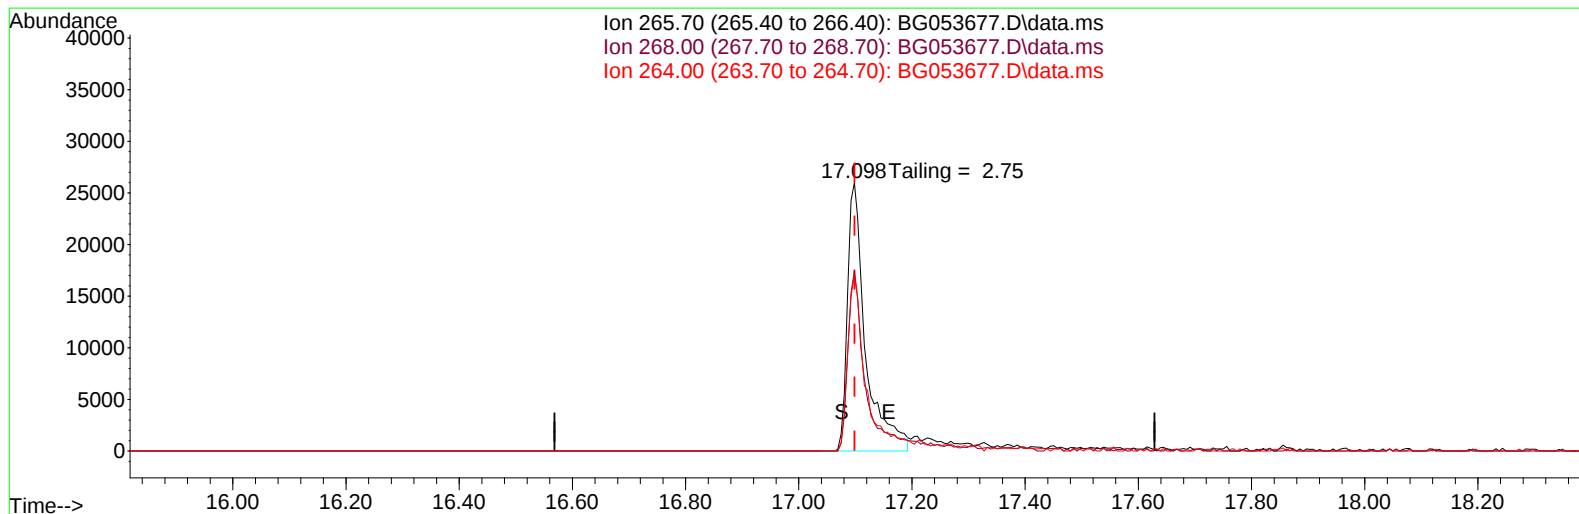

TIC: BG053677.D\data.ms




(70) Pentachlorophenol (C)

17.098min (-0.000) 22177.95 ng

response 58539

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.11
264.00	66.20	66.03
0.00	0.00	0.00

Quant Time: May 24 15:08:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 24 05:05:32 2022
Response via : Initial Calibration

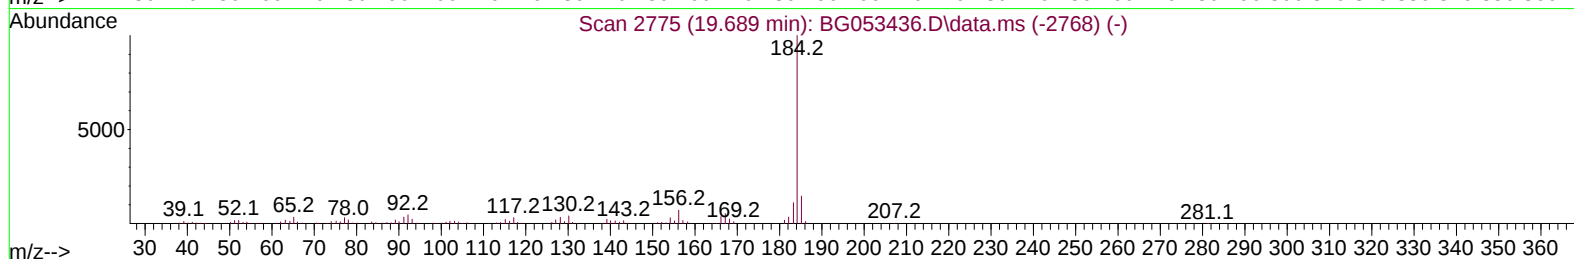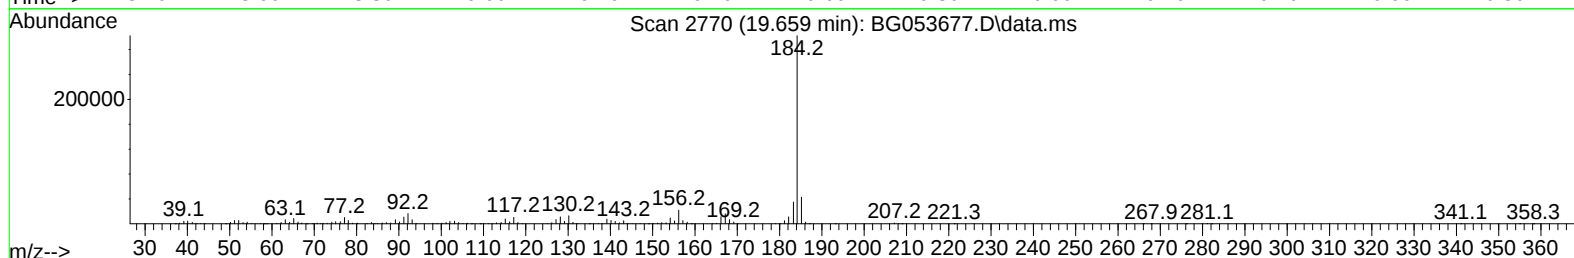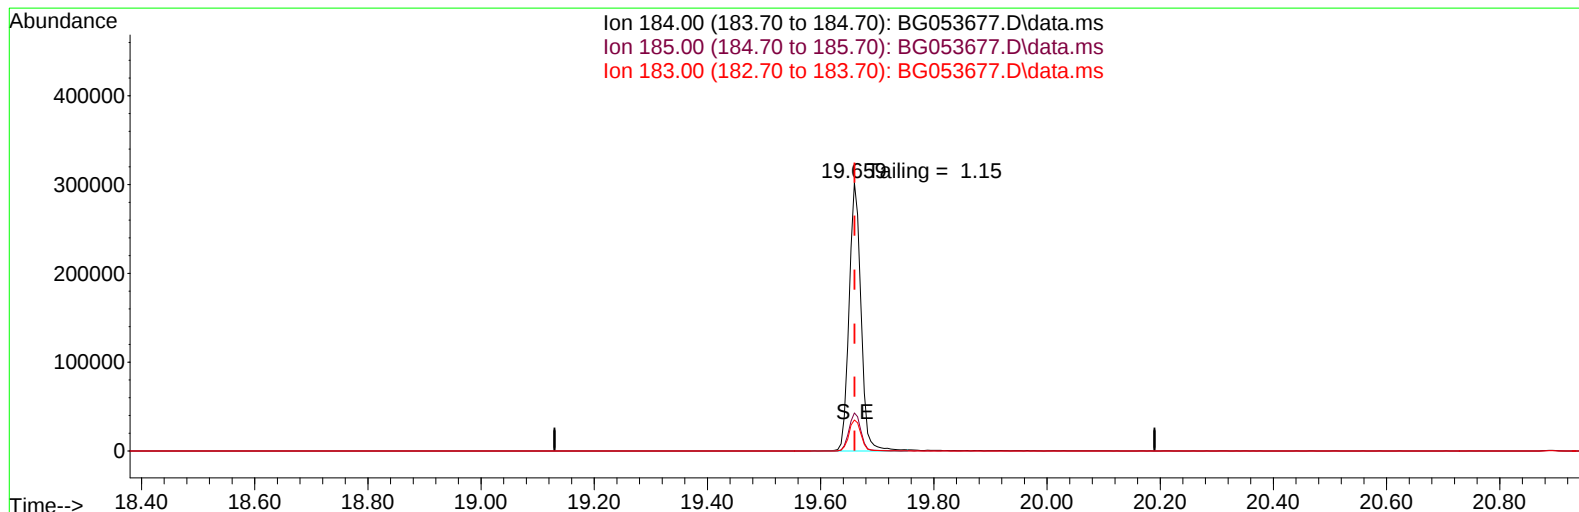

TIC: BG053677.D\data.ms

(77) Benzidine

19.659min (-0.000) 0.00 ng

response 444568

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.18
183.00	11.10	11.59
0.00	0.00	0.00