

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
 Data File : BG053680.D
 Acq On : 24 May 2022 11:29
 Operator : CG/JU
 Sample : N2968-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-31

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.634	376	382	389	rVV	132706	228870	10.23%	2.770%
2	5.710	389	395	400	rVB3	12291	25321	1.13%	0.306%
3	7.232	648	654	667	rBV	108496	204379	9.14%	2.474%
4	8.060	785	795	801	rBV	76090	135067	6.04%	1.635%
5	8.430	852	858	865	rBV	59182	104969	4.69%	1.270%
6	9.164	975	983	986	rBV2	14138	23268	1.04%	0.282%
7	9.223	986	993	1003	rVB	321512	618187	27.64%	7.482%
8	10.269	1164	1171	1179	rVB3	25601	46711	2.09%	0.565%
9	10.868	1266	1273	1279	rBV	112377	208529	9.32%	2.524%
10	10.921	1279	1282	1288	rVB	21043	33641	1.50%	0.407%
11	11.978	1455	1462	1469	rBV7	9805	23648	1.06%	0.286%
12	12.736	1583	1591	1596	rBV2	42959	83530	3.73%	1.011%
13	13.312	1681	1689	1695	rBV	909671	1427184	63.81%	17.273%
14	14.011	1800	1808	1813	rBV8	14175	35948	1.61%	0.435%
15	14.686	1916	1923	1931	rBV	201591	335616	15.01%	4.062%
16	15.861	2116	2123	2127	rBV7	17742	43691	1.95%	0.529%
17	16.178	2171	2177	2187	rBV	588017	902881	40.37%	10.927%
18	17.435	2385	2391	2398	rVB	267897	417325	18.66%	5.051%
19	18.317	2538	2541	2549	rBV4	46508	87710	3.92%	1.062%
20	19.585	2753	2757	2762	rBV7	30250	53157	2.38%	0.643%
21	20.038	2828	2834	2841	rVB	1736535	2236556	100.00%	27.068%
22	21.330	3050	3054	3060	rBV7	21960	36518	1.63%	0.442%
23	21.712	3112	3119	3129	rVB	288527	487101	21.78%	5.895%
24	24.972	3664	3674	3686	rVB2	156092	462924	20.70%	5.603%




Sum of corrected areas: 8262731

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
Data File : BG053680.D
Acq On : 24 May 2022 11:29
Operator : CG/JU
Sample : N2968-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-31

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

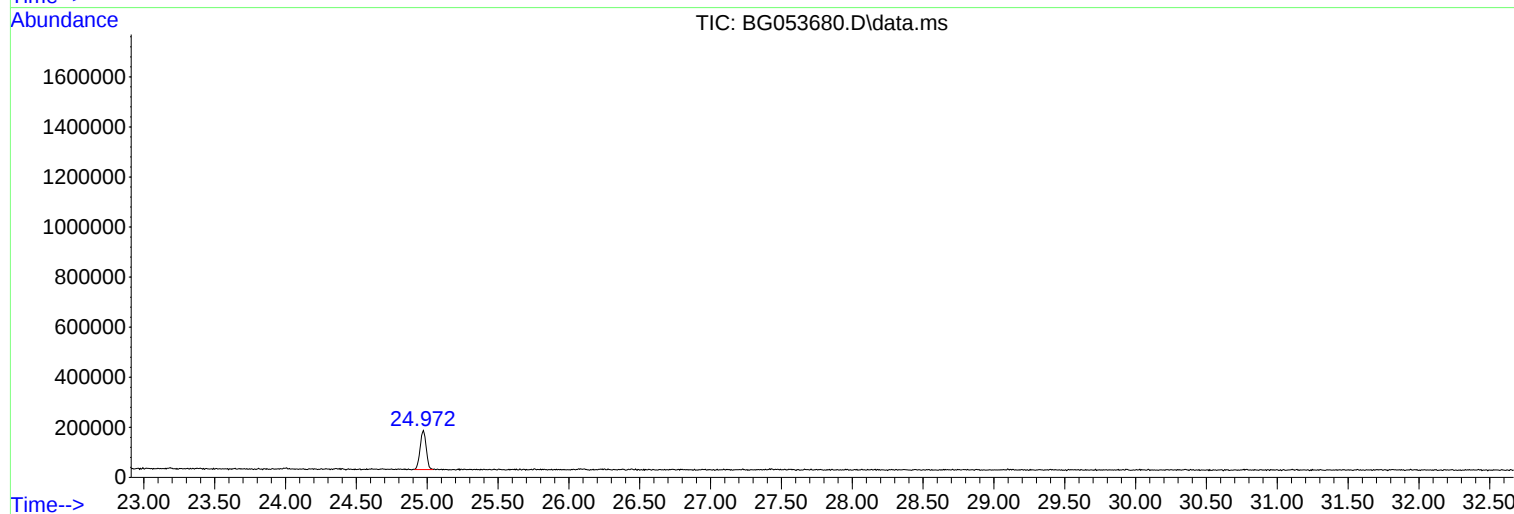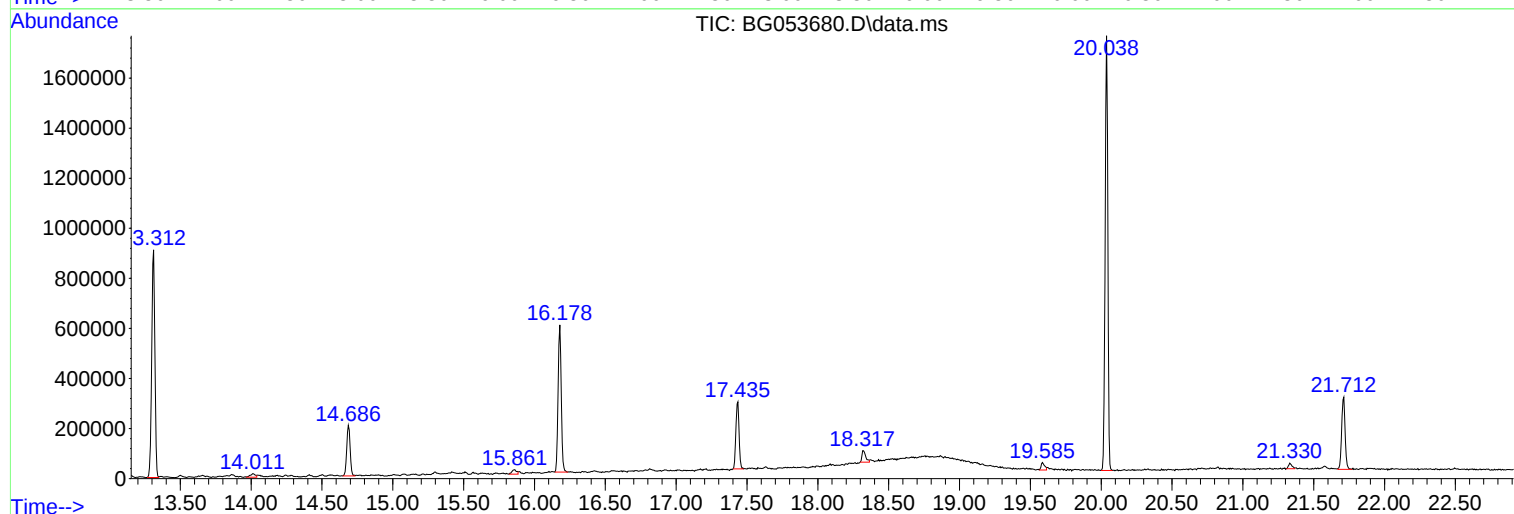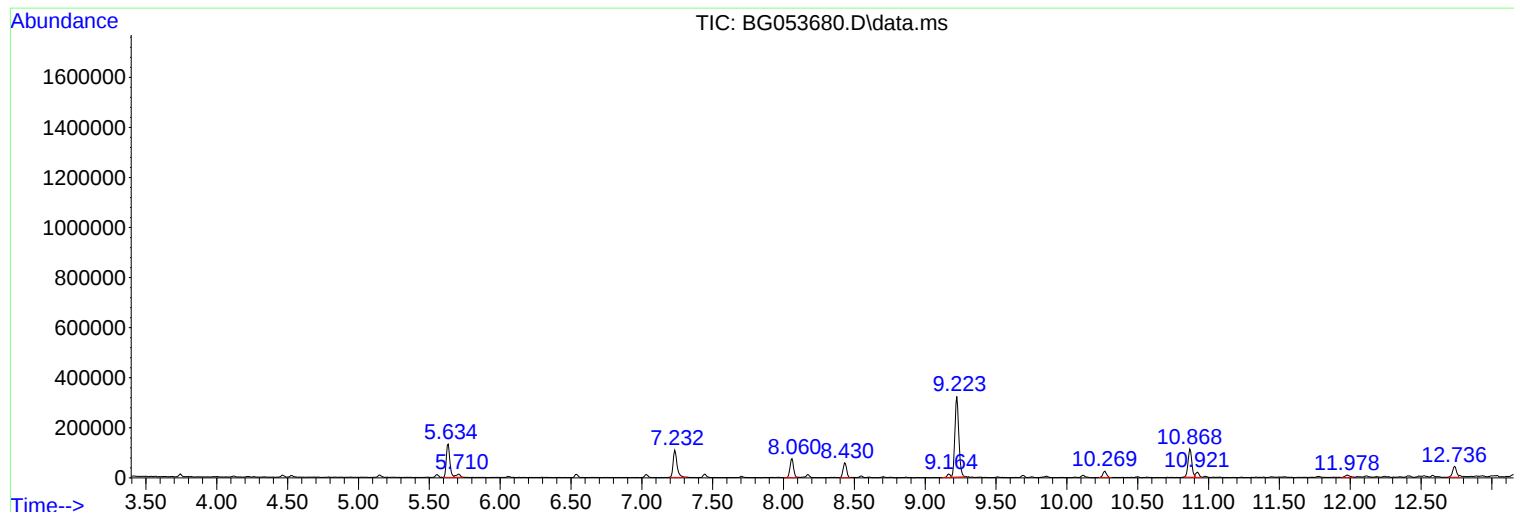

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
Data File : BG053680.D
Acq On : 24 May 2022 11:29
Operator : CG/JU
Sample : N2968-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-31

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
Data File : BG053680.D
Acq On : 24 May 2022 11:29
Operator : CG/JU
Sample : N2968-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-31

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------