

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
 Data File : BG053687.D
 Acq On : 24 May 2022 18:05
 Operator : CG/JU
 Sample : N3002-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-06

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.626	376	381	398	rBV	284975	502490	18.64%	4.788%
2	7.229	648	654	667	rBV	185388	349384	12.96%	3.329%
3	8.058	789	795	804	rBV	102023	174239	6.46%	1.660%
4	8.434	854	859	866	rVB2	19429	33162	1.23%	0.316%
5	9.221	987	993	1007	rVB	447956	839749	31.15%	8.002%
6	10.866	1264	1273	1287	rBV	145996	274109	10.17%	2.612%
7	13.309	1681	1689	1701	rBV	1274015	1927605	71.51%	18.367%
8	14.684	1915	1923	1930	rBV	266737	411114	15.25%	3.917%
9	16.176	2171	2177	2191	rBV	971644	1555641	57.71%	14.823%
10	17.433	2383	2391	2398	rBV	351921	526538	19.53%	5.017%
11	18.326	2538	2543	2550	rBV5	20997	48410	1.80%	0.461%
12	20.036	2828	2834	2840	rBV	2090763	2695409	100.00%	25.684%
13	21.328	3050	3054	3064	rBV6	30987	59500	2.21%	0.567%
14	21.710	3112	3119	3127	rVB2	326027	554545	20.57%	5.284%
15	24.970	3665	3674	3688	rVB2	188806	542812	20.14%	5.172%




Sum of corrected areas: 10494707

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
Data File : BG053687.D
Acq On : 24 May 2022 18:05
Operator : CG/JU
Sample : N3002-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

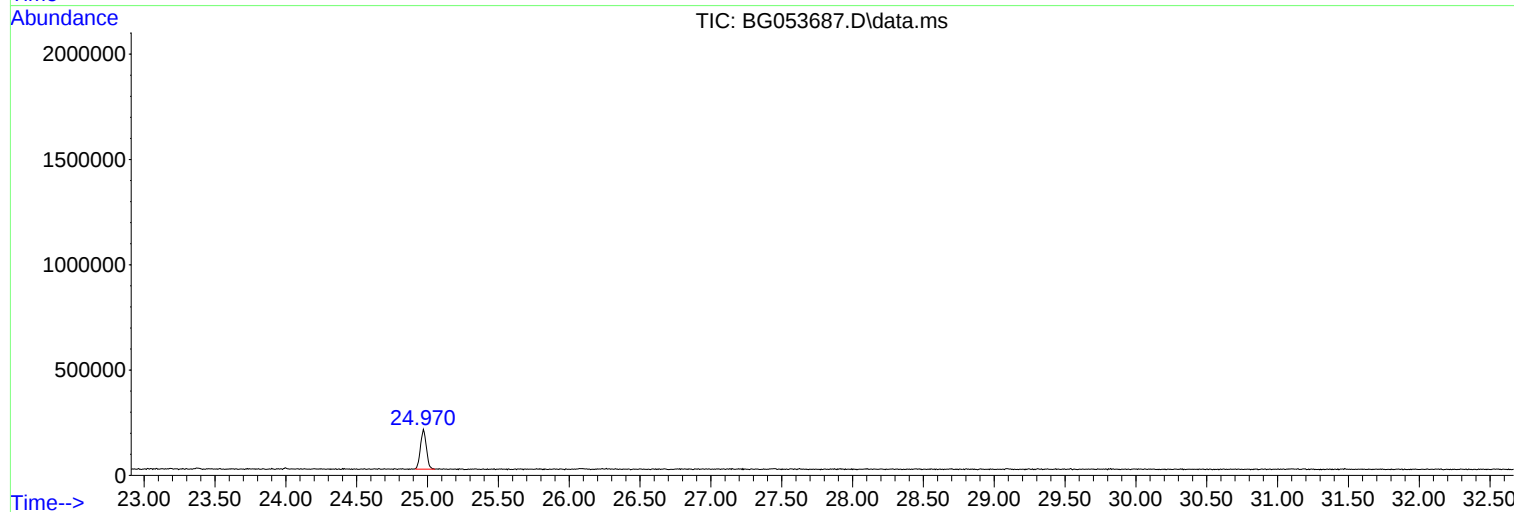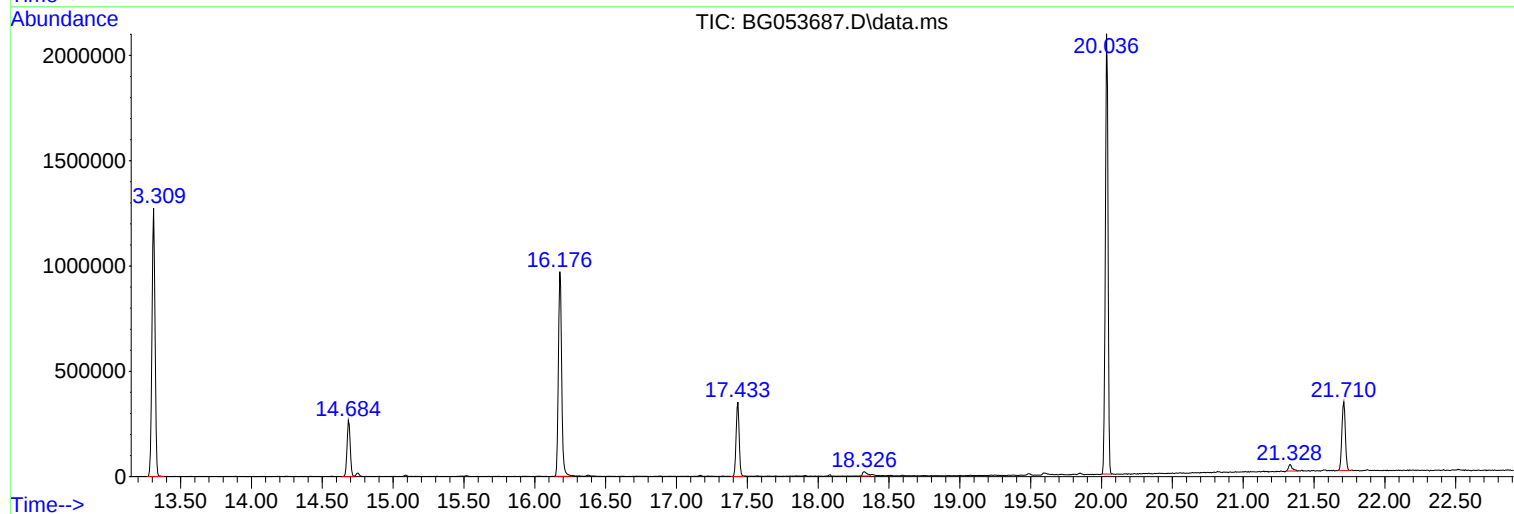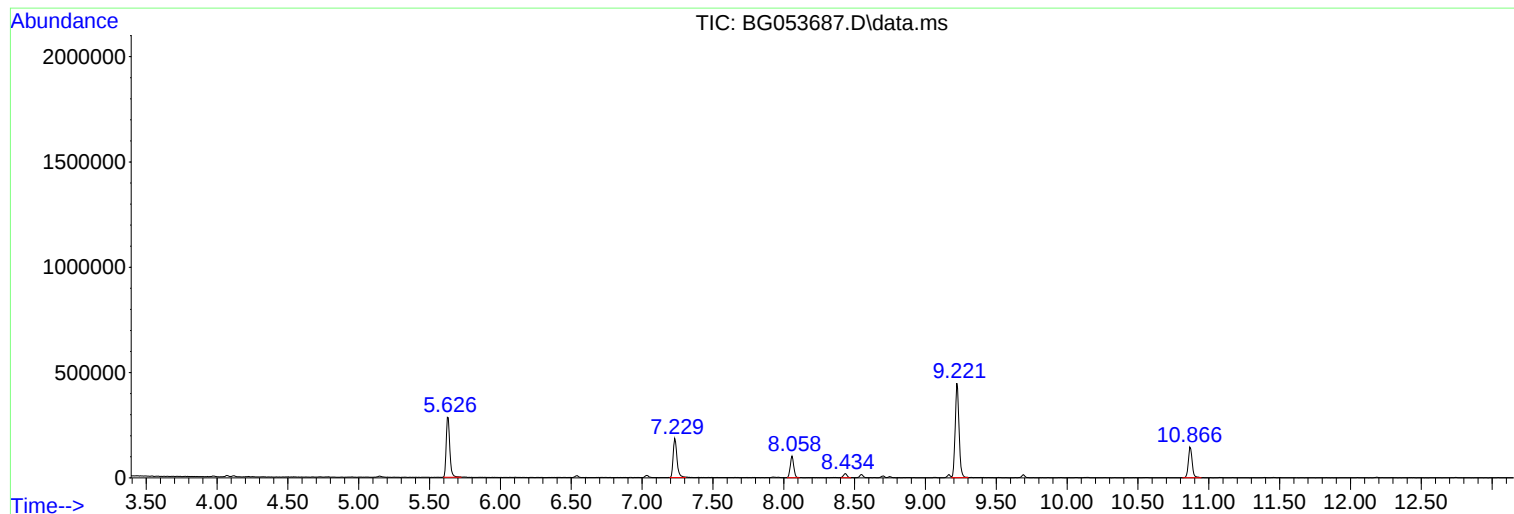

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
Data File : BG053687.D
Acq On : 24 May 2022 18:05
Operator : CG/JU
Sample : N3002-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
Data File : BG053687.D
Acq On : 24 May 2022 18:05
Operator : CG/JU
Sample : N3002-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc