

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
 Data File : BG053689.D
 Acq On : 24 May 2022 19:24
 Operator : CG/JU
 Sample : N3002-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.221	135	142	157	rBV	374755	697213	2.43%	0.457%
2	5.561	361	370	379	rBV	3881063	7547611	26.27%	4.950%
3	5.649	379	385	387	rVV	236711	376337	1.31%	0.247%
4	5.719	387	397	405	rVB	9259751	28734577	100.00%	18.844%
5	6.083	447	459	465	rBV	7895933	15759880	54.85%	10.335%
6	6.542	530	537	547	rBV	331880	557707	1.94%	0.366%
7	7.035	614	621	629	rBV	547942	919684	3.20%	0.603%
8	7.153	631	641	646	rVV	4127119	7622474	26.53%	4.999%
9	7.211	646	651	658	rVV	2355740	3965865	13.80%	2.601%
10	7.288	658	664	675	rVB	2461459	4196942	14.61%	2.752%
11	7.452	682	692	700	rBV	2528325	4337673	15.10%	2.845%
12	7.734	728	740	746	rVB	7264119	15229160	53.00%	9.987%
13	8.187	808	817	823	rBV	3074652	5388735	18.75%	3.534%
14	8.445	853	861	868	rVB	2587811	4615127	16.06%	3.027%
15	8.551	869	879	883	rBV	378554	634318	2.21%	0.416%
16	8.604	883	888	896	rVB2	876337	1517451	5.28%	0.995%
17	8.698	897	904	910	rBV	1011976	1717867	5.98%	1.127%
18	8.868	922	933	941	rBV3	269289	620105	2.16%	0.407%
19	9.015	952	958	963	rVV	583029	969077	3.37%	0.636%
20	9.068	963	967	978	rVV	520578	1055944	3.67%	0.692%
21	9.173	978	985	990	rVV	1188064	2275583	7.92%	1.492%
22	9.250	990	998	1009	rVB3	742502	1990598	6.93%	1.305%
23	9.502	1033	1041	1047	rBV	316396	576650	2.01%	0.378%
24	9.696	1067	1074	1079	rBV	566804	979188	3.41%	0.642%
25	9.755	1079	1084	1090	rVV	795509	1296854	4.51%	0.850%
26	9.843	1091	1099	1107	rVV4	146970	346697	1.21%	0.227%
27	9.919	1107	1112	1129	rVV7	134486	539378	1.88%	0.354%
28	10.055	1129	1135	1140	rVV3	274050	689212	2.40%	0.452%
29	10.113	1141	1145	1158	rVB	695975	1285356	4.47%	0.843%
30	10.272	1164	1172	1184	rBV2	1359107	2928745	10.19%	1.921%
31	10.366	1184	1188	1198	rVV4	141165	395732	1.38%	0.260%
32	10.507	1206	1212	1218	rVB3	194691	402185	1.40%	0.264%
33	10.754	1248	1254	1258	rBV	191303	332419	1.16%	0.218%
34	10.859	1264	1272	1277	rBV4	168380	437986	1.52%	0.287%
35	10.936	1277	1285	1291	rVB	3039039	6046353	21.04%	3.965%
36	11.041	1297	1303	1308	rVB	254832	447934	1.56%	0.294%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
 Data File : BG053689.D
 Acq On : 24 May 2022 19:24
 Operator : CG/JU
 Sample : N3002-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.782	1423	1429	1435	rVB2	144763	310917	1.08%	0.204%
38	11.976	1459	1462	1471	rVB7	150396	362507	1.26%	0.238%
39	12.252	1502	1509	1516	rVB	758874	1430771	4.98%	0.938%
40	12.522	1548	1555	1561	rVV	945942	1879631	6.54%	1.233%
41	12.581	1561	1565	1570	rVB	248462	418737	1.46%	0.275%
42	12.739	1583	1592	1598	rBV	934912	1689809	5.88%	1.108%
43	12.845	1598	1610	1615	rVV6	270567	1116243	3.88%	0.732%
44	12.921	1615	1623	1630	rVV2	411980	1575516	5.48%	1.033%
45	13.004	1631	1637	1649	rVV3	462972	1210712	4.21%	0.794%
46	13.150	1658	1662	1666	rVV	247766	499206	1.74%	0.327%
47	13.215	1666	1673	1681	rVV3	589839	1481793	5.16%	0.972%
48	13.309	1684	1689	1696	rVB	1007314	1596090	5.55%	1.047%
49	13.614	1729	1741	1745	rVV3	232343	722980	2.52%	0.474%
50	13.797	1763	1772	1780	rBV2	586805	1791416	6.23%	1.175%
51	13.861	1780	1783	1789	rVV2	207526	350986	1.22%	0.230%
52	13.926	1789	1794	1798	rVV4	164415	329130	1.15%	0.216%
53	13.990	1801	1805	1809	rVV2	194058	408073	1.42%	0.268%
54	14.037	1809	1813	1817	rVB	233936	355858	1.24%	0.233%
55	14.255	1846	1850	1861	rVB2	169695	437794	1.52%	0.287%
56	14.408	1870	1876	1882	rBV	326688	613675	2.14%	0.402%
57	14.689	1917	1924	1929	rBV2	326632	583204	2.03%	0.382%
58	15.248	2014	2019	2027	rBV	191448	368792	1.28%	0.242%
59	16.182	2172	2178	2187	rBV	807419	1290063	4.49%	0.846%
60	17.433	2385	2391	2399	rBV	301425	440661	1.53%	0.289%
61	18.320	2537	2542	2548	rBV3	184563	312125	1.09%	0.205%
62	20.035	2828	2834	2844	rVB	1791179	2442283	8.50%	1.602%
63	21.709	3113	3119	3127	rVB2	316947	514503	1.79%	0.337%
64	24.970	3664	3674	3685	rVB3	172381	520099	1.81%	0.341%




Sum of corrected areas: 152488191

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
Data File : BG053689.D
Acq On : 24 May 2022 19:24
Operator : CG/JU
Sample : N3002-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

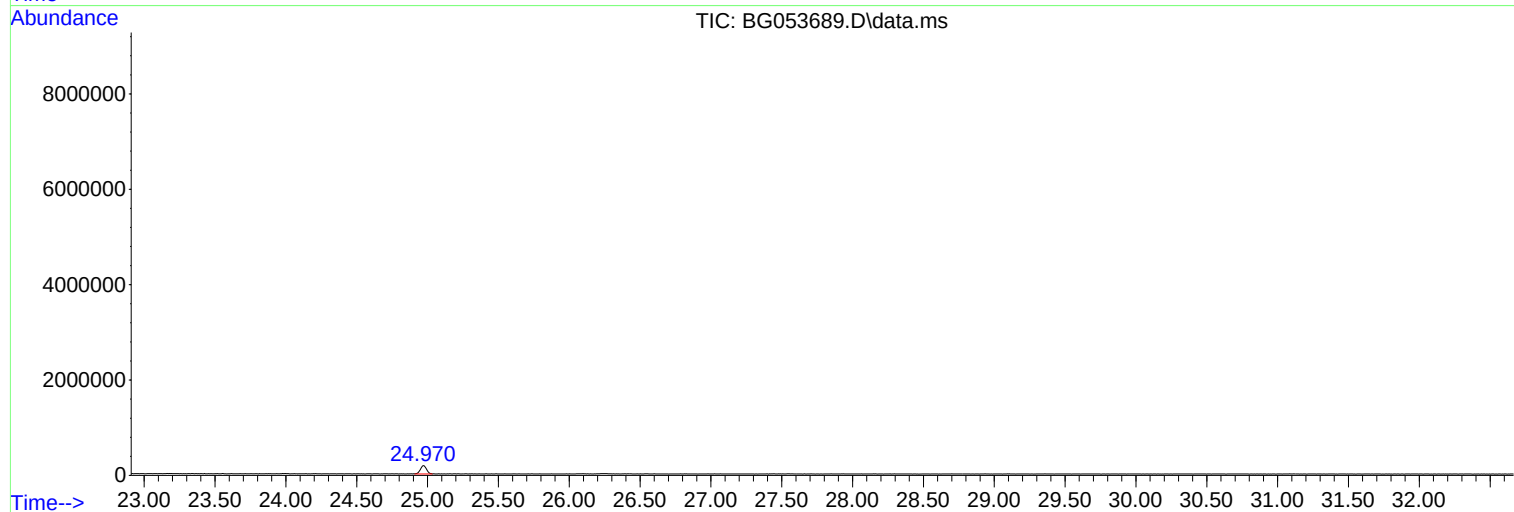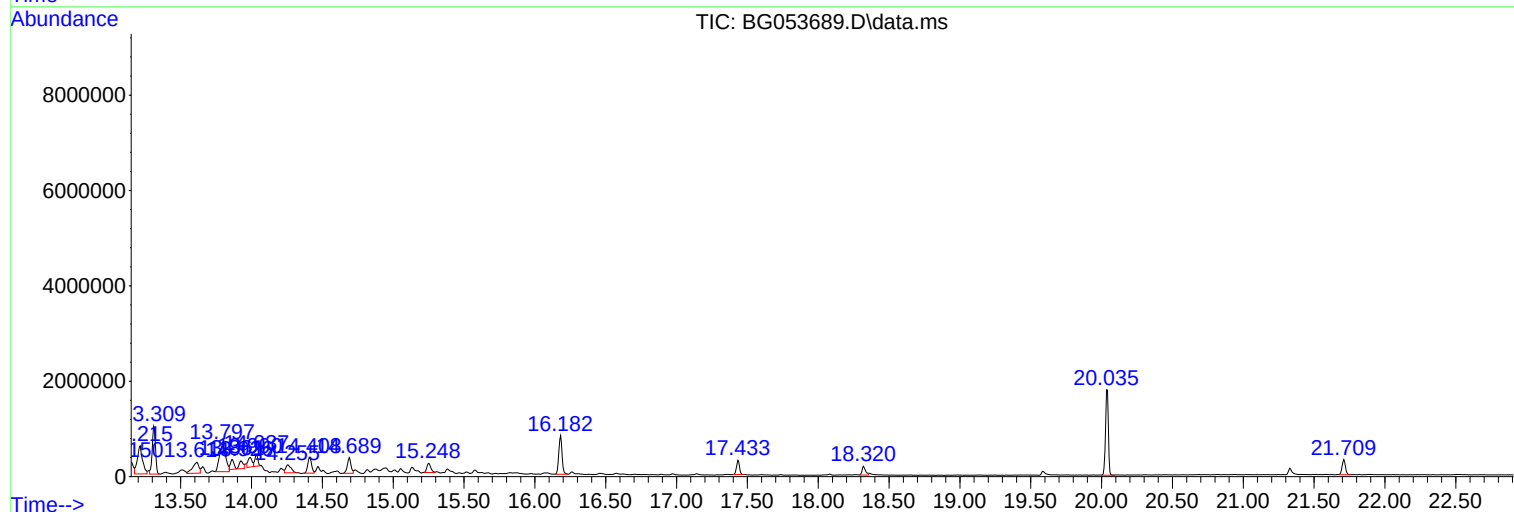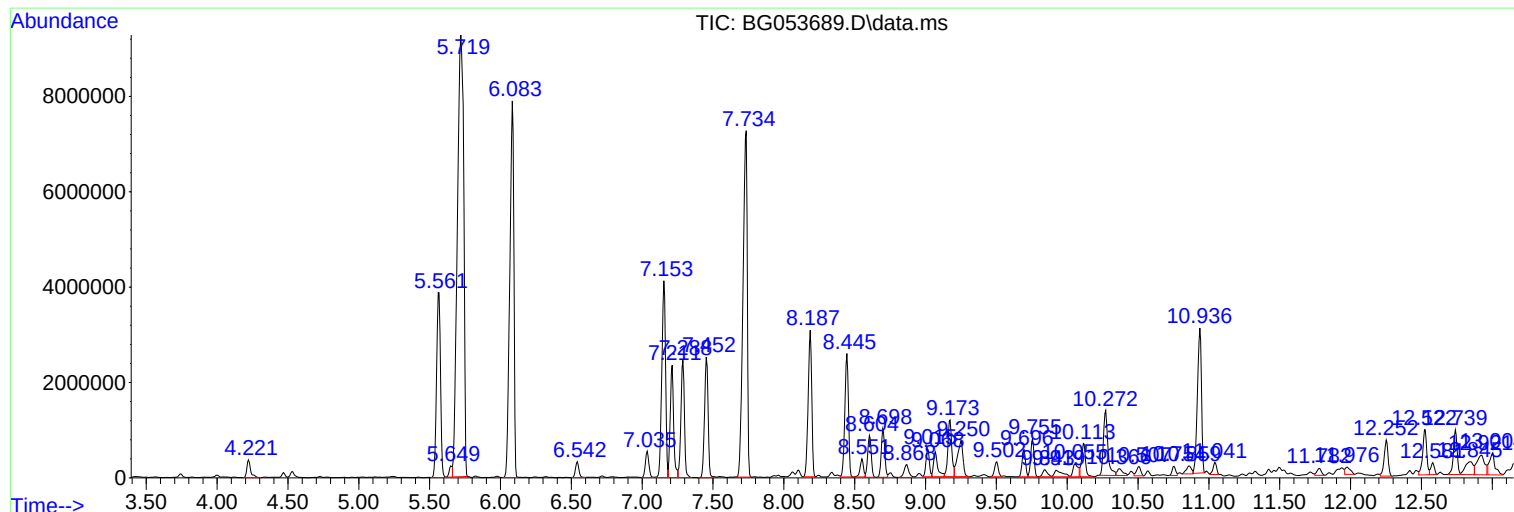

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
Data File : BG053689.D
Acq On : 24 May 2022 19:24
Operator : CG/JU
Sample : N3002-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052422\
Data File : BG053689.D
Acq On : 24 May 2022 19:24
Operator : CG/JU
Sample : N3002-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc