


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052422\  
 Data File : BG053677.D  
 Acq On : 24 May 2022 9:22  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG050522.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed May 25 15:11:41 2022

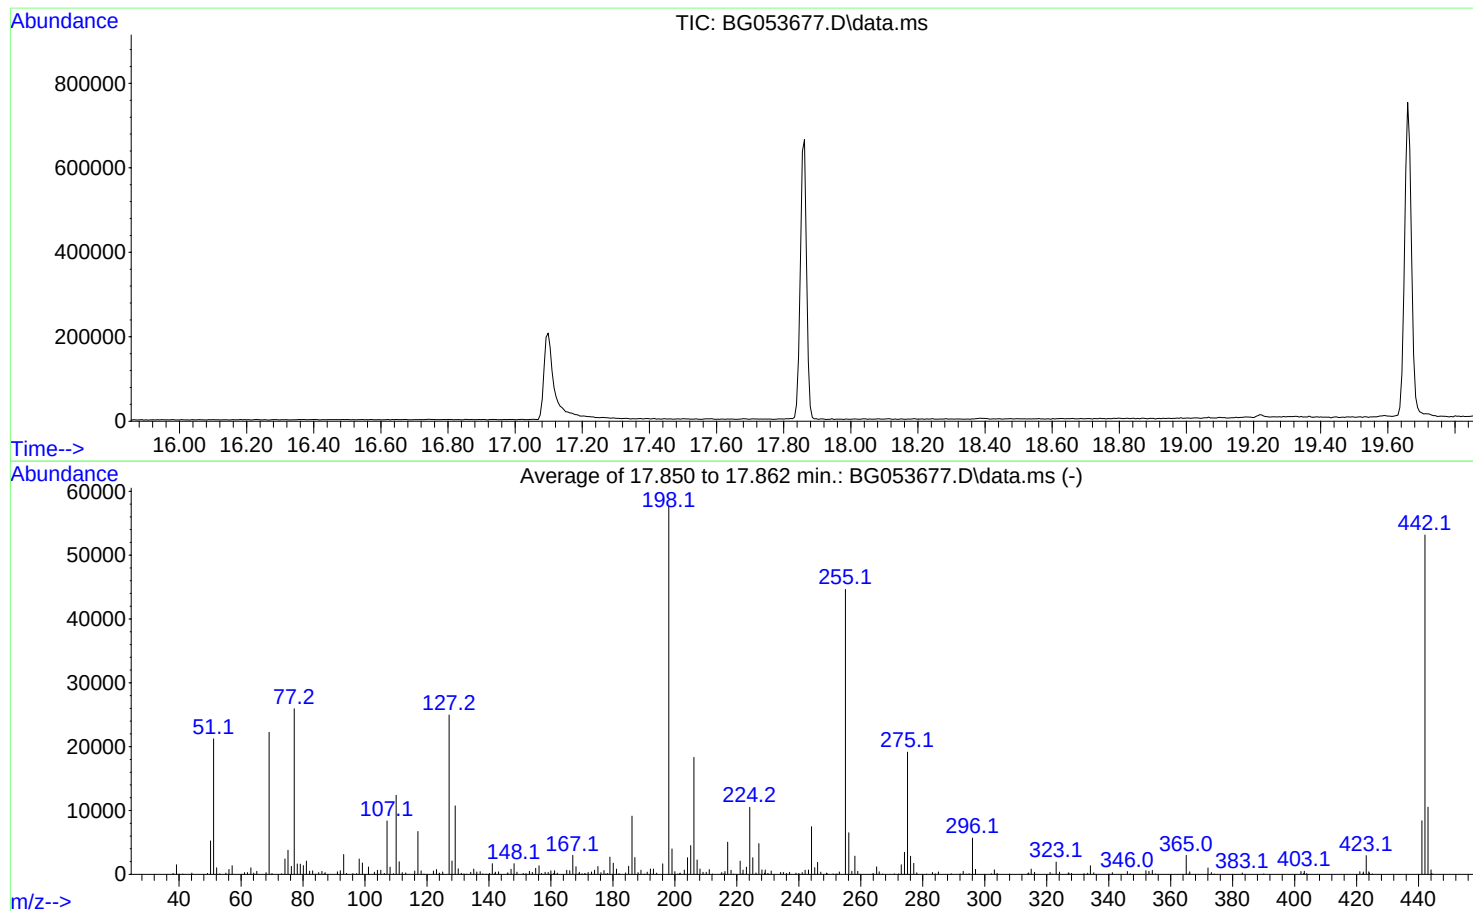




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.8         | 21219      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.2          | 268        | PASS                |
| 69             | 198             | 0.00            | 100             | 38.6         | 22264      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 133        | PASS                |
| 127            | 198             | 10              | 80              | 43.3         | 24968      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 57619      | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 3979       | PASS                |
| 275            | 198             | 10              | 60              | 33.2         | 19149      | PASS                |
| 365            | 198             | 1               | 100             | 5.2          | 2982       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.6         | 8400       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 53160      | PASS                |
| 443            | 442             | 15              | 24              | 19.8         | 10518      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052422\  
Data File : BG053677.D  
Acq On : 24 May 2022 9:22  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: May 24 15:08:11 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG050522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 24 05:05:32 2022  
Response via : Initial Calibration

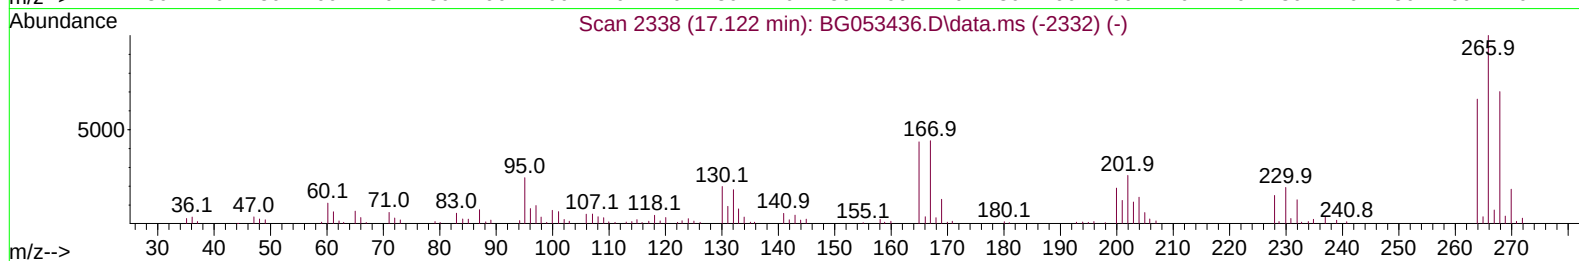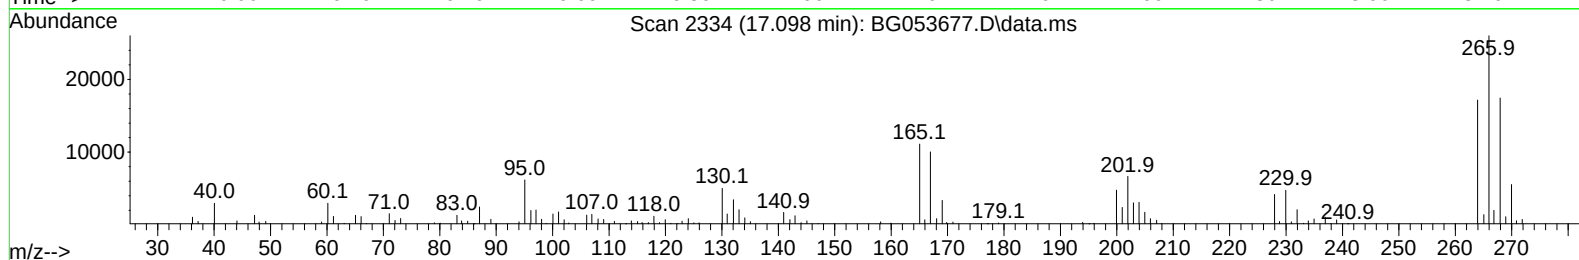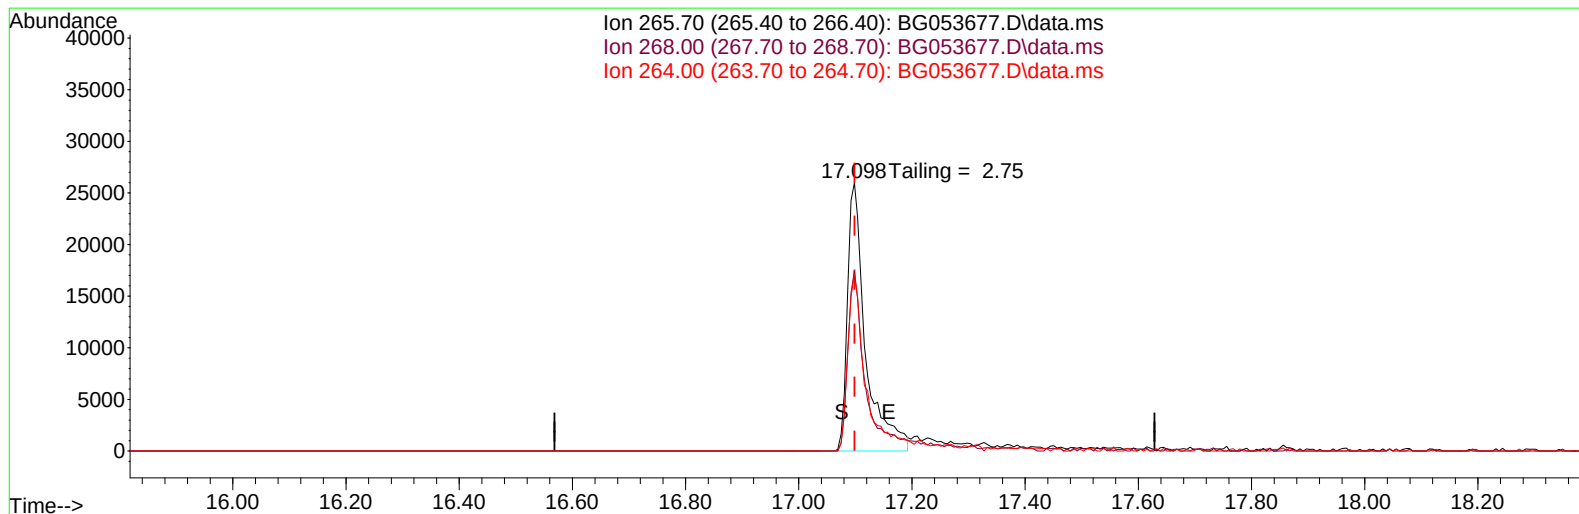

TIC: BG053677.D\data.ms

**(70) Pentachlorophenol (C)**

17.098min (-0.000) 22177.95 ng




response 58539

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 70.20  | 67.11  |
| 264.00 | 66.20  | 66.03  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052422\  
Data File : BG053677.D  
Acq On : 24 May 2022 9:22  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: May 24 15:08:11 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG050522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 24 05:05:32 2022  
Response via : Initial Calibration

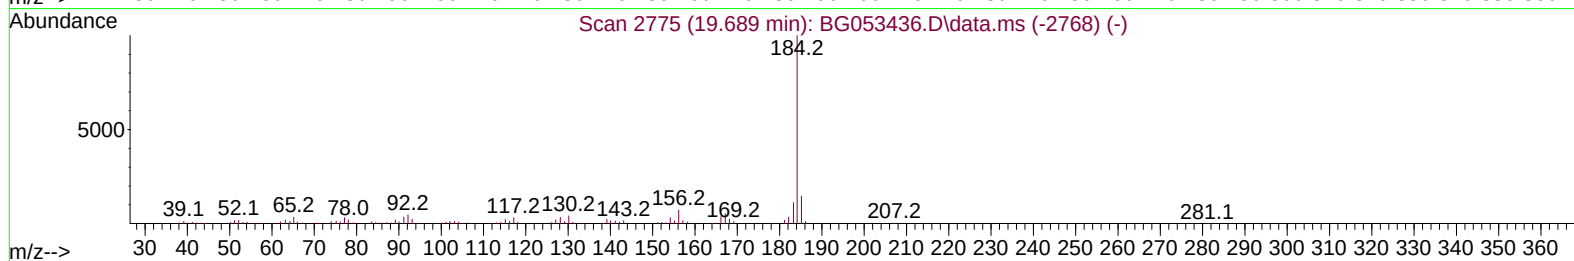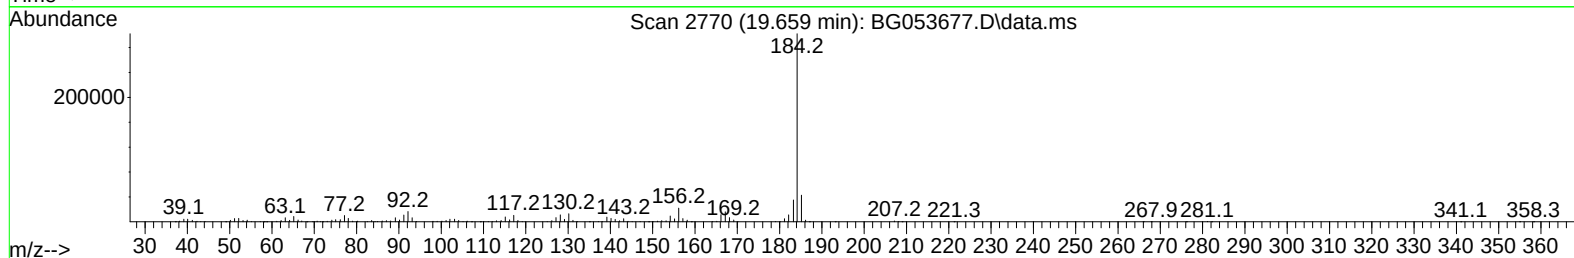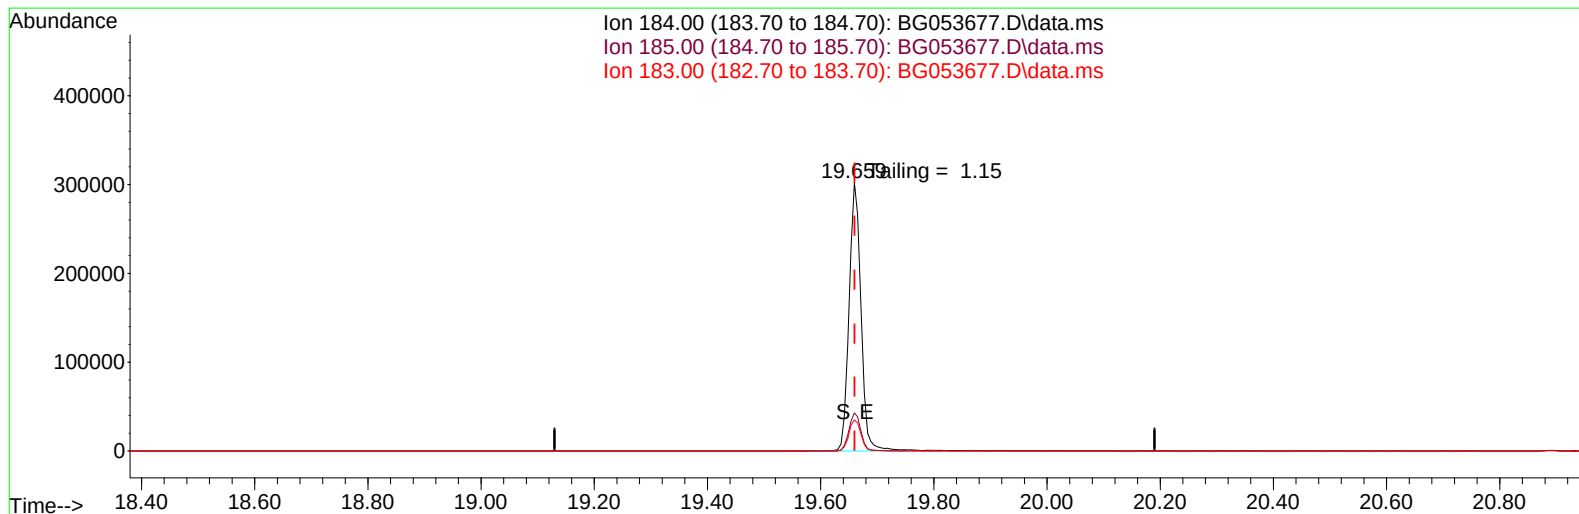

TIC: BG053677.D\data.ms

**(77) Benzidine**

**19.659min (-0.000) 0.00 ng**

**response 444568**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 14.18  |
| 183.00 | 11.10  | 11.59  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/24/2022     | BNA_G            | <u>BG053677.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 235448           | 20.89              |
| DDD           | 1498             | 20.45              |
| DDE           | 785              | 19.95              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 2283          | 237731           | 0.96               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP