

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052424\
 Data File : BG061280.D
 Acq On : 24 May 2024 8:18
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020495

Quant Time: May 24 23:46:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 15:23:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.888	152	20279	20.000	ng/ul	0.00
20) Naphthalene-d8	10.679	136	93736	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.521	164	80748	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.265	188	202909	20.000	ng/ul	0.00
79) Chrysene-d12	21.519	240	210306	20.000	ng/ul	0.00
88) Perylene-d12	24.604	264	235871	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.335	96	3238	8.936	ng/uL	0.00
4) Pyridine-d5	3.746	84	25185	19.536	ng/ul	0.00
7) Phenol-d5	7.065	99	29788	17.887	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.212	67	18889	18.046	ng/ul	0.00
11) 2-Chlorophenol-d4	7.418	132	22745	18.455	ng/ul	0.00
15) 4-Methylphenol-d8	8.599	113	26338	18.548	ng/ul	0.00
21) Nitrobenzene-d5	9.046	128	13587	18.826	ng/ul	0.00
24) 2-Nitrophenol-d4	9.762	143	14748	17.461	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.309	165	30277	18.387	ng/ul	0.00
31) 4-Chloroaniline-d4	10.814	131	39372	18.276	ng/ul	0.00
46) Dimethylphthalate-d6	13.922	166	111885	17.865	ng/ul	0.00
49) Acenaphthylene-d8	14.210	160	120681	18.535	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	13602	17.568	ng/ul	0.00
60) Fluorene-d10	15.514	176	98352	18.190	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.644	200	20182	16.445	ng/ul	0.00
73) Anthracene-d10	17.365	188	167072	18.676	ng/ul	0.00
81) Pyrene-d10	19.657	212	197613	18.300	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.392	264	205468	18.119	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.370	88	3407	7.833	ng/uL	99
5) Pyridine	3.763	79	24828	19.472	ng/ul	93
6) Benzaldehyde	7.024	77	17625	20.241	ng/ul	92
8) Phenol	7.089	94	30802	18.153	ng/ul	88
10) Bis(2-Chloroethyl)ether	7.306	93	23606	19.020	ng/ul	95
12) 2-Chlorophenol	7.453	128	24214	18.590	ng/ul	92
13) 2-Methylphenol	8.335	108	24286	18.468	ng/ul	93
14) 2,2'-oxybis(1-Chloropr...	8.411	45	61598	18.377	ng/ul#	97
16) Acetophenone	8.699	105	46873	19.341	ng/ul	89
17) N-Nitroso-di-n-propyla...	8.687	70	24294	18.232	ng/ul	89
18) 4-Methylphenol	8.664	108	28513	19.570	ng/ul	96
19) Hexachloroethane	8.963	117	11119	19.186	ng/ul	92
22) Nitrobenzene	9.081	77	35327	17.847	ng/ul#	95
23) Isophorone	9.604	82	69848	17.347	ng/ul	98
25) 2-Nitrophenol	9.798	139	16417	17.907	ng/ul	98
26) 2,4-Dimethylphenol	9.862	107	33139	18.243	ng/ul	95
27) Bis(2-Chloroethoxy)met...	10.091	93	37151	18.406	ng/ul#	95
29) 2,4-Dichlorophenol	10.338	162	27325	18.017	ng/ul#	93
30) Naphthalene	10.732	128	91227	18.439	ng/ul	100
32) 4-Chloroaniline	10.838	127	38862	18.153	ng/ul	96
33) Hexachlorobutadiene	11.014	225	26148	17.639	ng/ul	95
34) Caprolactam	11.584	113	4758	8.200	ng/ul	95
35) 4-Chloro-3-methylphenol	11.977	107	34959	17.831	ng/ul	93
36) 2-Methylnaphthalene	12.342	142	66650	18.576	ng/ul	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052424\
 Data File : BG061280.D
 Acq On : 24 May 2024 8:18
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020495

Quant Time: May 24 23:46:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 15:23:39 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.559	142	66884	18.164	ng/ul#	94
39) 1,2,4,5-Tetrachloroben...	12.712	216	50514	18.948	ng/ul	96
40) Hexachlorocyclopentadiene	12.688	237	24643	20.479	ng/ul	95
41) 2,4,6-Trichlorophenol	12.959	196	26697	17.779	ng/ul	97
42) 2,4,5-Trichlorophenol	13.041	196	29096	18.400	ng/ul#	95
43) 1,1'-Biphenyl	13.352	154	97884	18.747	ng/ul	95
44) 2-Chloronaphthalene	13.393	162	77781	18.929	ng/ul	99
45) 2-Nitroaniline	13.599	65	30315	17.876	ng/ul	92
47) Dimethylphthalate	13.975	163	116518	17.851	ng/ul	99
48) 2,6-Dinitrotoluene	14.098	165	22212	17.353	ng/ul	99
50) Acenaphthylene	14.239	152	134171	18.584	ng/ul	98
51) 3-Nitroaniline	14.422	138	20677	18.613	ng/ul#	94
52) Acenaphthene	14.580	153	89196	18.833	ng/ul	98
53) 2,4-Dinitrophenol	14.645	184	10932	16.105	ng/ul	94
55) 4-Nitrophenol	14.756	109	14643	16.086	ng/ul	98
56) Dibenzofuran	14.921	168	125205	18.489	ng/ul	99
57) 2,4-Dinitrotoluene	14.892	165	35075	18.010	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.156	232	24722	17.141	ng/ul#	98
59) Diethylphthalate	15.338	149	114263	17.727	ng/ul	96
61) Fluorene	15.567	166	107623	18.368	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.561	204	63580	18.503	ng/ul	96
63) 4-Nitroaniline	15.591	138	21541	18.618	ng/ul	89
66) 4,6-Dinitro-2-methylph...	15.661	198	20510	15.947	ng/ul#	92
67) N-Nitrosodiphenylamine	15.779	169	95384	18.703	ng/ul	100
68) 4-Bromophenyl-phenylether	16.454	248	43777	18.208	ng/ul	94
69) Hexachlorobenzene	16.578	284	49967	18.698	ng/ul	99
70) Atrazine	16.725	200	37052	18.358	ng/ul	98
71) Pentachlorophenol	16.930	266	16388	17.620	ng/ul	90
72) Phenanthrene	17.306	178	185461	18.832	ng/ul	98
74) Anthracene	17.400	178	191161	18.773	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.317	216	50345	18.770	ng/ul	93
76) Pentachlorobenzene	14.845	250	54893	18.511	ng/ul	97
77) Carbazole	17.671	167	157213	18.982	ng/ul	98
78) Di-n-butylphthalate	18.235	149	192761	18.574	ng/ul	97
80) Fluoranthene	19.322	202	239849	18.516	ng/ul	99
82) Pyrene	19.686	202	249378	18.546	ng/ul	99
83) Butylbenzylphthalate	20.579	149	86701	18.770	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.413	252	88816	19.896	ng/ul	97
85) Benzo(a)anthracene	21.496	228	263422	18.153	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.413	149	125834	18.404	ng/ul	99
87) Chrysene	21.560	228	245175	18.349	ng/ul	99
89) Di-n-octyl phthalate	22.577	149	214722	18.196	ng/ul	100
90) Benzo(b)fluoranthene	23.628	252	257339	18.324	ng/ul	98
91) Benzo(k)fluoranthene	23.693	252	255349	17.911	ng/ul	96
93) Benzo(a)pyrene	24.457	252	242503	18.185	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.100	276	296985	18.416	ng/ul	95
95) Dibenzo(a,h)anthracene	28.147	278	239924	18.043	ng/ul	97
96) Benzo(g,h,i)perylene	29.187	276	233889	18.231	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052424\
Data File : BG061280.D
Acq On : 24 May 2024 8:18
Operator : MA/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD020495

Quant Time: May 24 23:46:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 21 15:23:39 2024
Response via : Initial Calibration

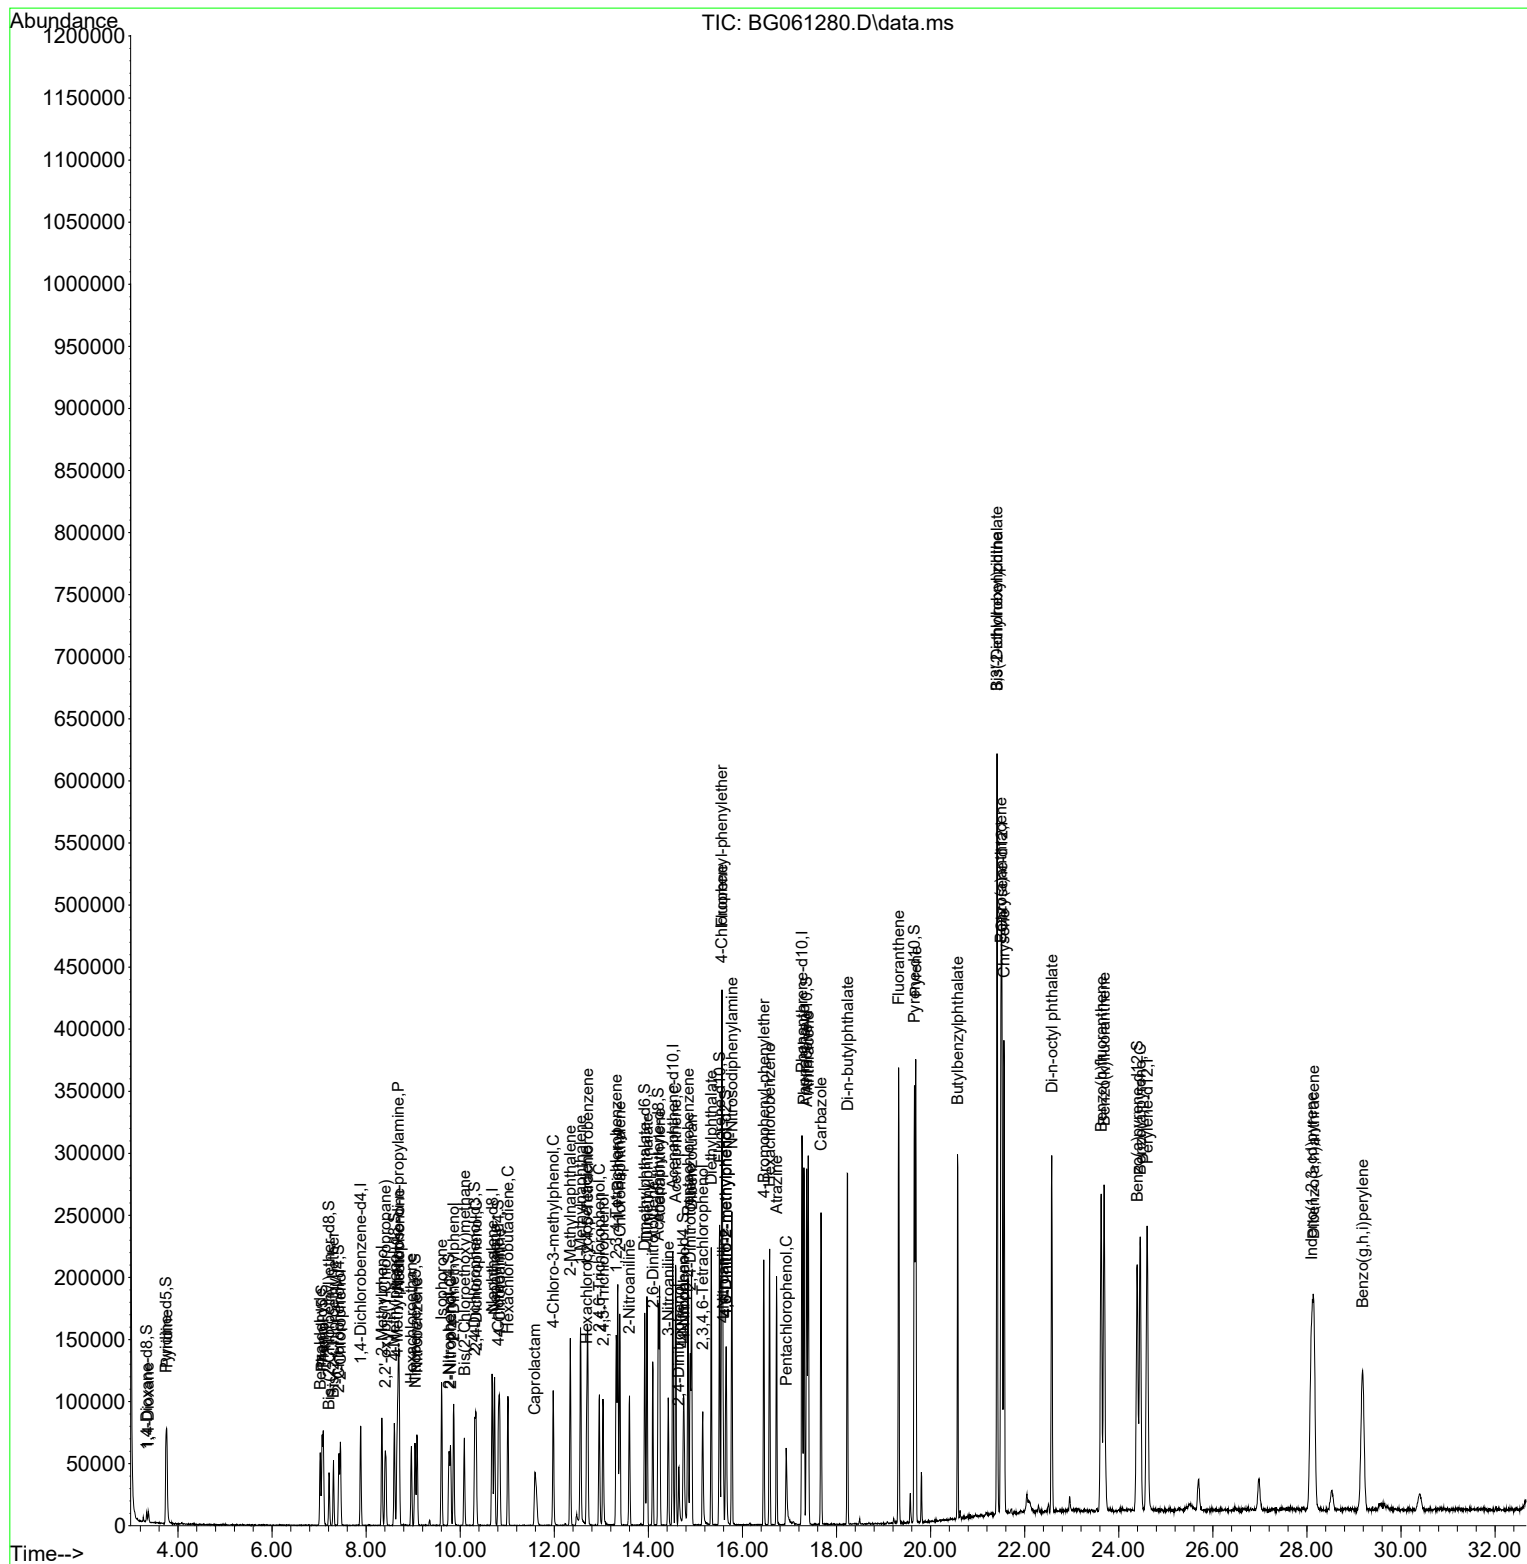



#2

1,4-Dioxane

Concen: 7.833 ng/uL

RT: 3.370 min Scan# 61

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion: 88 Resp: 3407

Ion Ratio Lower Upper

88 100

43 55.9 44.6 67.0

58 111.9 90.3 135.5

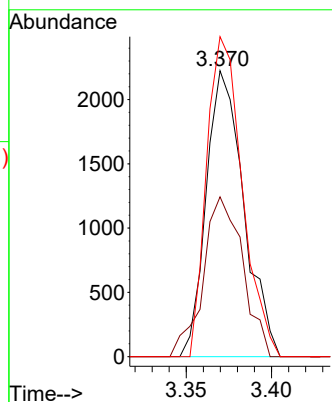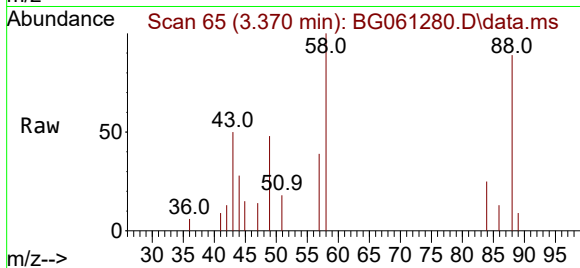

#5

Pyridine

Concen: 19.472 ng/uL

RT: 3.763 min Scan# 132

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion: 79 Resp: 24828


Ion Ratio Lower Upper

79 100

52 136.6 116.3 174.5

51 70.4 52.1 78.1




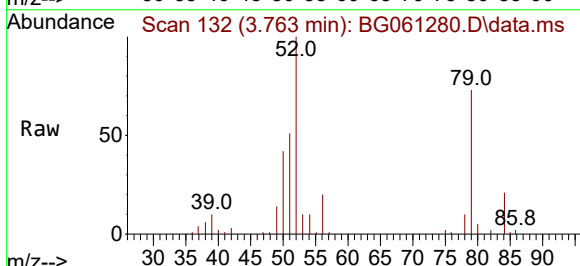




#6
Benzaldehyde
Concen: 20.241 ng/ul
RT: 7.024 min Scan# 687
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:	77	Resp:	17625
Ion	Ratio	Lower	Upper
77	100		
105	94.3	71.0	106.6
106	88.5	63.4	95.2

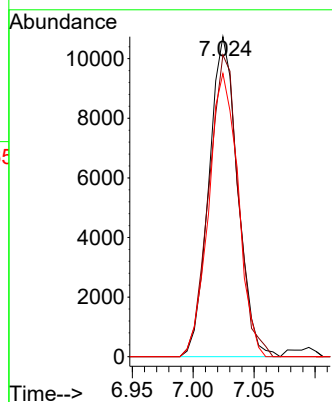

#8
Phenol
Concen: 18.153 ng/ul
RT: 7.089 min Scan# 698
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:	94	Resp:	30802
Ion	Ratio	Lower	Upper
94	100		
65	38.1	35.0	52.4
66	51.3	50.3	75.5

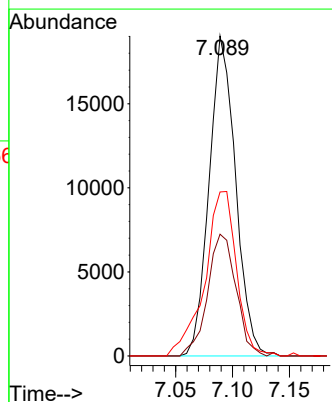







#10
 Bis(2-Chloroethyl)ether
 Concen: 19.020 ng/ul
 RT: 7.306 min Scan# 735
 Delta R.T. -0.001 min
 Lab File: BG061280.D
 Acq: 24 May 2024 8:18

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020495

Tgt Ion: 93 Resp: 23606




Ion	Ratio	Lower	Upper
93	100		
63	102.1	86.2	129.2
95	34.7	25.8	38.8




#12
 2-Chlorophenol
 Concen: 18.590 ng/ul
 RT: 7.453 min Scan# 760
 Delta R.T. -0.006 min
 Lab File: BG061280.D
 Acq: 24 May 2024 8:18

Tgt Ion:128 Resp: 24214

Ion	Ratio	Lower	Upper
128	100		
64	52.3	46.9	70.3
130	28.6	25.8	38.8





#13

2-Methylphenol

Concen: 18.468 ng/ul

RT: 8.335 min Scan# 910

Delta R.T. -0.006 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :





SSTD020495

Tgt Ion:108 Resp: 24286

Ion Ratio Lower Upper

108 100

107 93.3 69.5 104.3



#14

2,2'-oxybis(1-Chloropropane)

Concen: 18.377 ng/ul

RT: 8.411 min Scan# 923

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion: 45 Resp: 61598


Ion Ratio Lower Upper

45 100

77 9.3 6.2 9.2#

79 6.5 4.6 7.0









#16
Acetophenone
Concen: 19.341 ng/ul
RT: 8.699 min Scan# 91
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:105 Resp: 46873
Ion Ratio Lower Upper
105 100
77 74.8 70.4 105.6
51 44.6 38.4 57.6



#17
N-Nitroso-di-n-propylamine
Concen: 18.232 ng/ul
RT: 8.687 min Scan# 970
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion: 70 Resp: 24294
Ion Ratio Lower Upper
70 100
42 90.9 83.2 124.8
101 9.0 6.6 9.8
130 20.9 15.4 23.0









#18
4-Methylphenol
Concen: 19.570 ng/ul
RT: 8.664 min Scan# 90
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:108 Resp: 28513
Ion Ratio Lower Upper
108 100
107 107.5 89.3 133.9



#19
Hexachloroethane
Concen: 19.186 ng/ul
RT: 8.963 min Scan# 1017
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:117 Resp: 11119
Ion Ratio Lower Upper
117 100
201 132.9 110.8 166.2
199 70.1 65.1 97.7









#22
Nitrobenzene
Concen: 17.847 ng/ul
RT: 9.081 min Scan# 1037
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion: 77 Resp: 35327
Ion Ratio Lower Upper
77 100
123 39.1 32.7 49.1
65 13.4 14.2 21.2#



#23
Isophorone
Concen: 17.347 ng/ul
RT: 9.604 min Scan# 1126
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion: 82 Resp: 69848
Ion Ratio Lower Upper
82 100
95 8.2 6.9 10.3
138 16.0 13.5 20.3









#25
2-Nitrophenol
Concen: 17.907 ng/ul
RT: 9.798 min Scan# 1159
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:139 Resp: 16417
Ion Ratio Lower Upper
139 100
65 68.9 56.1 84.1
109 40.7 33.8 50.6



#26
2,4-Dimethylphenol
Concen: 18.243 ng/ul
RT: 9.862 min Scan# 1170
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:107 Resp: 33139
Ion Ratio Lower Upper
107 100
121 43.9 36.4 54.6
122 76.5 65.8 98.8





#27

Bis(2-Chloroethoxy)methane

Concen: 18.406 ng/ul

RT: 10.091 min Scan# 1209

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion: 93 Resp: 37151

Ion Ratio Lower Upper

93 100

95 29.6 25.8 38.8

123 10.8 7.2 10.8#



#29

2,4-Dichlorophenol

Concen: 18.017 ng/ul

RT: 10.338 min Scan# 1251

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion:162 Resp: 27325


Ion Ratio Lower Upper

162 100

164 69.4 58.4 87.6

98 29.4 29.9 44.9#



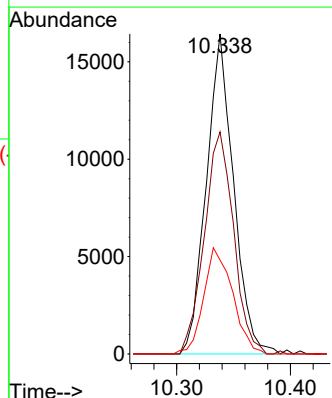





#30
Naphthalene
Concen: 18.439 ng/ul
RT: 10.732 min Scan# 1318
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:128 Resp: 91227
Ion Ratio Lower Upper
128 100
129 10.9 8.6 12.8
127 13.6 10.8 16.2



#32
4-Chloroaniline
Concen: 18.153 ng/ul
RT: 10.838 min Scan# 1336
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:127 Resp: 38862
Ion Ratio Lower Upper
127 100
129 30.3 25.9 38.9









#33
Hexachlorobutadiene
Concen: 17.639 ng/ul
RT: 11.014 min Scan# 11
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:225 Resp: 26148
Ion Ratio Lower Upper
225 100
223 69.4 53.8 80.8
227 69.2 50.2 75.2



#34
Caprolactam
Concen: 8.200 ng/ul
RT: 11.584 min Scan# 1463
Delta R.T. -0.012 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:113 Resp: 4758
Ion Ratio Lower Upper
113 100
55 234.3 199.0 298.4
56 188.0 150.6 226.0









#35
 4-Chloro-3-methylphenol
 Concen: 17.831 ng/ul
 RT: 11.977 min Scan# 1530
 Delta R.T. -0.006 min
 Lab File: BG061280.D
 Acq: 24 May 2024 8:18




Instrument :
 BNA_G
 ClientSampleId :
 SST020495


Tgt Ion:107	Resp:	34959
Ion Ratio	Lower	Upper
107	100	
144	24.6	21.2 31.8
142	69.7	61.6 92.4



#36
 2-Methylnaphthalene
 Concen: 18.576 ng/ul
 RT: 12.342 min Scan# 1592
 Delta R.T. -0.001 min
 Lab File: BG061280.D
 Acq: 24 May 2024 8:18

Tgt Ion:142	Resp:	66650
Ion Ratio	Lower	Upper
142	100	
141	93.2	72.2 108.2







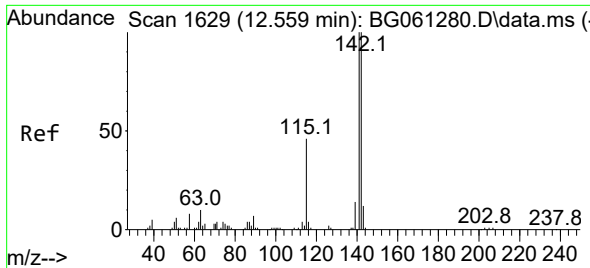

#37
1-Methylnaphthalene
Concen: 18.164 ng/ul
RT: 12.559 min Scan# 1629
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:142 Resp: 66884
Ion Ratio Lower Upper
142 100
141 100.8 75.5 113.3
116 3.9 4.0 6.0#

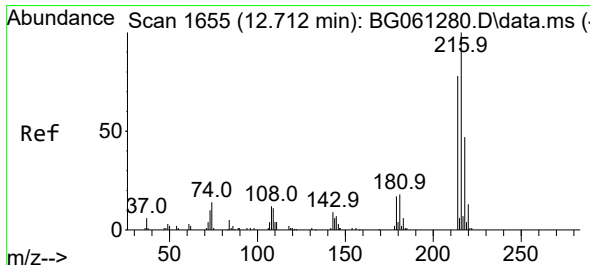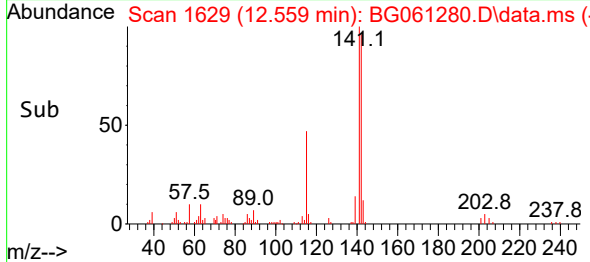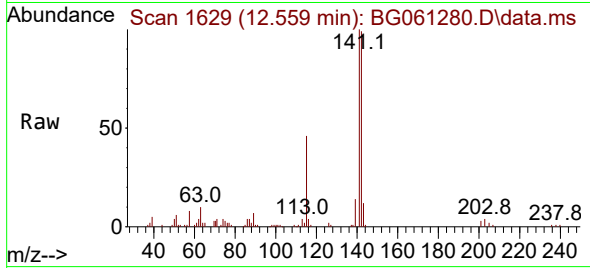

#39
1,2,4,5-Tetrachlorobenzene
Concen: 18.948 ng/ul
RT: 12.712 min Scan# 1655
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:216 Resp: 50514
Ion Ratio Lower Upper
216 100
214 77.8 64.5 96.7
179 16.6 16.0 24.0
108 13.3 9.9 14.9

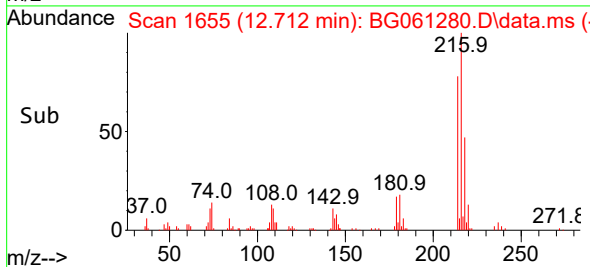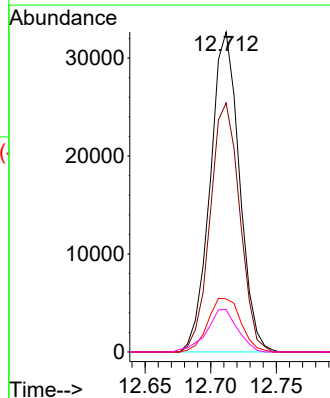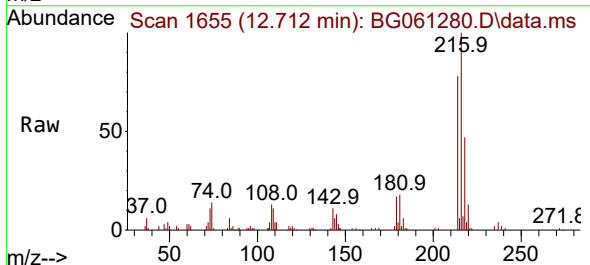



#40

Hexachlorocyclopentadiene

Concen: 20.479 ng/ul

RT: 12.688 min Scan# 1651

Delta R.T. -0.006 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion:237 Resp: 24643

Ion Ratio Lower Upper

237 100

235 61.2 45.4 68.2

272 13.4 11.4 17.0



#41

2,4,6-Trichlorophenol

Concen: 17.779 ng/ul

RT: 12.959 min Scan# 1697

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion:196 Resp: 26697


Ion Ratio Lower Upper

196 100

198 94.7 78.5 117.7

200 30.8 26.1 39.1





#42

2,4,5-Trichlorophenol

Concen: 18.400 ng/ul

RT: 13.041 min Scan# 1711

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion:196 Resp: 29096

Ion Ratio Lower Upper

196 100

198 93.8 77.4 116.2

200 32.4 21.0 31.6#

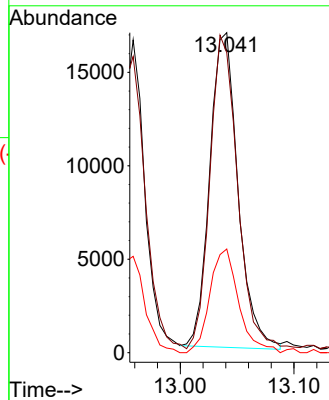

#43

1,1'-Biphenyl

Concen: 18.747 ng/ul

RT: 13.352 min Scan# 1764

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion:154 Resp: 97884


Ion Ratio Lower Upper

154 100

153 43.1 31.2 46.8

76 10.7 8.5 12.7



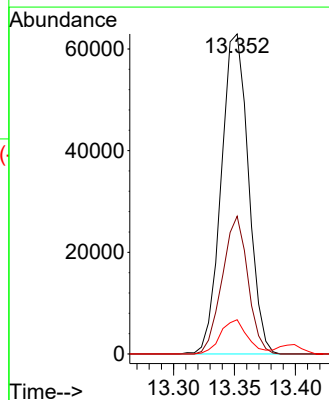





#44
2-Chloronaphthalene
Concen: 18.929 ng/ul
RT: 13.393 min Scan# 1771
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:162 Resp: 77781
Ion Ratio Lower Upper
162 100
164 35.0 26.8 40.2
127 39.9 31.9 47.9



#45
2-Nitroaniline
Concen: 17.876 ng/ul
RT: 13.599 min Scan# 1806
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion: 65 Resp: 30315
Ion Ratio Lower Upper
65 100
92 51.1 46.2 69.4
138 87.3 65.0 97.6









#47
Dimethylphthalate
Concen: 17.851 ng/ul
RT: 13.975 min Scan# 1870
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:163 Resp: 116518
Ion Ratio Lower Upper
163 100
194 3.9 3.1 4.7
164 9.8 8.1 12.1

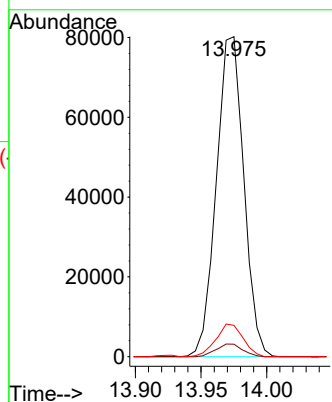

#48
2,6-Dinitrotoluene
Concen: 17.353 ng/ul
RT: 14.098 min Scan# 1891
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:165 Resp: 22212
Ion Ratio Lower Upper
165 100
89 57.3 46.0 69.0
121 21.3 17.9 26.9


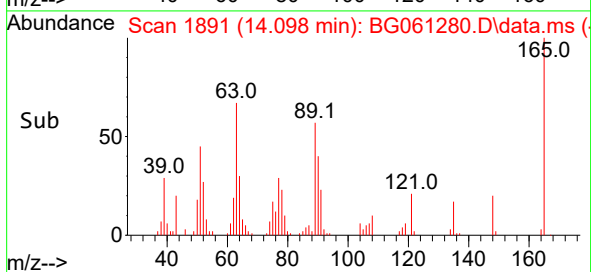






#50
Acenaphthylene
Concen: 18.584 ng/ul
RT: 14.239 min Scan# 1915
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:152 Resp: 134171
Ion Ratio Lower Upper
152 100
151 21.0 16.2 24.2
153 12.1 10.2 15.4

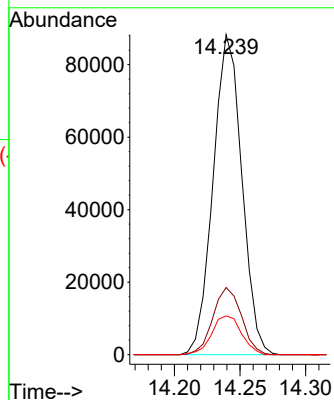

#51
3-Nitroaniline
Concen: 18.613 ng/ul
RT: 14.422 min Scan# 1946
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:138 Resp: 20677
Ion Ratio Lower Upper
138 100
108 9.3 10.1 15.1#
92 115.6 97.6 146.4



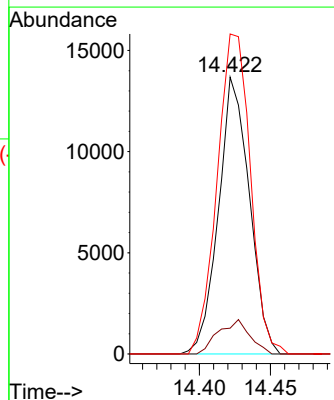





#52
Acenaphthene
Concen: 18.833 ng/ul
RT: 14.580 min Scan# 1973
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:153 Resp: 89196
Ion Ratio Lower Upper
153 100
152 47.3 37.8 56.8
154 83.0 69.0 103.6

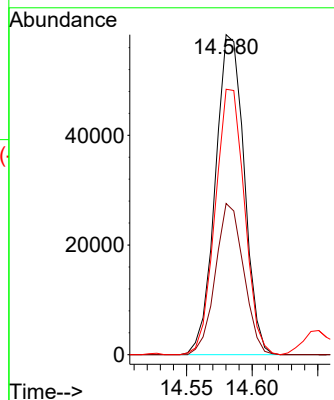

#53
2,4-Dinitrophenol
Concen: 16.105 ng/ul
RT: 14.645 min Scan# 1984
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:184 Resp: 10932
Ion Ratio Lower Upper
184 100
63 72.1 61.3 91.9
154 62.8 55.0 82.4



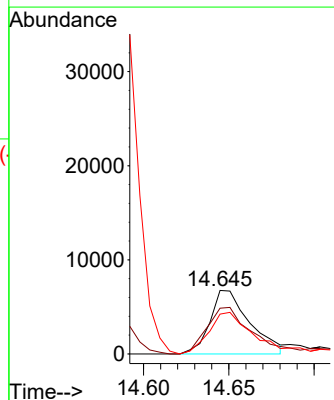





#55
4-Nitrophenol
Concen: 16.086 ng/ul
RT: 14.756 min Scan# 2003
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:109 Resp: 14643
Ion Ratio Lower Upper
109 100
139 98.0 74.9 112.3
65 130.9 104.0 156.0



#56
Dibenzofuran
Concen: 18.489 ng/ul
RT: 14.921 min Scan# 2031
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:168 Resp: 125205
Ion Ratio Lower Upper
168 100
139 42.2 33.4 50.2





#57

2,4-Dinitrotoluene

Concen: 18.010 ng/ul

RT: 14.892 min Scan# 2026

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion:165 Resp: 35075

Ion Ratio Lower Upper

165 100

63 54.7 43.4 65.2

182 2.6 2.0 3.0

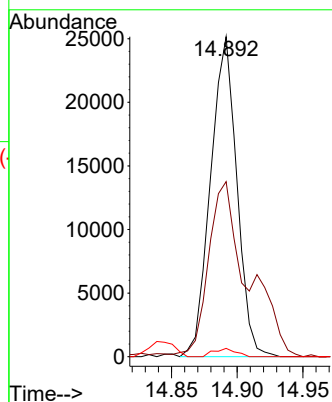

#58

2,3,4,6-Tetrachlorophenol

Concen: 17.141 ng/ul

RT: 15.156 min Scan# 2071

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Tgt Ion:232 Resp: 24722




Ion Ratio Lower Upper


232 100

131 39.5 30.2 45.2

130 0.0 1.8 2.6#

166 26.0 21.0 31.6

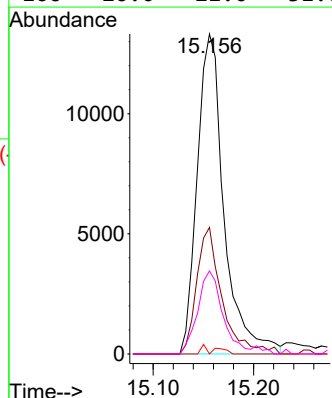



#59

Diethylphthalate

Concen: 17.727 ng/ul

RT: 15.338 min Scan# 2102

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion:149 Resp: 114263

Ion Ratio Lower Upper

149 100

177 22.1 19.1 28.7

150 12.3 11.0 16.4



#61

Fluorene

Concen: 18.368 ng/ul

RT: 15.567 min Scan# 2141

Delta R.T. -0.006 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion:166 Resp: 107623


Ion Ratio Lower Upper

166 100

165 102.1 81.8 122.8

167 12.3 10.6 16.0









#62
4-Chlorophenyl-phenylether
Concen: 18.503 ng/ul
RT: 15.561 min Scan# 2140
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:204 Resp: 63580
Ion Ratio Lower Upper
204 100
206 29.8 26.3 39.5
141 51.5 43.0 64.6



#63
4-Nitroaniline
Concen: 18.618 ng/ul
RT: 15.591 min Scan# 2145
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:138 Resp: 21541
Ion Ratio Lower Upper
138 100
92 53.0 48.6 73.0
108 106.9 95.5 143.3









#66
 4,6-Dinitro-2-methylphenol
 Concen: 15.947 ng/ul
 RT: 15.661 min Scan# 2157
 Delta R.T. -0.001 min
 Lab File: BG061280.D
 Acq: 24 May 2024 8:18




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020495


Tgt Ion:198 Resp: 20510
 Ion Ratio Lower Upper
 198 100
 182 5.5 2.9 4.3#
 77 23.5 22.3 33.5



#67
 N-Nitrosodiphenylamine
 Concen: 18.703 ng/ul
 RT: 15.779 min Scan# 2177
 Delta R.T. -0.001 min
 Lab File: BG061280.D
 Acq: 24 May 2024 8:18

Tgt Ion:169 Resp: 95384
 Ion Ratio Lower Upper
 169 100
 168 64.9 51.9 77.9
 167 36.1 29.4 44.2









#68
4-Bromophenyl-phenylether
Concen: 18.208 ng/ul
RT: 16.454 min Scan# 211
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:248 Resp: 43777
Ion Ratio Lower Upper
248 100
250 105.3 79.4 119.2
141 68.1 50.2 75.4



#69
Hexachlorobenzene
Concen: 18.698 ng/ul
RT: 16.578 min Scan# 2313
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:284 Resp: 49967
Ion Ratio Lower Upper
284 100
142 26.9 21.2 31.8
249 35.3 28.7 43.1





#70

Atrazine

Concen: 18.358 ng/ul

RT: 16.725 min Scan# 21

Delta R.T. -0.006 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion:200 Resp: 37052

Ion Ratio Lower Upper

200 100

173 22.3 15.9 23.9

215 46.8 37.3 55.9



#71

Pentachlorophenol

Concen: 17.620 ng/ul

RT: 16.930 min Scan# 2373

Delta R.T. -0.006 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion:266 Resp: 16388


Ion Ratio Lower Upper

266 100

264 62.0 41.9 62.9

268 60.7 52.6 79.0


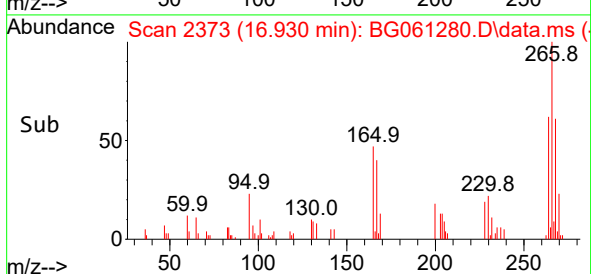






#72
Phenanthrene
Concen: 18.832 ng/ul
RT: 17.306 min Scan# 2437
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:178 Resp: 185461
Ion Ratio Lower Upper
178 100
179 14.6 12.7 19.1
176 19.5 15.5 23.3



#74
Anthracene
Concen: 18.773 ng/ul
RT: 17.400 min Scan# 2453
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:178 Resp: 191161
Ion Ratio Lower Upper
178 100
179 15.0 11.8 17.6
176 19.0 14.9 22.3









#75
1,2,3,4-Tetrachlorobenzene
Concen: 18.770 ng/uL
RT: 13.317 min Scan# 1758
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:216 Resp: 50345
Ion Ratio Lower Upper
216 100
214 82.5 60.0 90.0
218 51.5 38.5 57.7



#76
Pentachlorobenzene
Concen: 18.511 ng/uL
RT: 14.845 min Scan# 1818
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:250 Resp: 54893
Ion Ratio Lower Upper
250 100
248 64.4 52.6 79.0
252 65.4 54.7 82.1



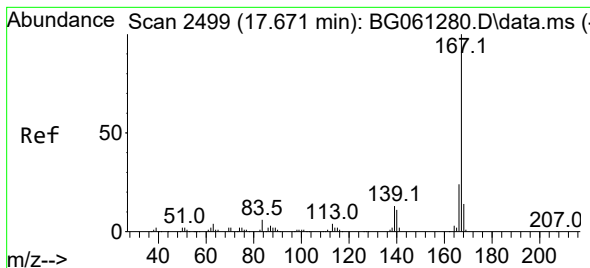

#77

Carbazole

Concen: 18.982 ng/ul

RT: 17.671 min Scan# 2499

Delta R.T. -0.006 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion:167 Resp: 157213

Ion Ratio Lower Upper

167 100

166 24.1 18.6 28.0

139 12.6 10.6 15.8

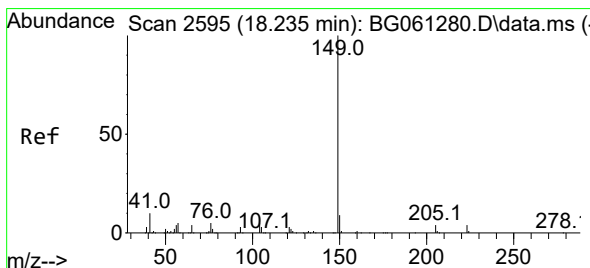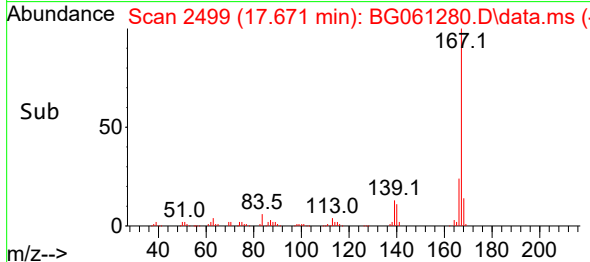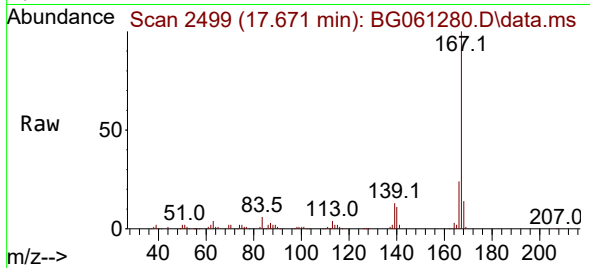

#78

Di-n-butylphthalate

Concen: 18.574 ng/ul

RT: 18.235 min Scan# 2595

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion:149 Resp: 192761


Ion Ratio Lower Upper

149 100

150 8.7 7.8 11.8

104 5.3 4.8 7.2


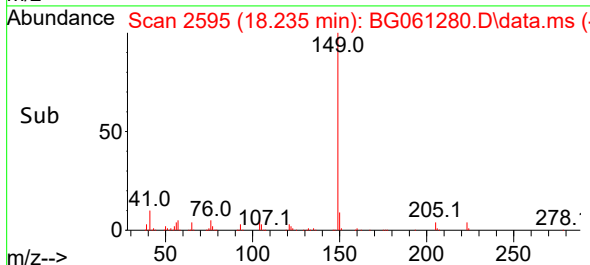
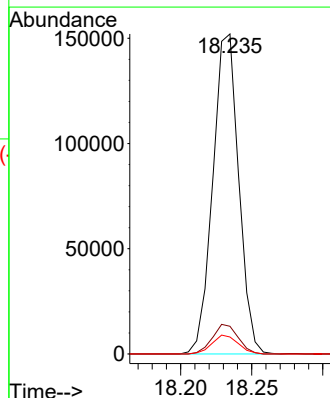
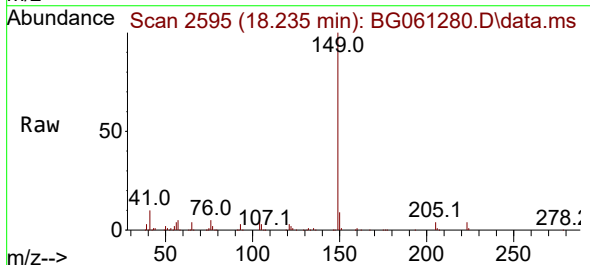




#80
Fluoranthene
Concen: 18.516 ng/ul
RT: 19.322 min Scan# 21
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18




Instrument :
BNA_G
ClientSampleId :
SSTD020495


Tgt Ion:202 Resp: 239849
Ion Ratio Lower Upper
202 100
101 6.4 4.8 7.2
100 5.0 4.1 6.1



#82
Pyrene
Concen: 18.546 ng/ul
RT: 19.686 min Scan# 2842
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:202 Resp: 249378
Ion Ratio Lower Upper
202 100
101 7.3 5.7 8.5
100 5.9 5.1 7.7





#83

Butylbenzylphthalate

Concen: 18.770 ng/ul

RT: 20.579 min Scan# 2994

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion:149 Resp: 86701

Ion Ratio Lower Upper

149 100

91 66.0 54.8 82.2

206 23.8 19.4 29.0



#84

3,3'-Dichlorobenzidine

Concen: 19.896 ng/ul

RT: 21.413 min Scan# 3136

Delta R.T. -0.006 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion:252 Resp: 88816


Ion Ratio Lower Upper

252 100

254 63.3 52.7 79.1

126 7.0 5.0 7.6





#85

Benzo(a)anthracene

Concen: 18.153 ng/ul

RT: 21.496 min Scan# 3150

Delta R.T. -0.006 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion:228 Resp: 263422

Ion Ratio Lower Upper

228 100

229 18.9 15.2 22.8

226 26.8 21.4 32.2

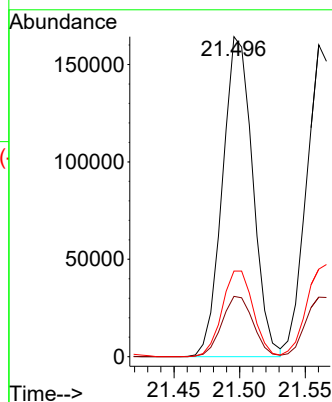

#86

Bis(2-ethylhexyl)phthalate

Concen: 18.404 ng/ul

RT: 21.413 min Scan# 3136

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion:149 Resp: 125834


Ion Ratio Lower Upper

149 100

167 25.9 21.1 31.7


279 4.8 3.3 4.9








#87
Chrysene
Concen: 18.349 ng/ul
RT: 21.560 min Scan# 3161
Delta R.T. -0.006 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Instrument :
BNA_G
ClientSampleId :
SSTD020495







Tgt Ion:228 Resp: 245175
Ion Ratio Lower Upper
228 100
226 28.1 23.4 35.0
229 19.1 15.4 23.2



#89
Di-n-octyl phthalate
Concen: 18.196 ng/ul
RT: 22.577 min Scan# 3334
Delta R.T. -0.001 min
Lab File: BG061280.D
Acq: 24 May 2024 8:18

Tgt Ion:149 Resp: 214722





#90

Benzo(b)fluoranthene

Concen: 18.324 ng/ul

RT: 23.628 min Scan# 3513

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion:252 Resp: 257339

Ion Ratio Lower Upper

252 100

253 21.3 17.8 26.8

125 5.0 4.6 6.8

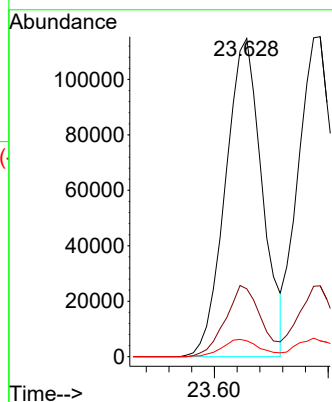

#91

Benzo(k)fluoranthene

Concen: 17.911 ng/ul

RT: 23.693 min Scan# 3524

Delta R.T. -0.001 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion:252 Resp: 255349


Ion Ratio Lower Upper

252 100

253 22.1 16.0 24.0

125 4.9 4.3 6.5

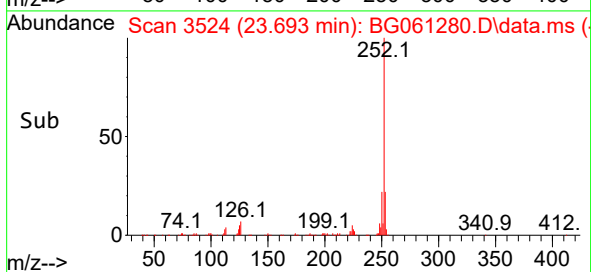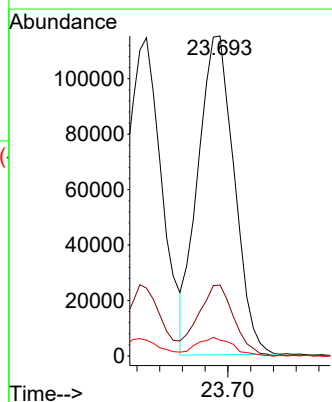



#93

Benzo(a)pyrene

Concen: 18.185 ng/ul

RT: 24.457 min Scan# 30

Delta R.T. -0.006 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18

Instrument :

BNA_G

ClientSampleId :

SSTD020495





Tgt Ion:252 Resp: 242503

Ion Ratio Lower Upper

252 100

253 21.1 16.4 24.6

125 5.8 4.3 6.5

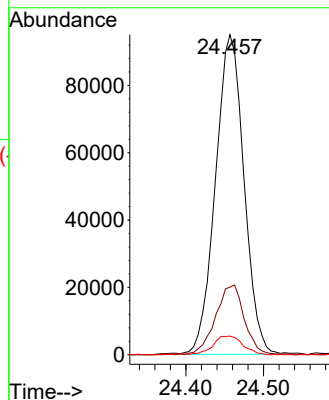

#94

Indeno(1,2,3-cd)pyrene

Concen: 18.416 ng/ul

RT: 28.100 min Scan# 4274

Delta R.T. -0.006 min

Lab File: BG061280.D

Acq: 24 May 2024 8:18




Tgt Ion:276 Resp: 296985


Ion Ratio Lower Upper

276 100

138 13.0 8.6 13.0

277 22.1 19.7 29.5



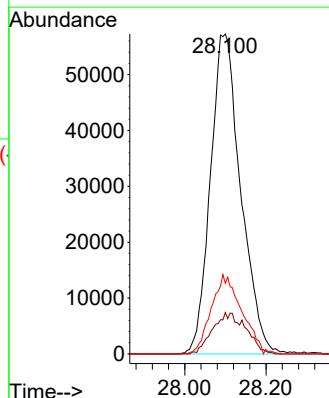





#95
 Dibenzo(a,h)anthracene
 Concen: 18.043 ng/ul
 RT: 28.147 min Scan# 41
 Delta R.T. -0.012 min
 Lab File: BG061280.D
 Acq: 24 May 2024 8:18

Instrument :
 BNA_G
 ClientSampleId :
 SST020495

Tgt Ion:278 Resp: 239924
 Ion Ratio Lower Upper
 278 100
 139 8.9 6.4 9.6
 279 23.2 19.9 29.9

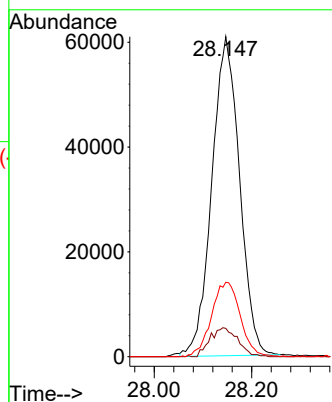

#96
 Benzo(g,h,i)perylene
 Concen: 18.231 ng/ul
 RT: 29.187 min Scan# 4459
 Delta R.T. -0.006 min
 Lab File: BG061280.D
 Acq: 24 May 2024 8:18

Tgt Ion:276 Resp: 233889
 Ion Ratio Lower Upper
 276 100
 138 12.2 8.7 13.1
 277 21.8 18.2 27.2

