

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052522\
 Data File : BG053705.D
 Acq On : 25 May 2022 22:27
 Operator : CG/JU
 Sample : N2893-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P004-SS002-0006-01

Quant Time: May 26 02:53:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 25 15:11:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.989	152	27580	20.000	ng	0.00
21) Naphthalene-d8	10.797	136	112701	20.000	ng	0.00
39) Acenaphthene-d10	14.627	164	84127	20.000	ng	0.00
64) Phenanthrene-d10	17.370	188	183384	20.000	ng	# 0.00
76) Chrysene-d12	21.635	240	173724	20.000	ng	0.00
86) Perylene-d12	24.837	264	181183	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.557	112	146870	90.376	ng	0.00
7) Phenol-d6	7.161	99	221947	89.991	ng	0.00
23) Nitrobenzene-d5	9.152	82	156029	58.934	ng	0.00
42) 2,4,6-Tribromophenol	16.113	330	110288	88.886	ng	0.00
45) 2-Fluorobiphenyl	13.247	172	358859	62.334	ng	0.00
79) Terphenyl-d14	19.979	244	589949	63.248	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052522\
Data File : BG053705.D
Acq On : 25 May 2022 22:27
Operator : CG/JU
Sample : N2893-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P004-SS002-0006-01


Quant Time: May 26 02:53:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

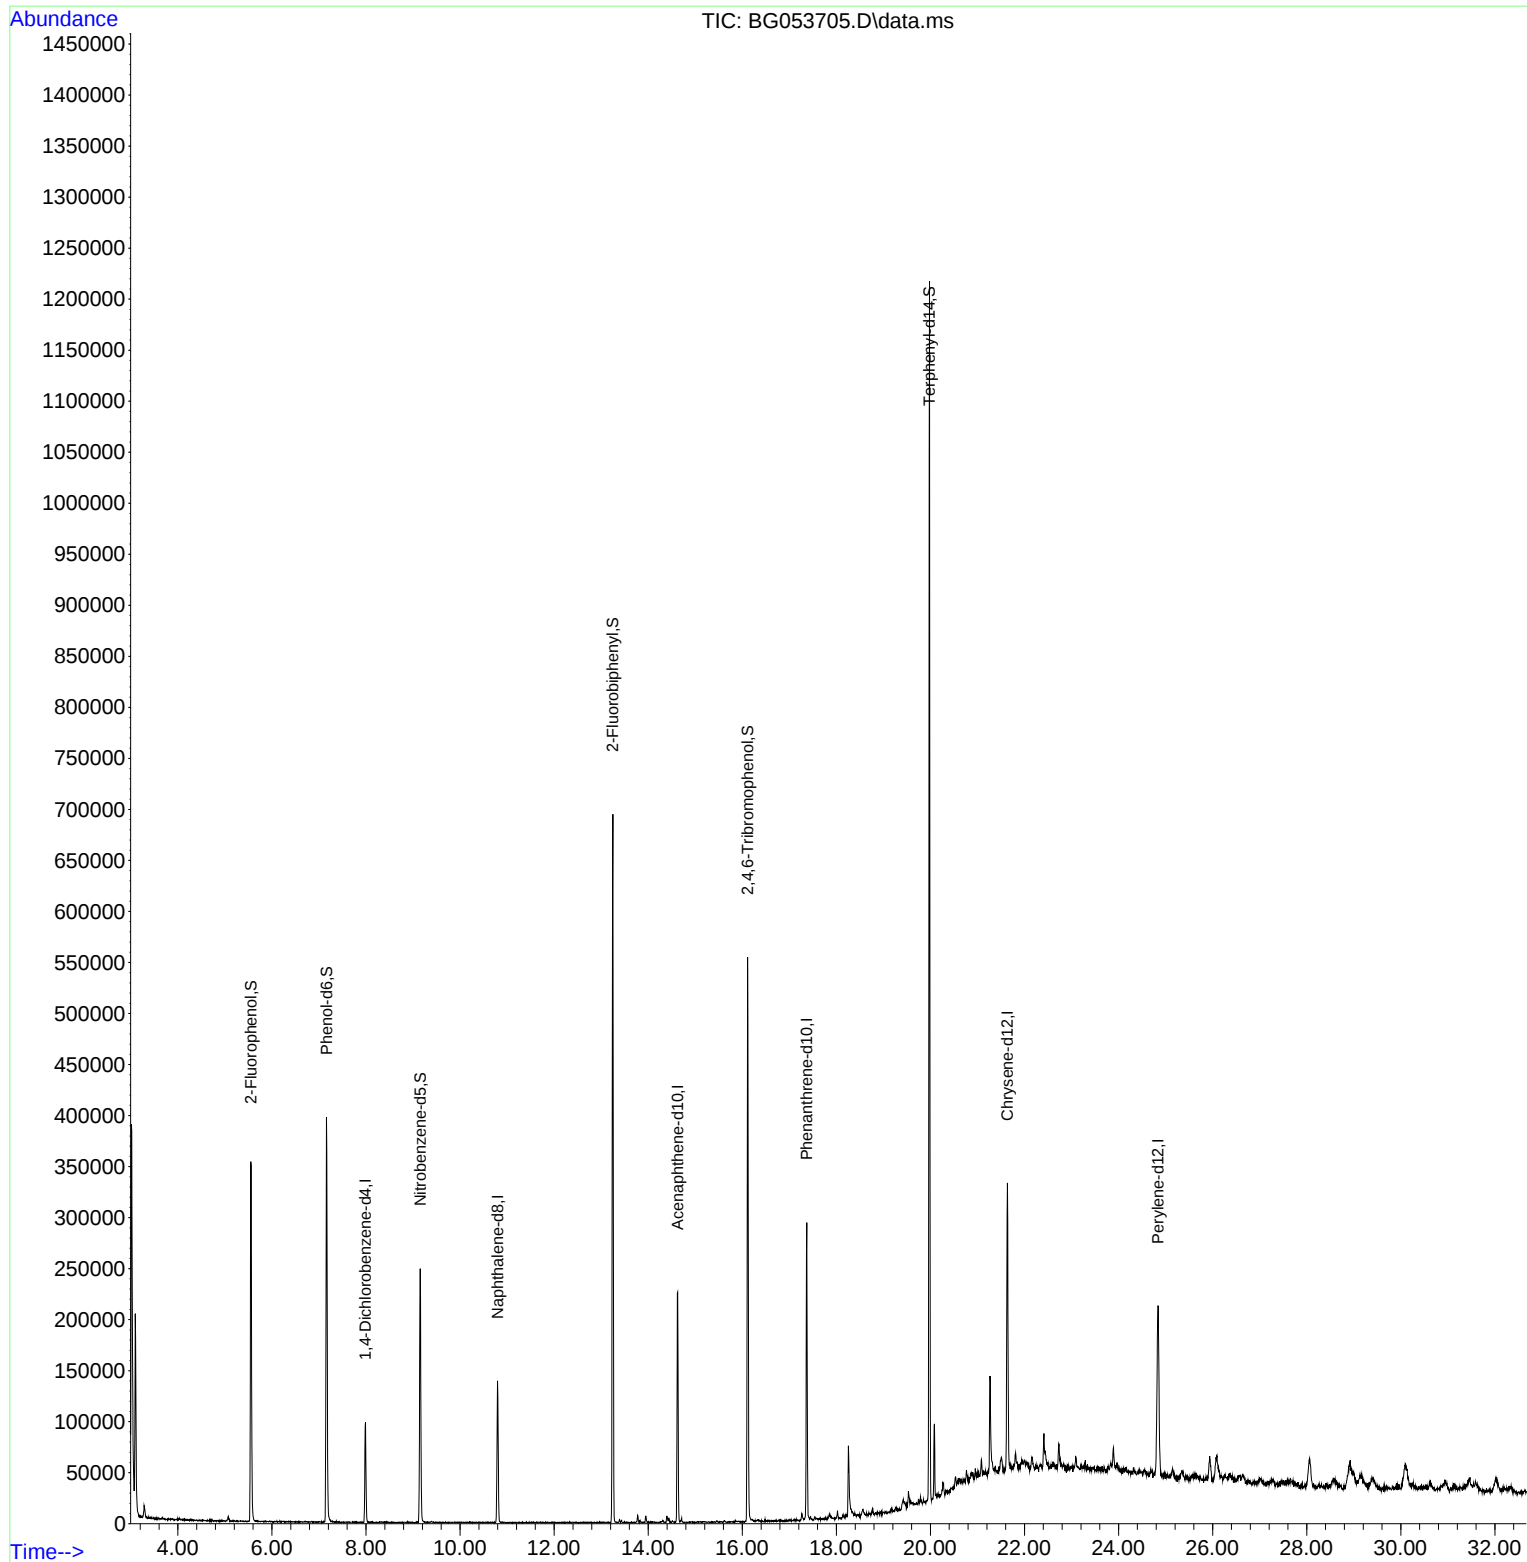





#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.989 min Scan# 802
Delta R.T. 0.003 min
Lab File: BG053705.D
Acq: 25 May 2022 22:27

Instrument :
BNA_G
ClientSampleId :
P004-SS002-0006-01



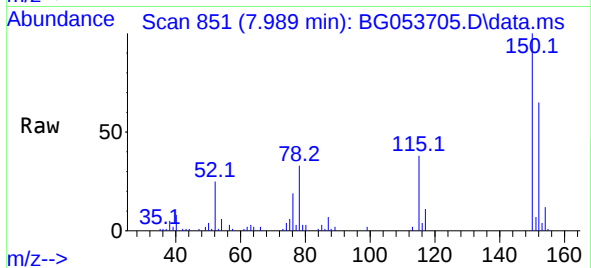


Tgt Ion:152 Resp: 27580
Ion Ratio Lower Upper
152 100
150 153.8 131.6 197.4
115 58.0 50.9 76.3

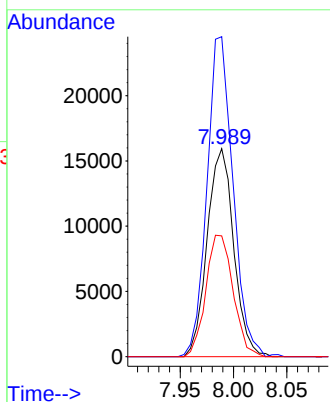

#5
2-Fluorophenol
Concen: 90.376 ng
RT: 5.557 min Scan# 437
Delta R.T. 0.003 min
Lab File: BG053705.D
Acq: 25 May 2022 22:27

Tgt Ion:112 Resp: 146870
Ion Ratio Lower Upper
112 100
64 68.4 55.1 82.7
63 39.7 30.4 45.6


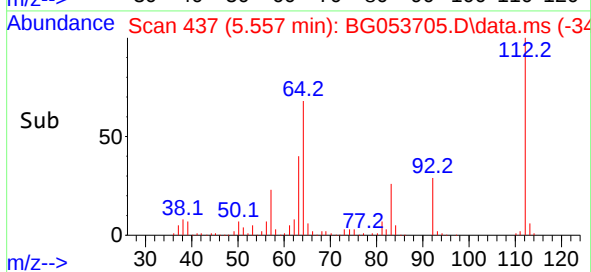
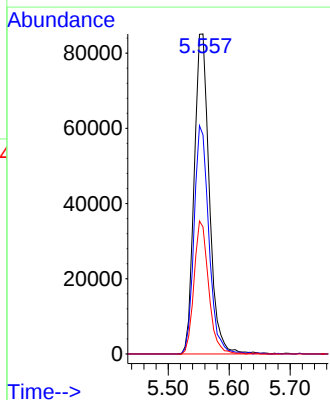





#7
Phenol-d6
Concen: 89.991 ng
RT: 7.161 min Scan# 71
Delta R.T. -0.003 min
Lab File: BG053705.D
Acq: 25 May 2022 22:27




Instrument :
BNA_G
ClientSampleId :
P004-SS002-0006-01

Tgt Ion:	99	Resp:	221947
Ion	Ratio	Lower	Upper
99	100		
42	20.7	17.0	25.6
71	43.1	33.8	50.8

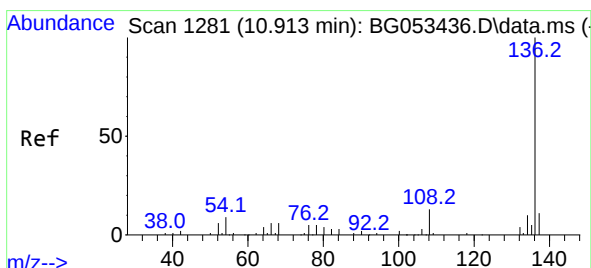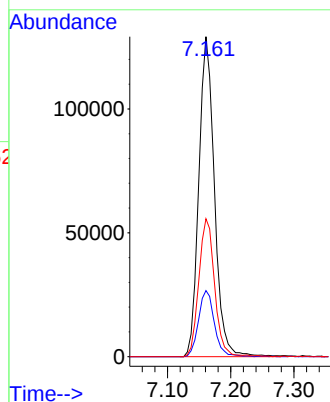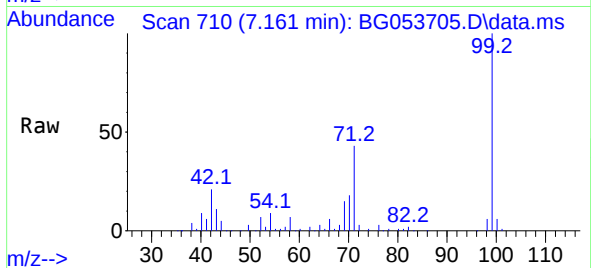

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.797 min Scan# 1329
Delta R.T. -0.003 min
Lab File: BG053705.D
Acq: 25 May 2022 22:27

Tgt Ion:	136	Resp:	112701
Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.5	12.7
54	8.6	7.4	11.2
68	5.5	4.9	7.3


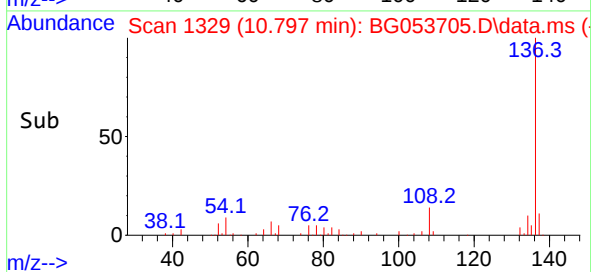
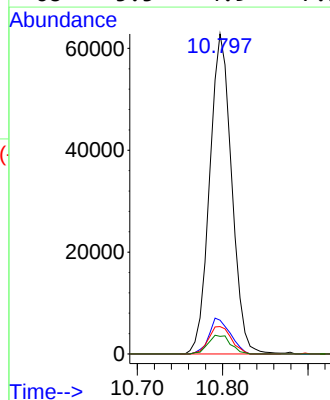





#23
Nitrobenzene-d5
Concen: 58.934 ng
RT: 9.152 min Scan# 1049
Delta R.T. -0.003 min
Lab File: BG053705.D
Acq: 25 May 2022 22:27




Instrument :
BNA_G
ClientSampleId :
P004-SS002-0006-01

Tgt Ion: 82 Resp: 156029
Ion Ratio Lower Upper
82 100
128 34.8 27.9 41.9
54 49.2 41.2 61.8

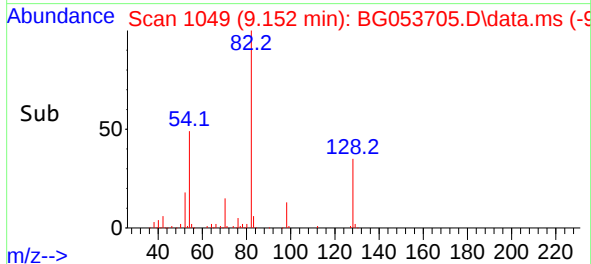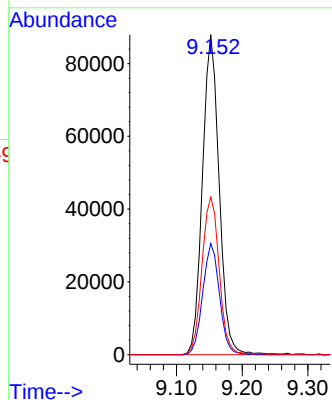

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.627 min Scan# 1981
Delta R.T. 0.003 min
Lab File: BG053705.D
Acq: 25 May 2022 22:27

Tgt Ion:164 Resp: 84127
Ion Ratio Lower Upper
164 100
162 97.8 82.3 123.5
160 42.0 34.2 51.2

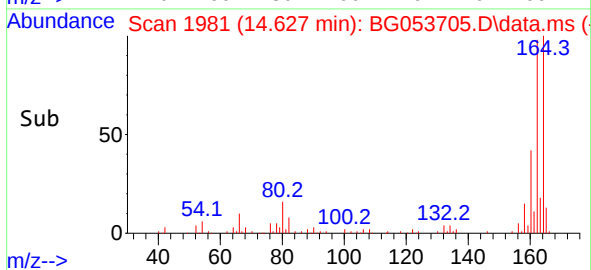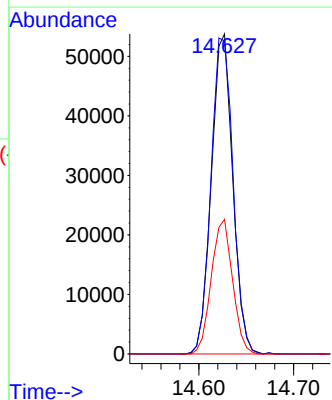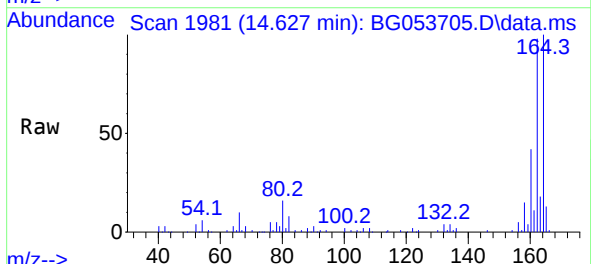



#42

2,4,6-Tribromophenol

Concen: 88.886 ng

RT: 16.113 min Scan# 21

Delta R.T. -0.003 min

Lab File: BG053705.D

Acq: 25 May 2022 22:27

Instrument :

BNA_G

ClientSampleId :

P004-SS002-0006-01





Tgt Ion:330 Resp: 110288

Ion Ratio Lower Upper

330 100

332 97.0 76.0 114.0

141 31.7 27.1 40.7

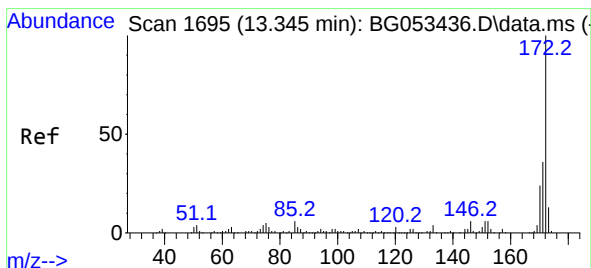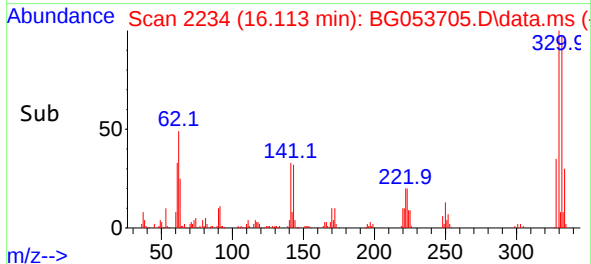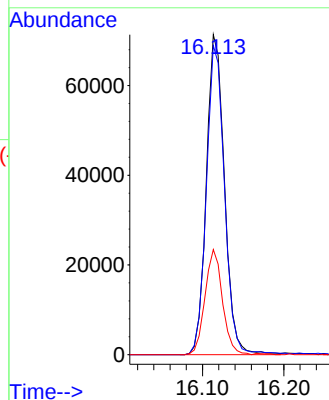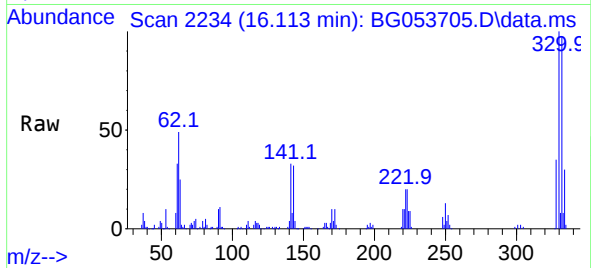

#45

2-Fluorobiphenyl

Concen: 62.334 ng

RT: 13.247 min Scan# 1746

Delta R.T. 0.003 min

Lab File: BG053705.D

Acq: 25 May 2022 22:27




Tgt Ion:172 Resp: 358859

Ion Ratio Lower Upper

172 100

171 35.3 28.5 42.7

170 22.7 18.9 28.3


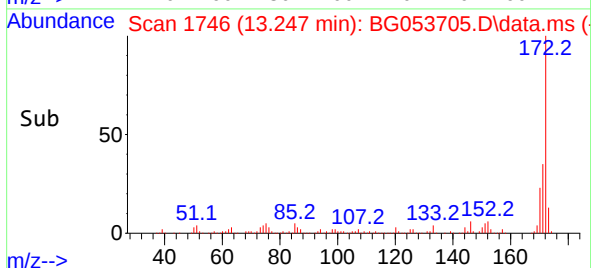
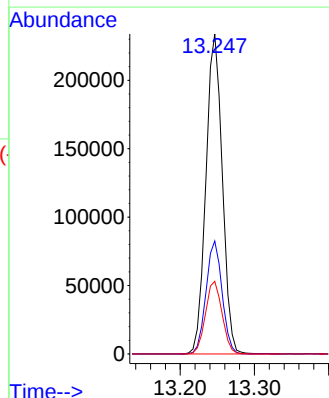
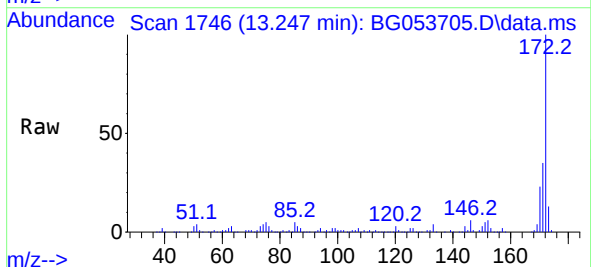




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.370 min Scan# 24
Delta R.T. -0.003 min
Lab File: BG053705.D
Acq: 25 May 2022 22:27




Instrument :
BNA_G
ClientSampleId :
P004-SS002-0006-01


Tgt Ion:188 Resp: 183384
Ion Ratio Lower Upper
188 100
94 5.3 5.4 8.0#
80 7.5 6.8 10.2

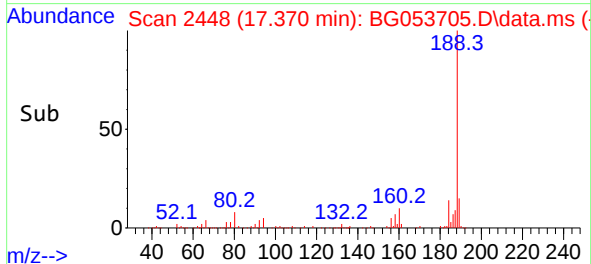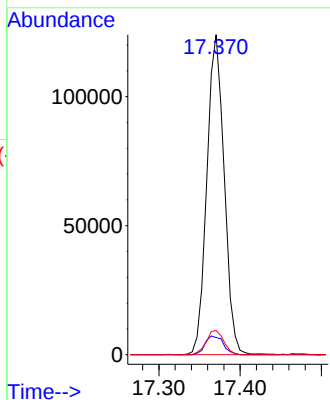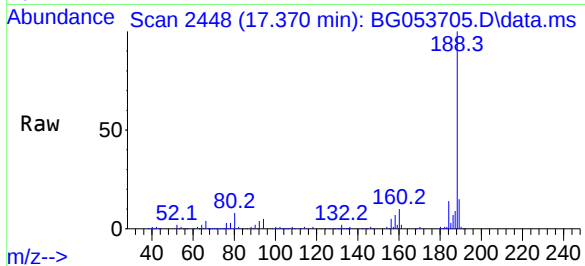

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.635 min Scan# 3174
Delta R.T. -0.003 min
Lab File: BG053705.D
Acq: 25 May 2022 22:27

Tgt Ion:240 Resp: 173724
Ion Ratio Lower Upper
240 100
120 5.6 4.6 7.0
236 24.9 20.2 30.4


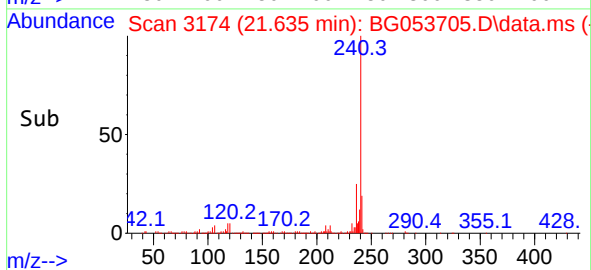
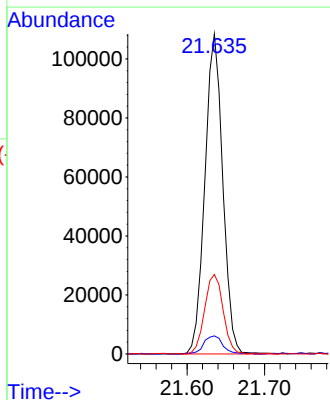
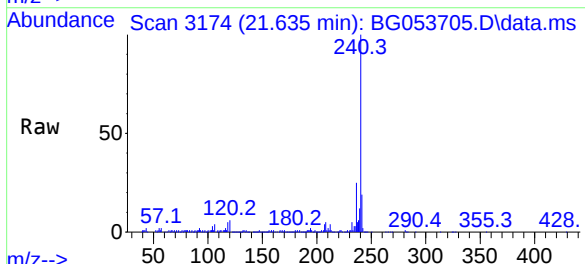




#79
 Terphenyl-d14
 Concen: 63.248 ng
 RT: 19.979 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: BG053705.D
 Acq: 25 May 2022 22:27

Instrument :
 BNA_G
 ClientSampleId :
 P004-SS002-0006-01

Tgt Ion:244 Resp: 589949
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.5 9.7
 122 5.8 5.0 7.4

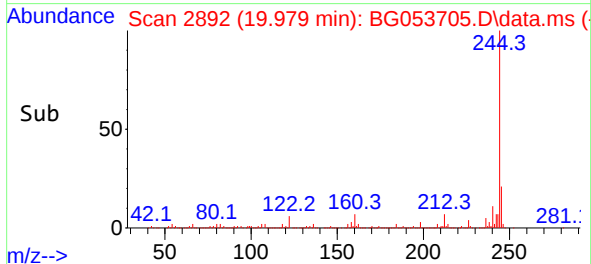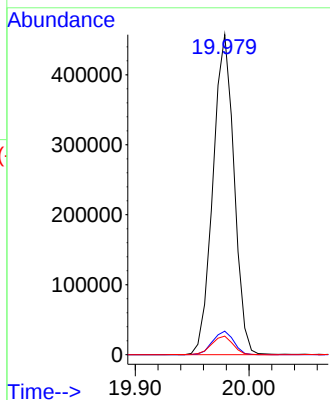

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.837 min Scan# 3719
 Delta R.T. -0.003 min
 Lab File: BG053705.D
 Acq: 25 May 2022 22:27

Tgt Ion:264 Resp: 181183
 Ion Ratio Lower Upper
 264 100
 260 22.8 19.0 28.6
 265 21.2 17.4 26.2

