

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052522\
 Data File : BG053694.D
 Acq On : 25 May 2022 15:11
 Operator : CG/JU
 Sample : PB145039BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB145039BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.090	13	17	25	rVB	21486	32799	1.13%	0.299%
2	5.552	430	436	452	rBV	577621	948365	32.70%	8.658%
3	7.161	703	710	725	rBV	606242	1042525	35.95%	9.518%
4	7.989	844	851	862	rVB	100828	177904	6.14%	1.624%
5	9.153	1039	1049	1063	rBV	375759	670677	23.13%	6.123%
6	10.797	1322	1329	1339	rVB	142311	257446	8.88%	2.350%
7	13.247	1739	1746	1756	rBV	1010066	1555873	53.65%	14.204%
8	14.627	1974	1981	1990	rVB	248215	392475	13.53%	3.583%
9	16.114	2228	2234	2250	rBV	756096	1209359	41.70%	11.041%
10	17.371	2441	2448	2457	rBV	345856	526987	18.17%	4.811%
11	19.979	2886	2892	2898	rBV	2212490	2899811	100.00%	26.474%
12	21.636	3167	3174	3181	rBV	386059	623023	21.48%	5.688%
13	24.837	3709	3719	3734	rVB2	217919	616232	21.25%	5.626%




Sum of corrected areas: 10953476

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052522\
Data File : BG053694.D
Acq On : 25 May 2022 15:11
Operator : CG/JU
Sample : PB145039BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145039BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

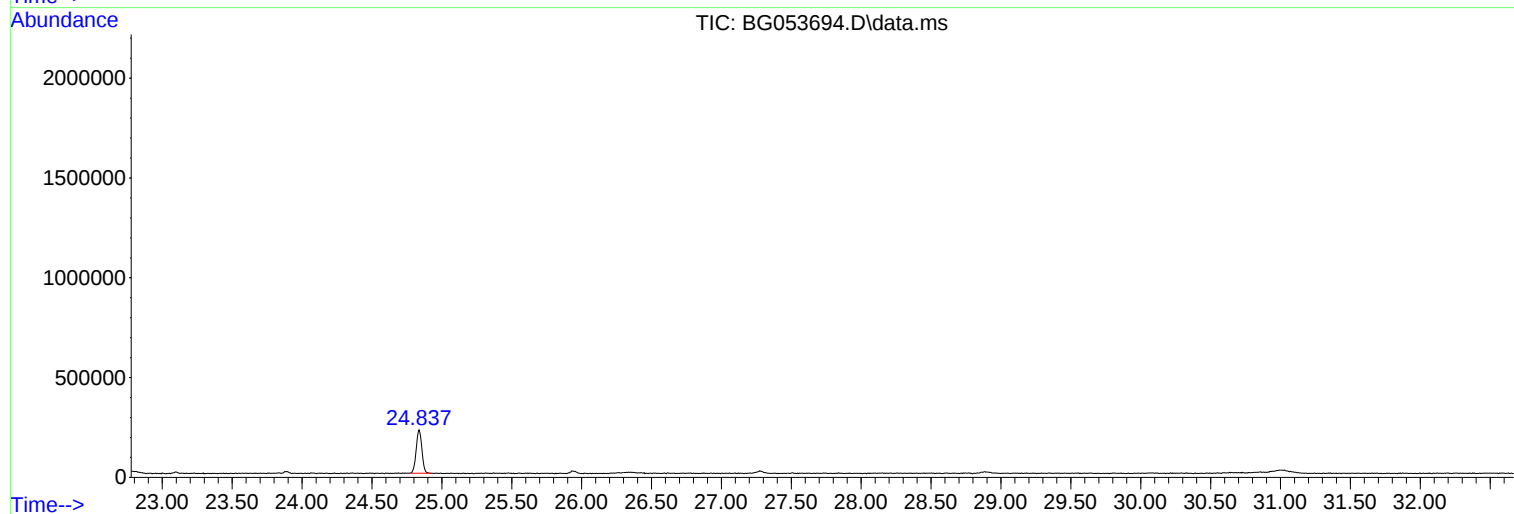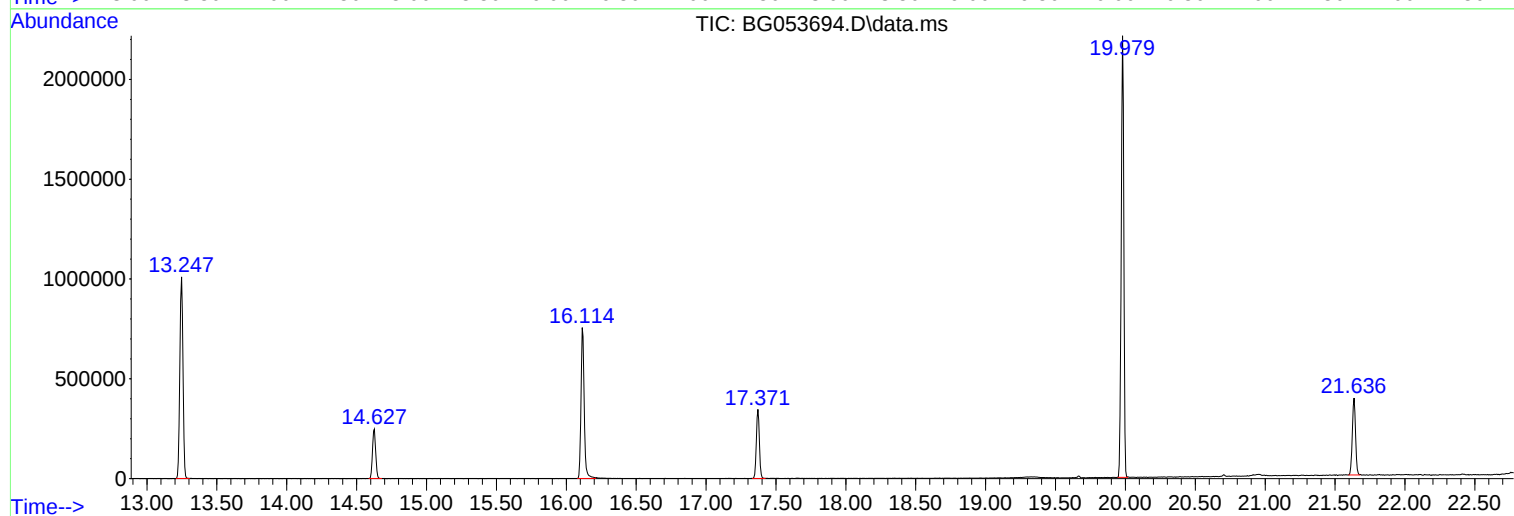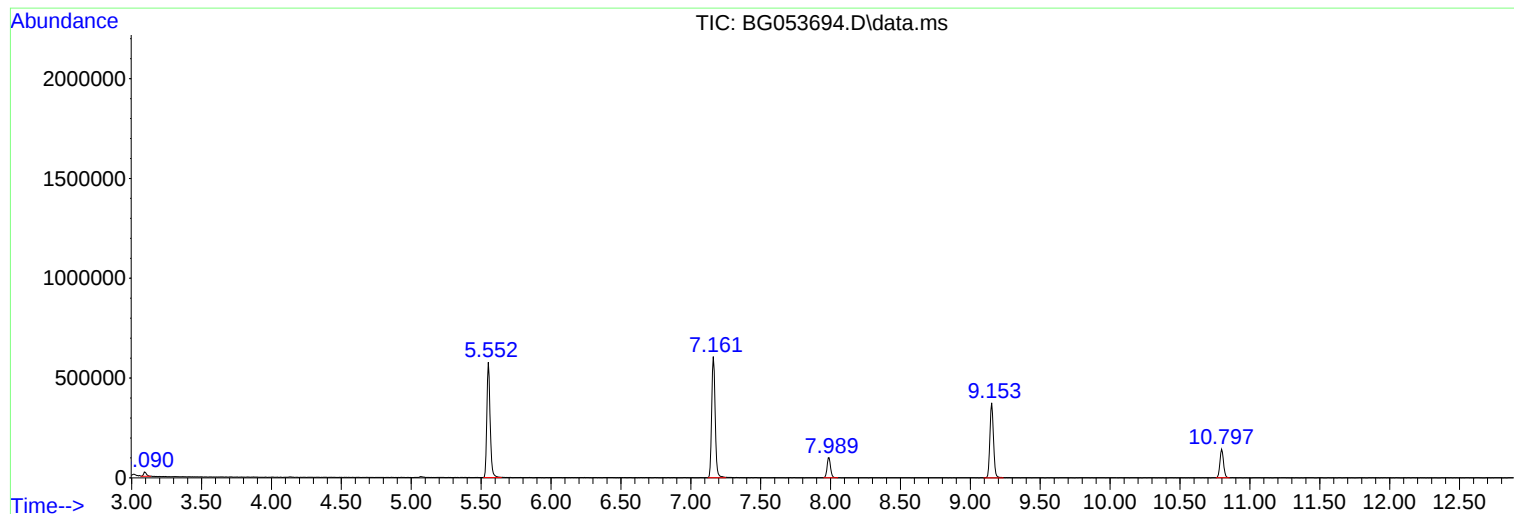

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052522\
Data File : BG053694.D
Acq On : 25 May 2022 15:11
Operator : CG/JU
Sample : PB145039BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145039BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.090	3.69 ng	32799	1,4-Dichlorobenzene-d4	7.984

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	25
3			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	23
4			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	12
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

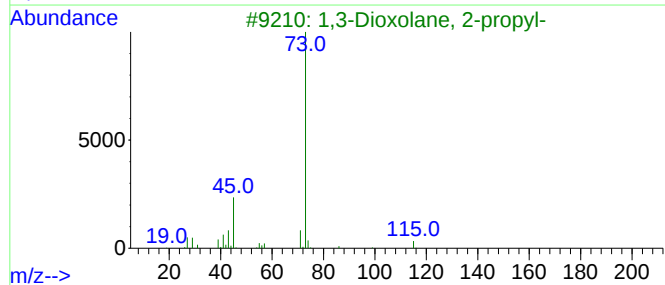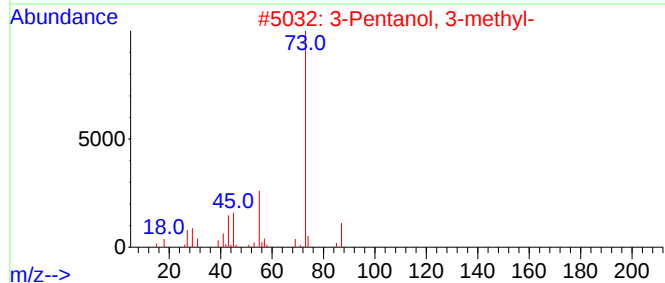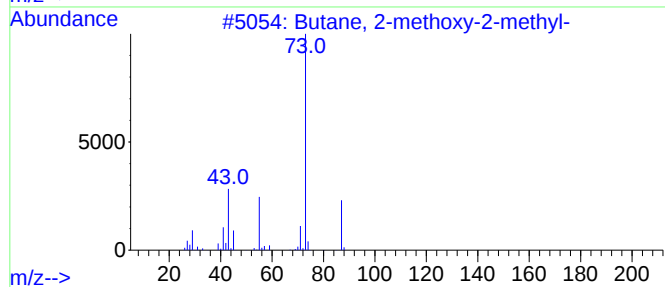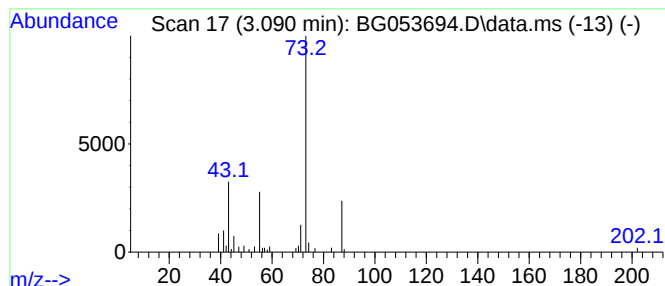

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052522\
Data File : BG053694.D
Acq On : 25 May 2022 15:11
Operator : CG/JU
Sample : PB145039BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145039BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.090	3.7	ng	32799	1	7.984	177904	20.0