
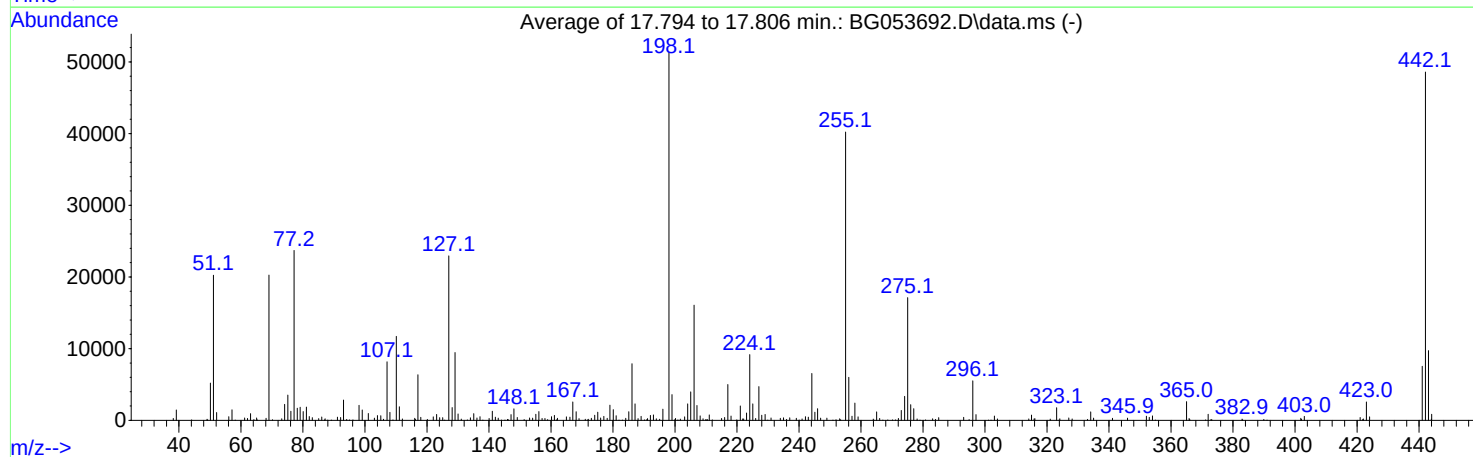


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052522\
 Data File : BG053692.D
 Acq On : 25 May 2022 13:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 15:11:41 2022

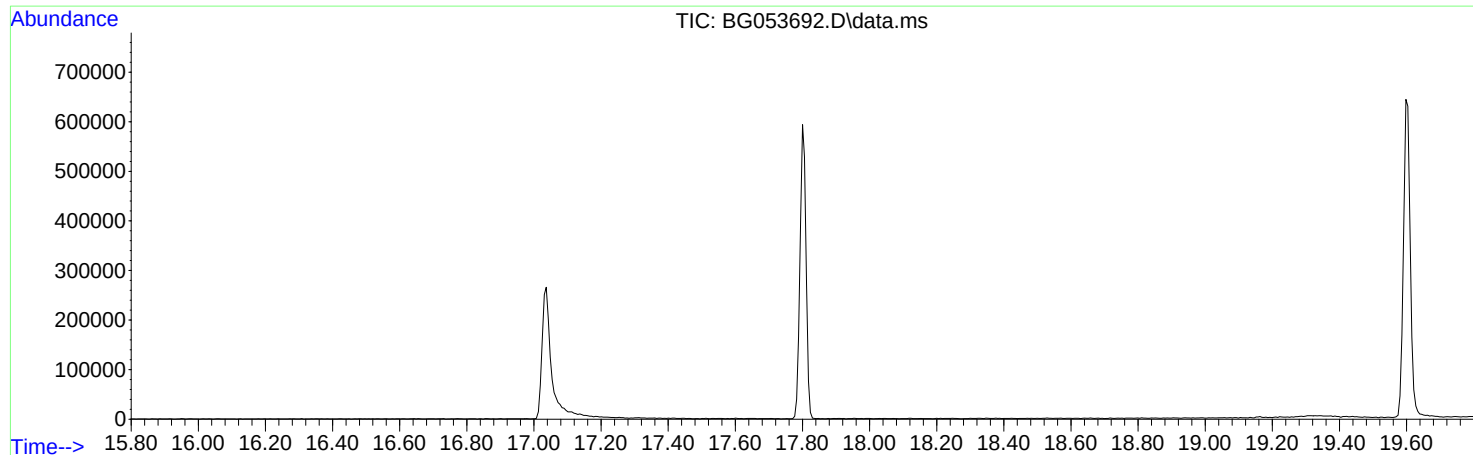




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	20253	PASS
68	69	0.00	2	1.4	283	PASS
69	198	0.00	100	39.5	20272	PASS
70	69	0.00	2	0.5	93	PASS
127	198	10	80	44.7	22949	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51309	PASS
199	198	5	9	7.0	3587	PASS
275	198	10	60	33.3	17111	PASS
365	198	1	100	5.1	2609	PASS
441	198	0.01	100	14.7	7539	PASS
442	442	50	100	100.0	48597	PASS
443	442	15	24	20.0	9743	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052522\
Data File : BG053692.D
Acq On : 25 May 2022 13:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 26 06:47:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

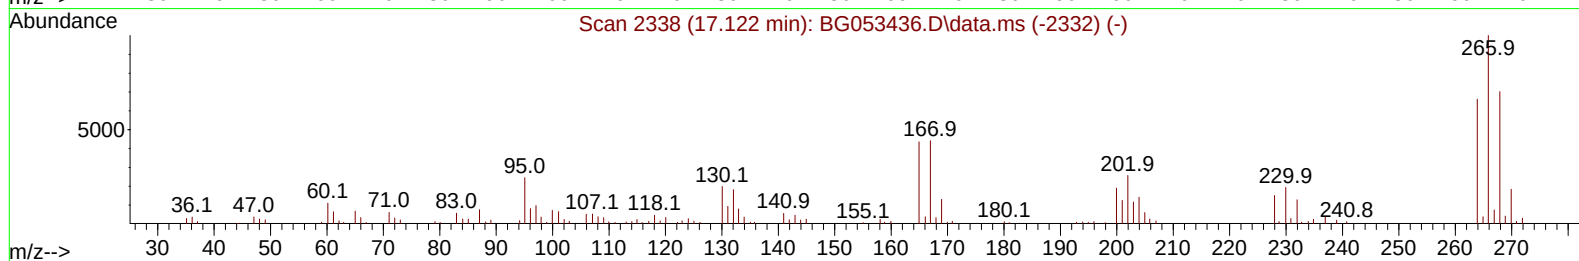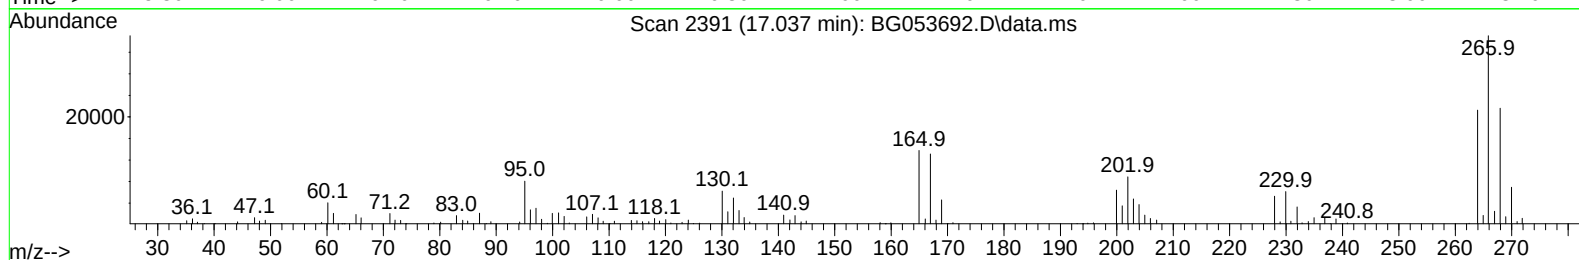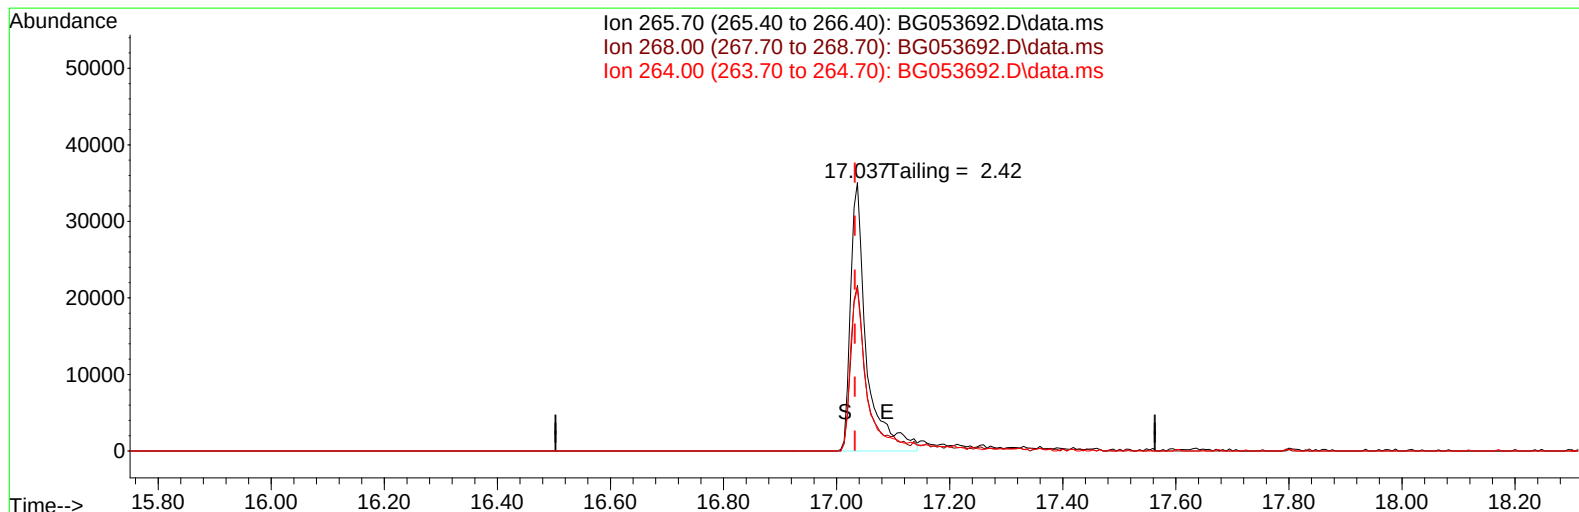

TIC: BG053692.D\data.ms

(70) Pentachlorophenol (C)

17.037min (+ 0.004) 28428.00 ng




response 65062

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.62
264.00	66.20	60.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052522\
Data File : BG053692.D
Acq On : 25 May 2022 13:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 26 06:47:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

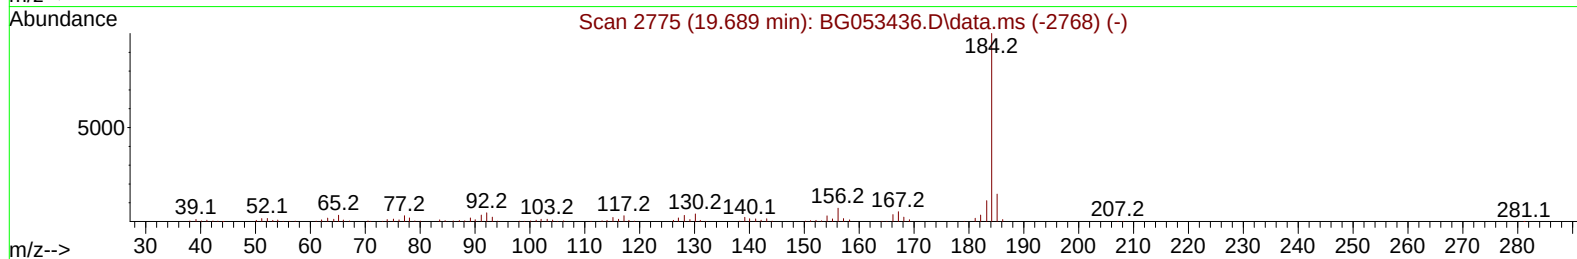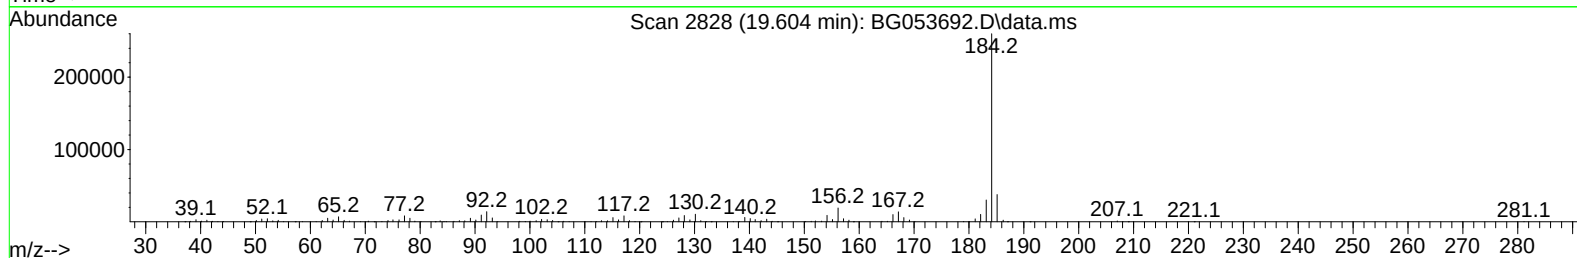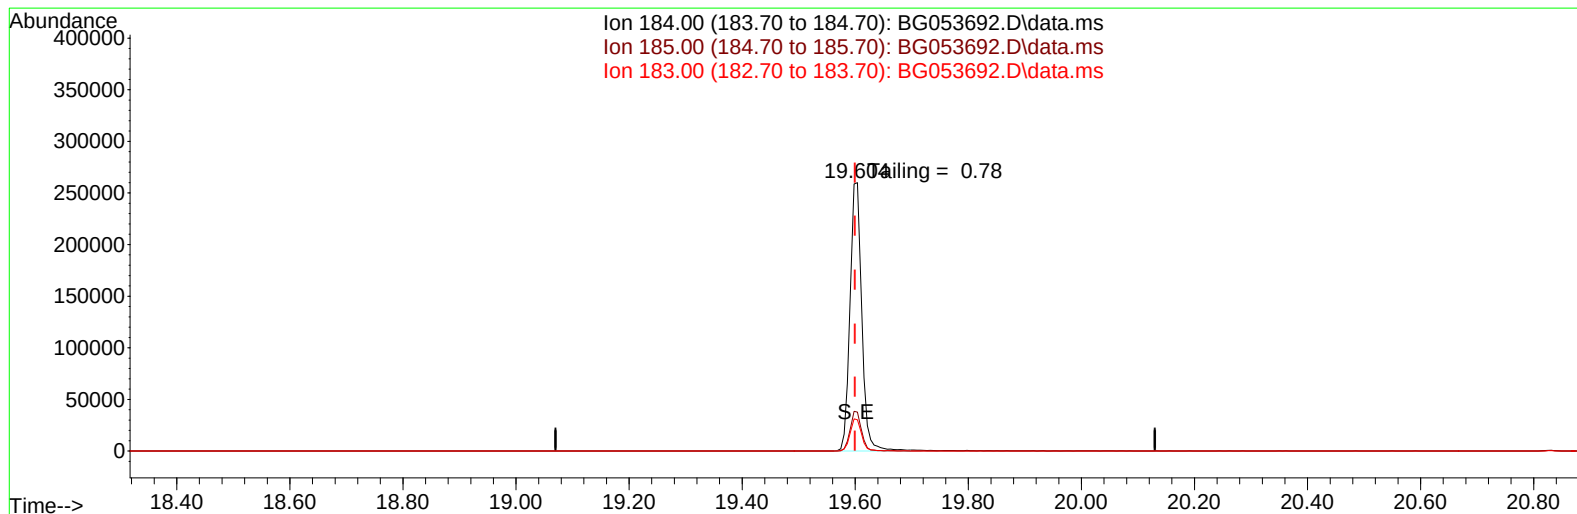

TIC: BG053692.D\data.ms

(77) Benzidine

19.604min (+ 0.004) 0.00 ng

response 379047

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.51
183.00	11.10	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/25/2022	BNA_G	<u>BG053692.D</u>
Compound Name	Response	Retention Time
DDT	192748	20.832
DDD	3530	20.391
DDE	0	19.915
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3530	196278	1.80

Instrument :
BNA_G
ClientSampleId :
DFTPP