

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG053019\
 Data File : BG040968.D
 Acq On : 31 May 2019 2:31
 Operator : HP/JU
 Sample : K3041-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-2-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	3	6	18	rVB2	251549	539960	9.30%	1.834%
2	3.228	18	24	42	rVB	1164845	2134500	36.76%	7.248%
3	3.528	70	75	82	rBV	80327	97916	1.69%	0.332%
4	5.196	353	359	367	rVB	120689	202516	3.49%	0.688%
5	5.661	430	438	448	rBV	1176010	1858803	32.01%	6.312%
6	7.265	704	711	722	rBV	1087924	1861072	32.05%	6.320%
7	7.647	767	776	786	rBV	1277682	2173590	37.44%	7.381%
8	8.122	850	857	867	rVB	246487	418897	7.21%	1.422%
9	8.446	904	912	920	rBV	877904	1469269	25.31%	4.989%
10	9.303	1048	1058	1067	rBV	799282	1455493	25.07%	4.942%
11	10.943	1327	1337	1345	rBV	295842	537272	9.25%	1.824%
12	13.375	1744	1751	1762	rBV	2082666	3102251	53.43%	10.534%
13	14.750	1979	1985	1995	rVB2	498269	799377	13.77%	2.714%
14	16.236	2231	2238	2253	rBV	2047374	2998983	51.65%	10.184%
15	17.494	2444	2452	2462	rBV2	716628	1107143	19.07%	3.760%
16	20.091	2888	2894	2907	rBV	4406955	5806213	100.00%	19.716%
17	21.777	3174	3181	3189	rBV2	779101	1318734	22.71%	4.478%
18	22.547	3307	3312	3317	rBV2	41424	65080	1.12%	0.221%
19	23.258	3428	3433	3447	rVB6	51958	122835	2.12%	0.417%
20	24.092	3570	3575	3580	rBV3	38846	76414	1.32%	0.259%
21	25.114	3735	3749	3761	rVB2	419340	1302853	22.44%	4.424%


Sum of corrected areas: 29449171

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG053019\
Data File : BG040968.D
Acq On : 31 May 2019 2:31
Operator : HP/JU
Sample : K3041-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-2-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

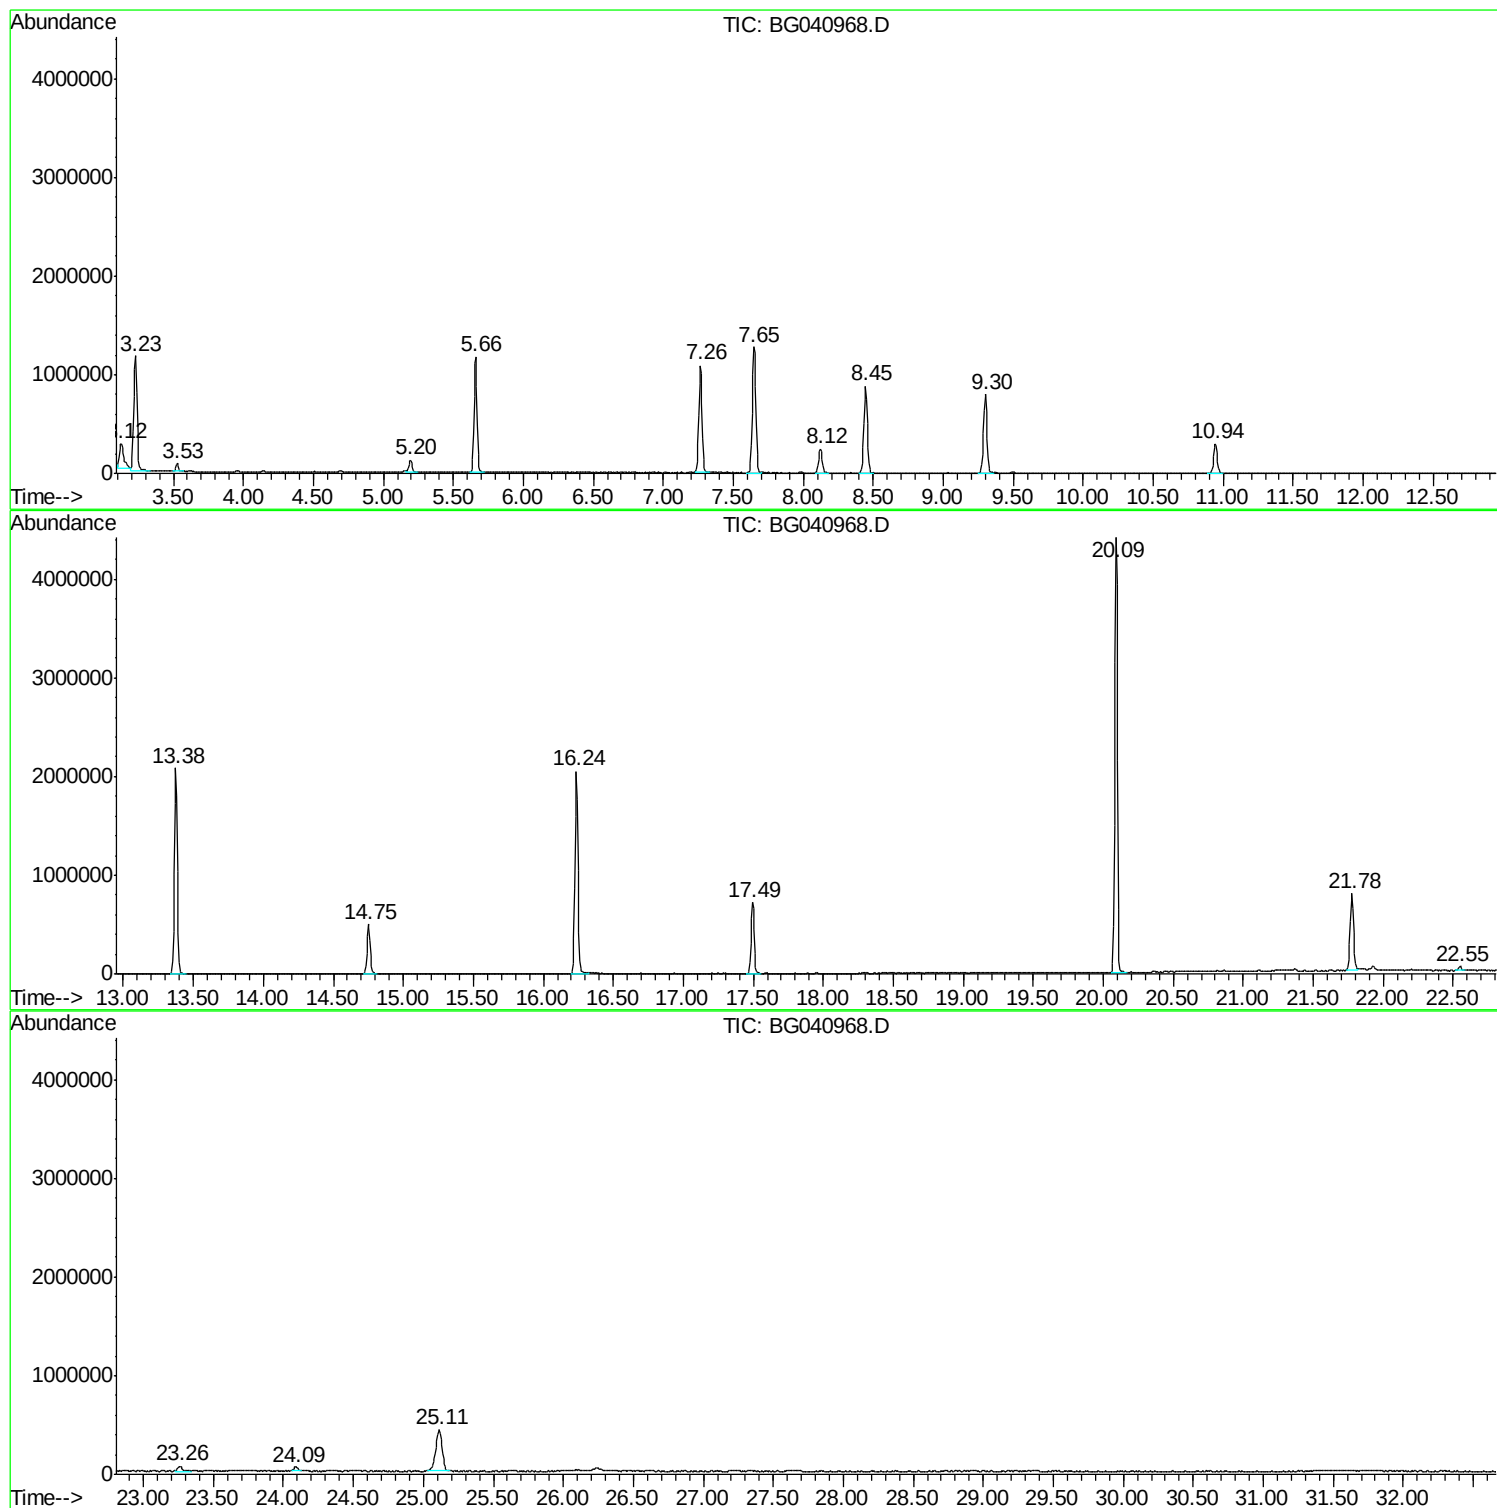

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG053019\
Data_File : BG040968.D
Acq_On : 31_May, 2019 2:311
Operator : HP/JUU
Sample : K3041-088
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
TP-2-S

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
