


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG053019\
 Data File : BG040944.D
 Acq On : 30 May 2019 9:40
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 18:39:57 2019

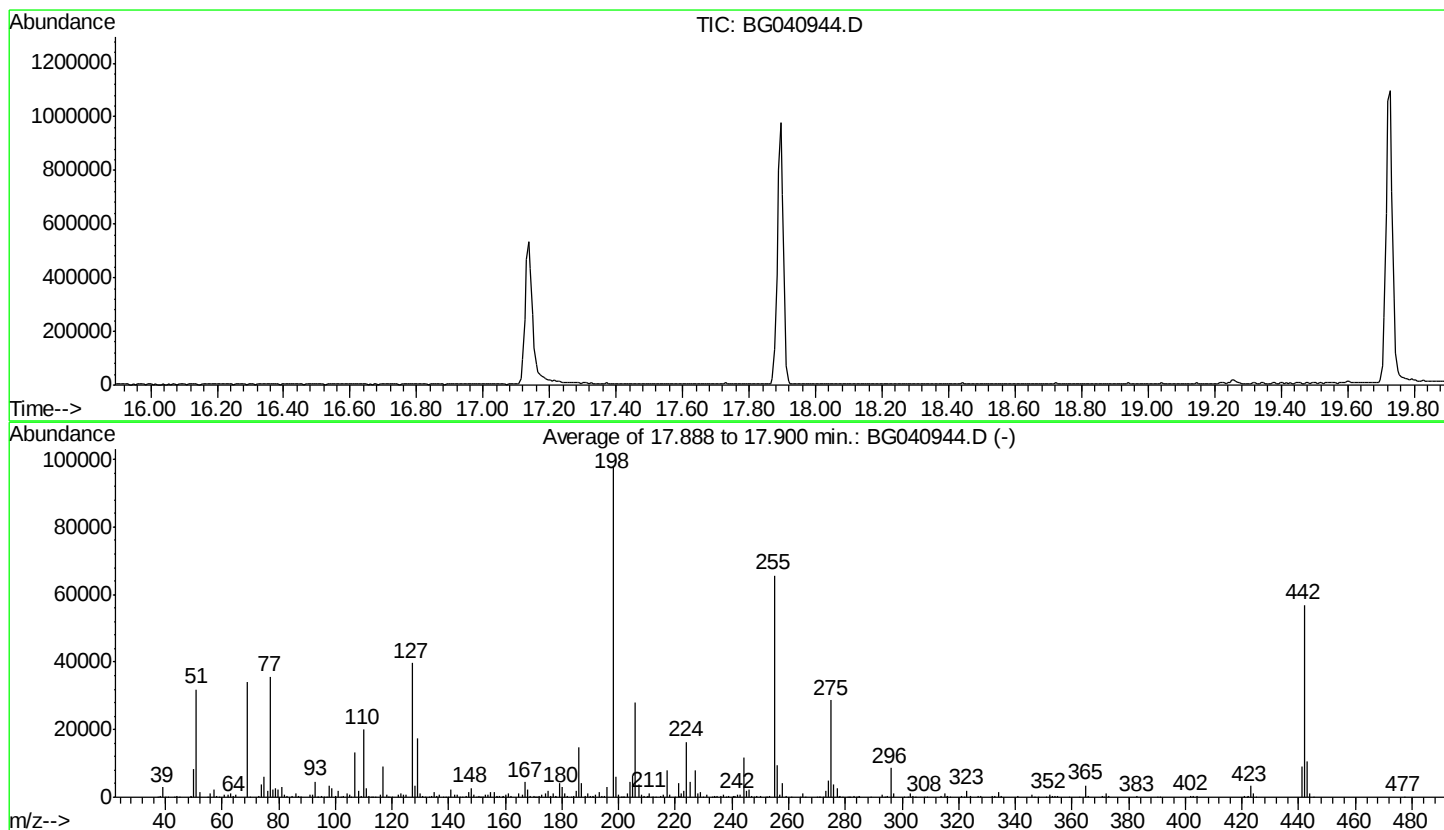

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	31989	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.8	34178	PASS
70	69	0.00	2	0.4	128	PASS
127	198	10	80	40.4	39669	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98136	PASS
199	198	5	9	6.3	6153	PASS
275	198	10	60	29.3	28720	PASS
365	198	1	100	3.5	3447	PASS
441	198	0.01	100	9.4	9271	PASS
442	198	50	100	58.1	57016	PASS
443	442	15	24	18.5	10561	PASS