


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG053019\
 Data File : BG040955.D
 Acq On : 30 May 2019 18:17
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 18:39:57 2019

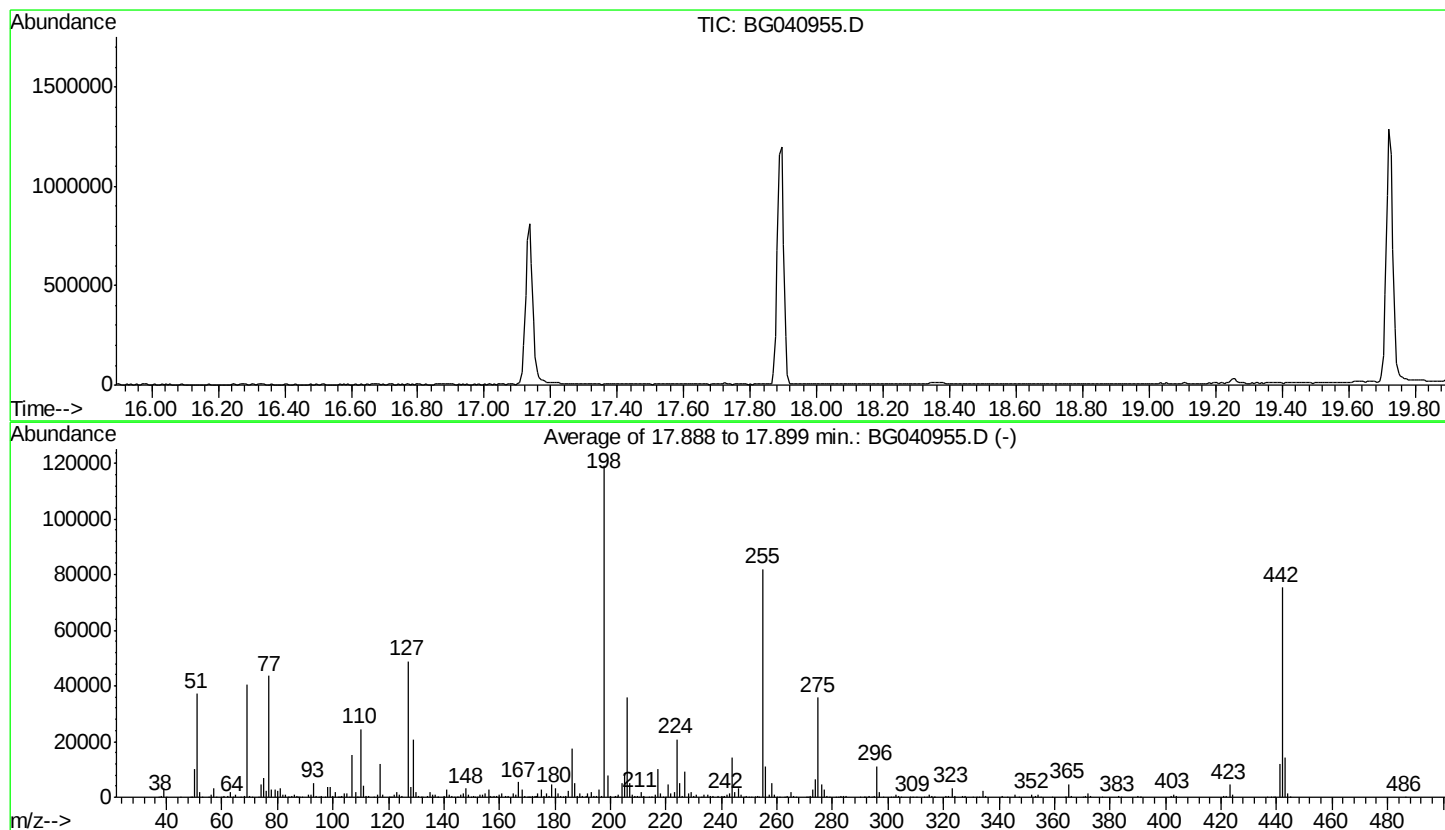

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	37269	PASS
68	69	0.00	2	1.1	449	PASS
69	198	0.00	100	34.1	40639	PASS
70	69	0.00	2	0.8	317	PASS
127	198	10	80	41.0	48880	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	119213	PASS
199	198	5	9	6.7	7928	PASS
275	198	10	60	30.0	35778	PASS
365	198	1	100	4.0	4785	PASS
441	198	0.01	100	9.9	11827	PASS
442	198	50	100	63.1	75258	PASS
443	442	15	24	18.9	14207	PASS