
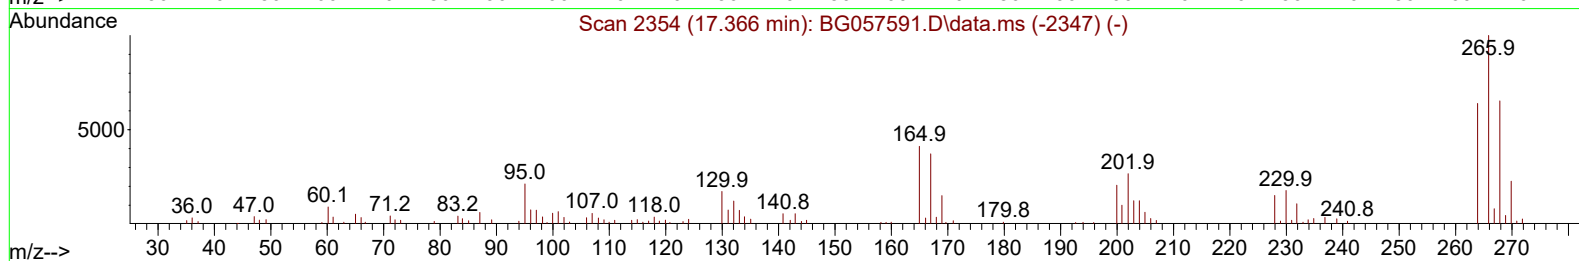
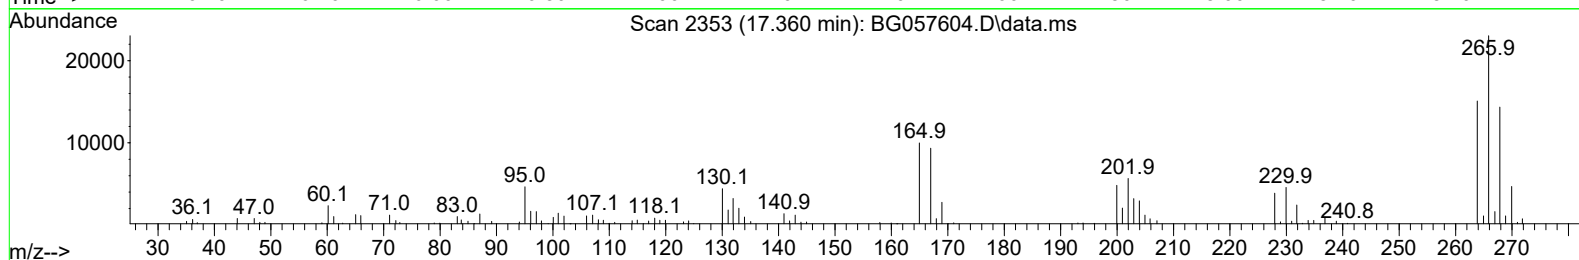


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053023\
Data File : BG057604.D
Acq On : 30 May 2023 12:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 08:14:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 03:25:39 2023
Response via : Initial Calibration

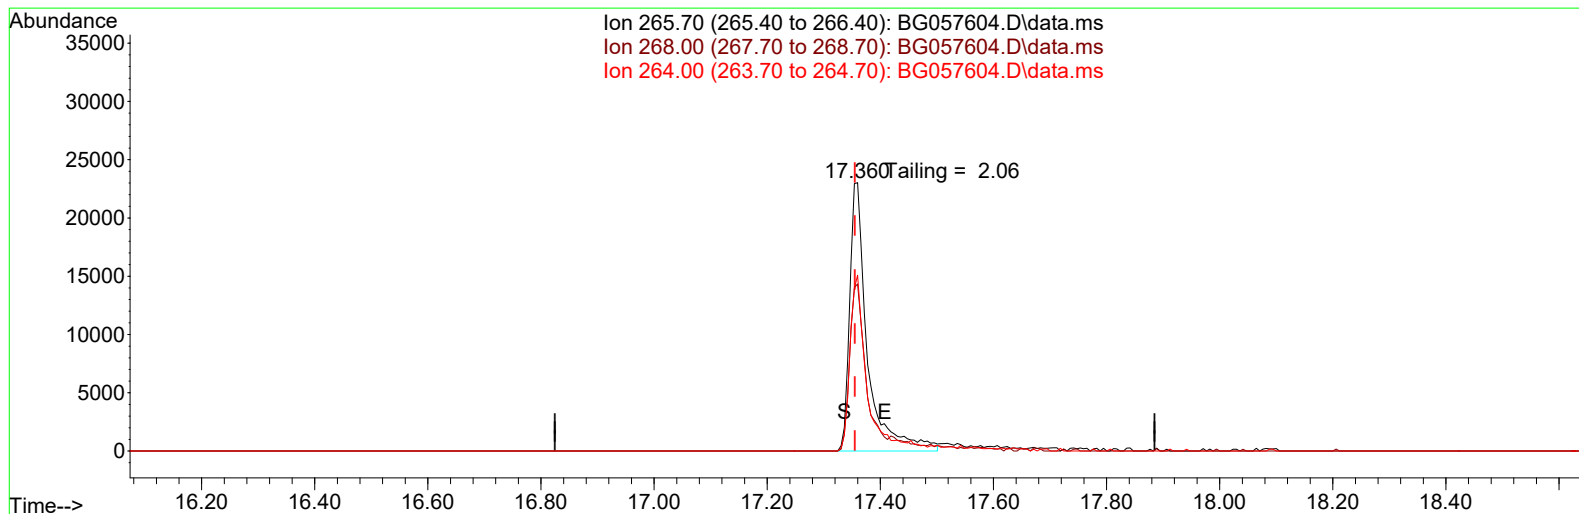

TIC: BG057604.D\data.ms

(70) Pentachlorophenol (C)




17.360min (+ 0.005) 31179.61 ng

response 49048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.27
264.00	64.00	65.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053023\
Data File : BG057604.D
Acq On : 30 May 2023 12:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 08:14:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 03:25:39 2023
Response via : Initial Calibration

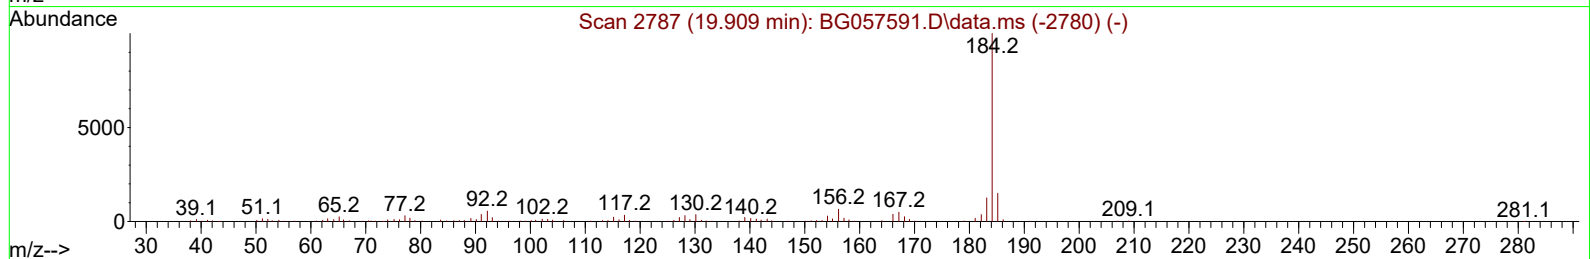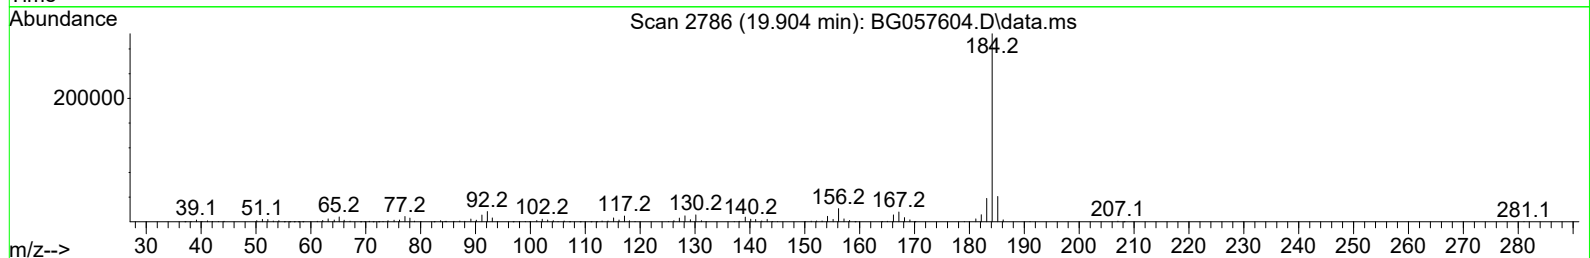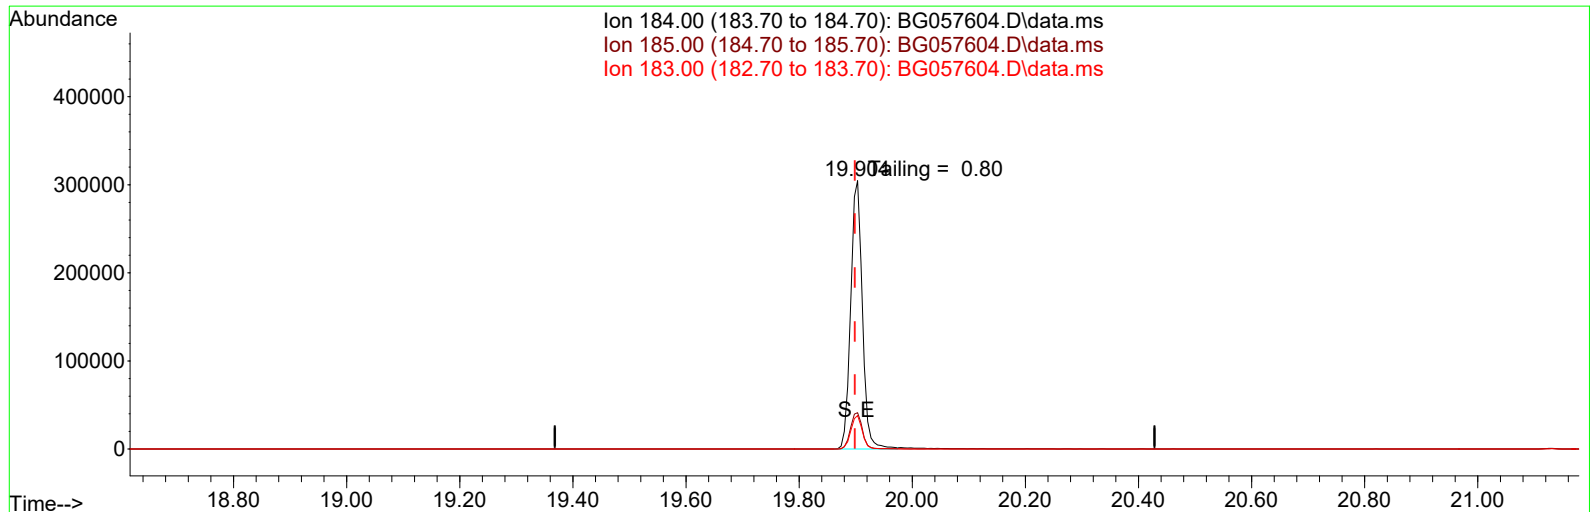

TIC: BG057604.D\data.ms

(77) Benzidine

19.904min (+ 0.005) 0.00 ng

response 442538

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.52
183.00	12.50	12.49
0.00	0.00	0.00