

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053023\
 Data File : BG057611.D
 Acq On : 30 May 2023 18:10
 Operator : CG/JU
 Sample : 02955-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC26

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057611.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.371	303	312	318	rBV	10617	17094	1.32%	0.247%
2	5.858	388	395	411	rBV	261815	442063	34.04%	6.399%
3	7.485	665	672	684	rBV	291545	528414	40.69%	7.649%
4	8.337	811	817	828	rVB	75291	123920	9.54%	1.794%
5	9.518	1011	1018	1030	rBV	172400	311727	24.01%	4.512%
6	11.175	1294	1300	1309	rBV	105005	185967	14.32%	2.692%
7	13.583	1703	1710	1717	rVB	468343	726755	55.97%	10.520%
8	14.958	1934	1944	1951	rBV	194415	301516	23.22%	4.364%
9	16.291	2164	2171	2177	rVB	40380	58047	4.47%	0.840%
10	16.438	2190	2196	2209	rBV	474779	733425	56.48%	10.616%
11	17.695	2404	2410	2415	rBV	290203	418602	32.24%	6.059%
12	17.736	2415	2417	2423	rVB	24267	30500	2.35%	0.441%
13	18.529	2547	2552	2562	rBV4	37620	72263	5.56%	1.046%
14	18.606	2562	2565	2572	rVB	12489	18214	1.40%	0.264%
15	19.728	2751	2756	2761	rVB	76337	107088	8.25%	1.550%
16	20.051	2806	2811	2814	rBV2	12568	23038	1.77%	0.333%
17	20.086	2814	2817	2823	rVB	71770	102125	7.86%	1.478%
18	20.262	2841	2847	2852	rBV	1017022	1298547	100.00%	18.797%
19	21.555	3063	3067	3079	rBV4	46490	114662	8.83%	1.660%
20	21.819	3108	3112	3116	rBV2	10946	18960	1.46%	0.274%
21	21.995	3134	3142	3147	rBV3	271071	527796	40.65%	7.640%
22	22.048	3148	3151	3158	rVB	40999	64985	5.00%	0.941%
23	23.070	3321	3325	3332	rBV10	12211	26620	2.05%	0.385%
24	24.363	3540	3545	3553	rBV2	40669	119717	9.22%	1.733%
25	25.314	3702	3707	3715	rVB	34198	83050	6.40%	1.202%
26	25.485	3726	3736	3745	rBV	149194	439288	33.83%	6.359%
27	29.497	4415	4419	4420	rBV4	9630	13992	1.08%	0.203%




Sum of corrected areas: 6908375

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053023\
Data File : BG057611.D
Acq On : 30 May 2023 18:10
Operator : CG/JU
Sample : 02955-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC26

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

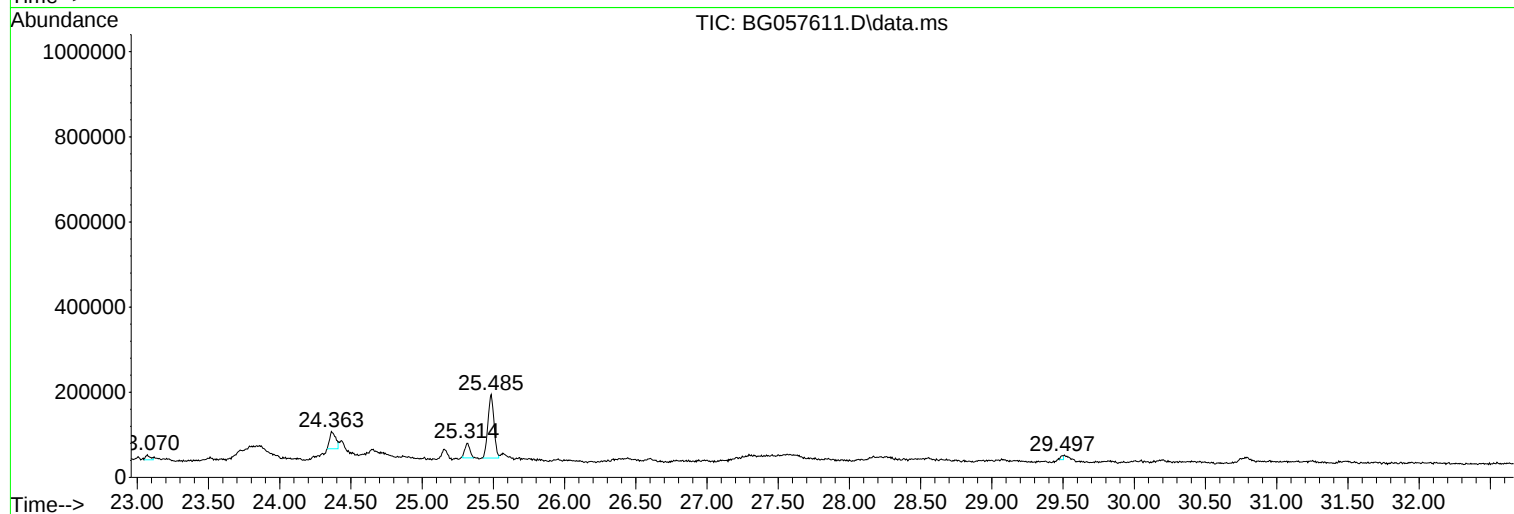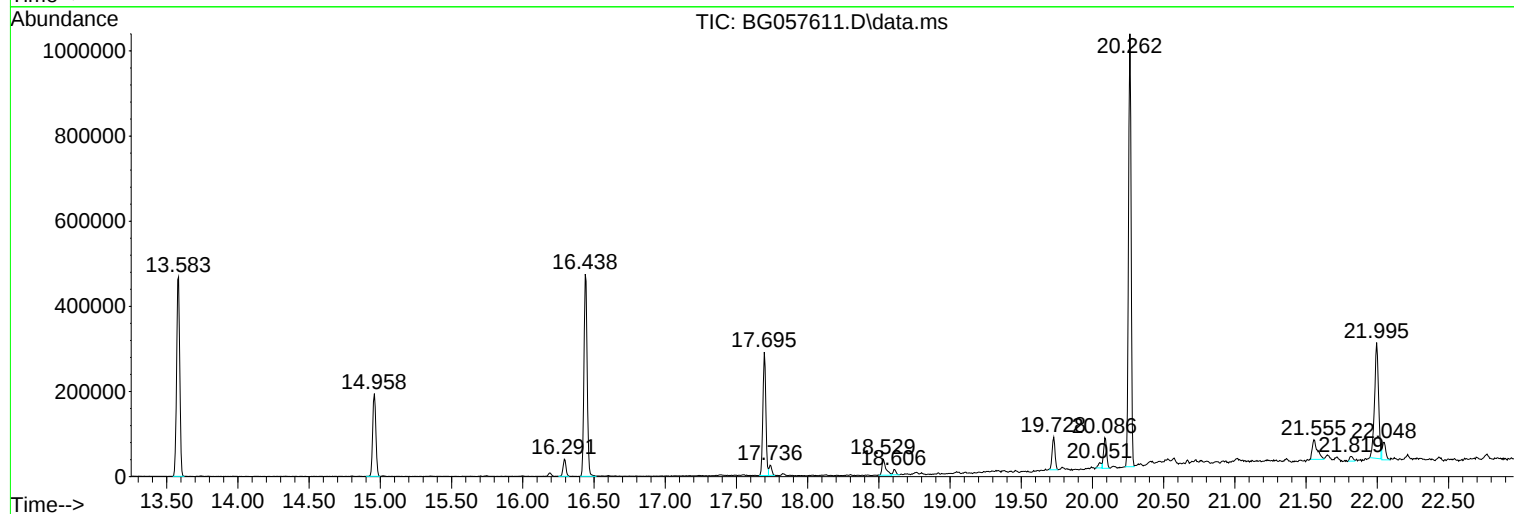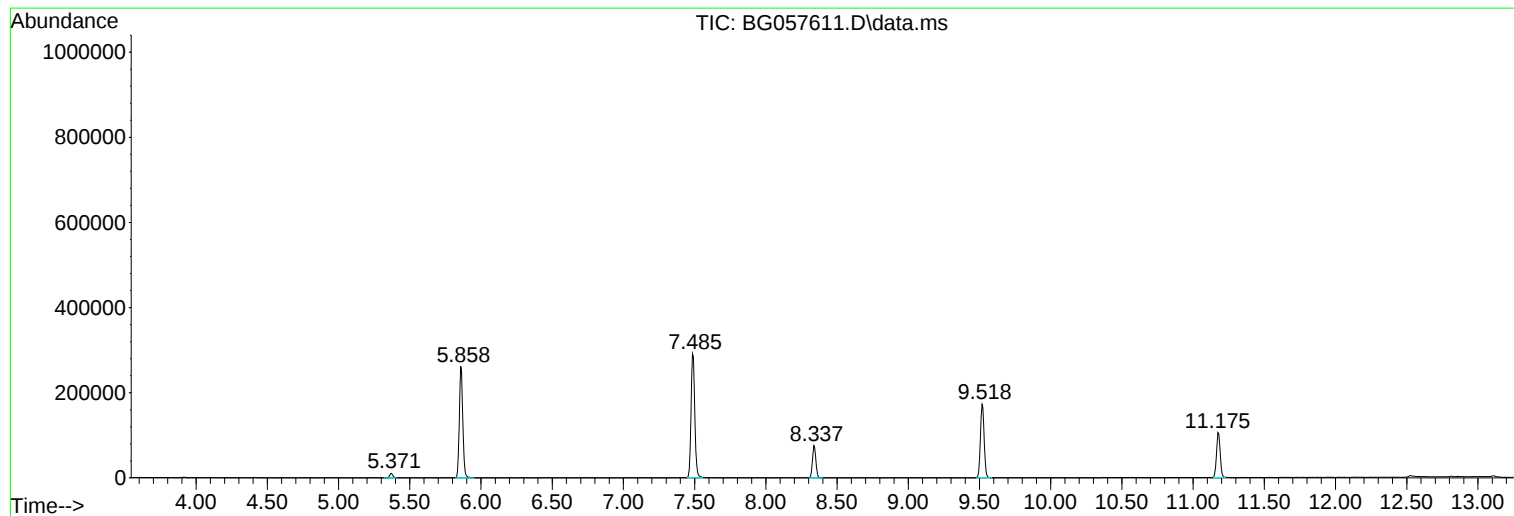

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053023\
Data File : BG057611.D
Acq On : 30 May 2023 18:10
Operator : CG/JU
Sample : 02955-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC26

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053023\
Data File : BG057611.D
Acq On : 30 May 2023 18:10
Operator : CG/JU
Sample : 02955-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC26

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------