
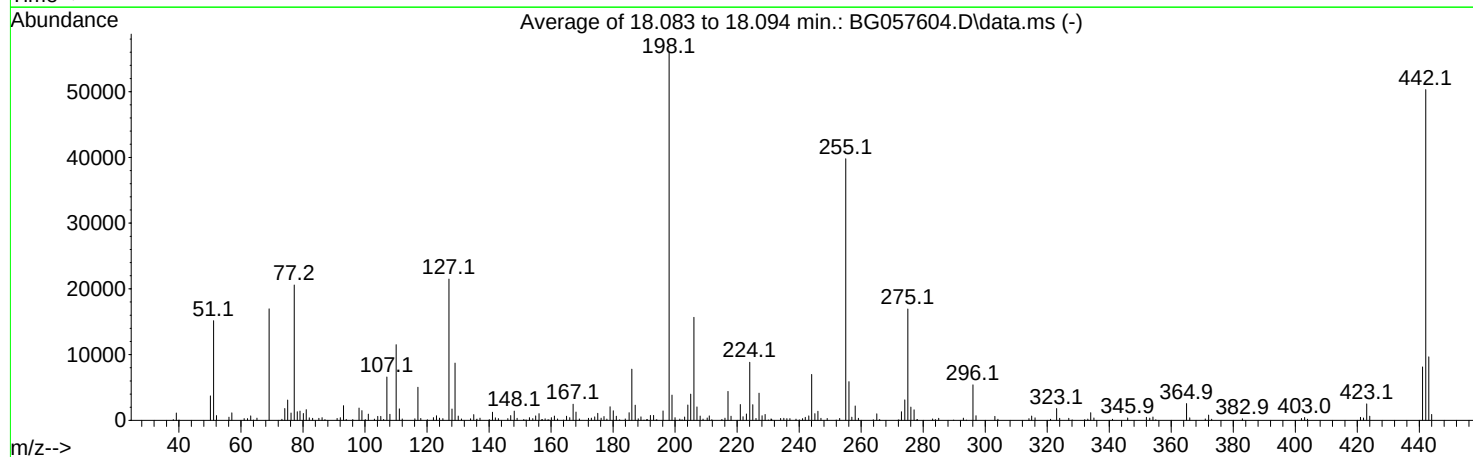


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053023\
 Data File : BG057604.D
 Acq On : 30 May 2023 12:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 31 03:25:39 2023

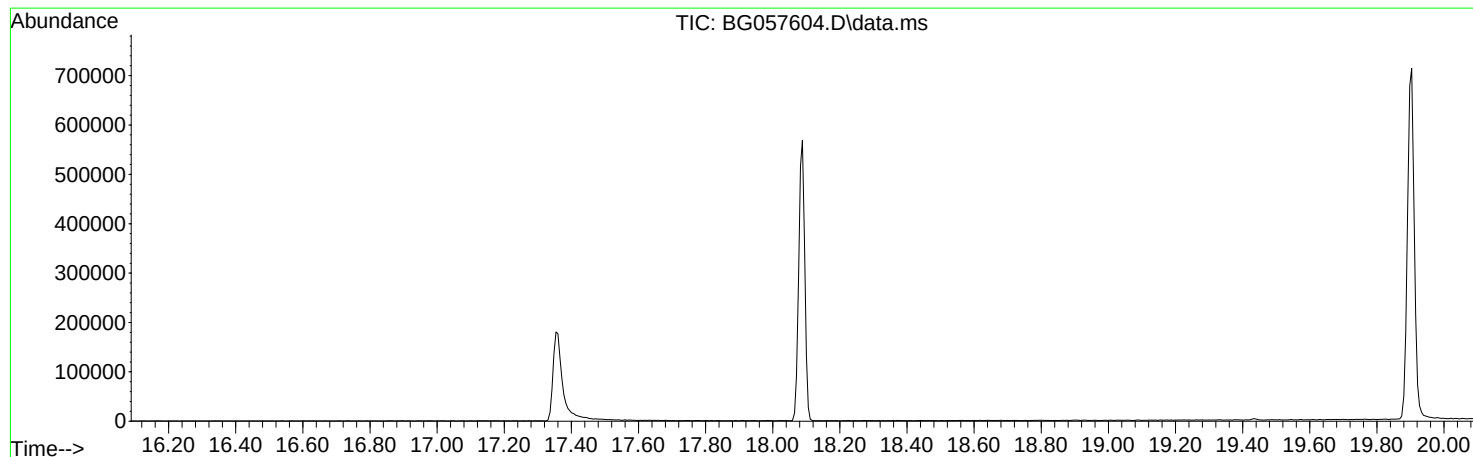

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	15154	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.3	16963	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.4	21484	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55957	PASS
199	198	5	9	6.9	3843	PASS
275	198	10	60	30.3	16950	PASS
365	198	1	100	4.6	2554	PASS
441	198	0.01	100	14.5	8138	PASS
442	442	50	100	100.0	50301	PASS
443	442	15	24	19.2	9660	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/30/2023	BNA_G	<u>BG057604.D</u>
Compound Name	Response	Retention Time
DDT	212990	21.131
DDD	4203	20.726
DDE	315	20.18
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4518	217508	2.08

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053023\
Data File : BG057604.D
Acq On : 30 May 2023 12:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 31 08:14:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 03:25:39 2023
Response via : Initial Calibration

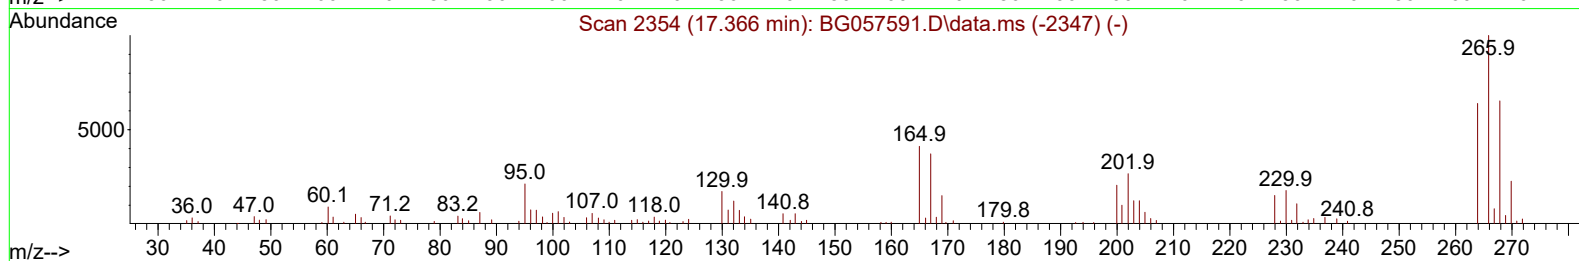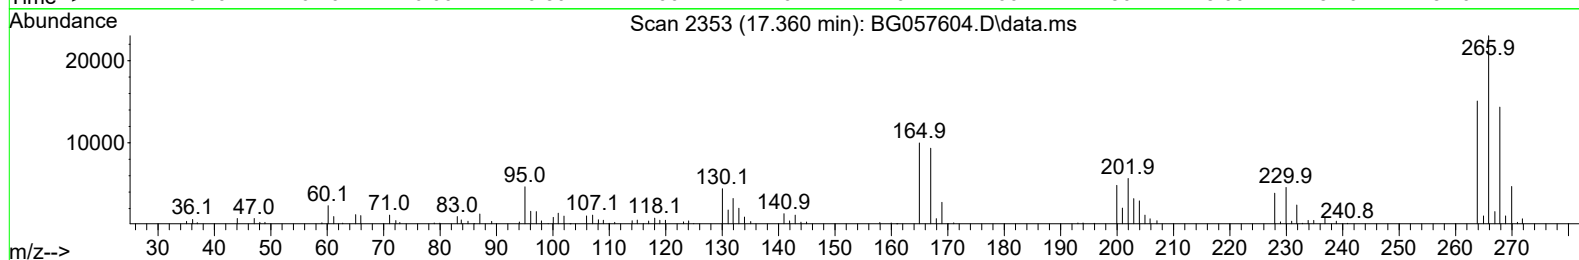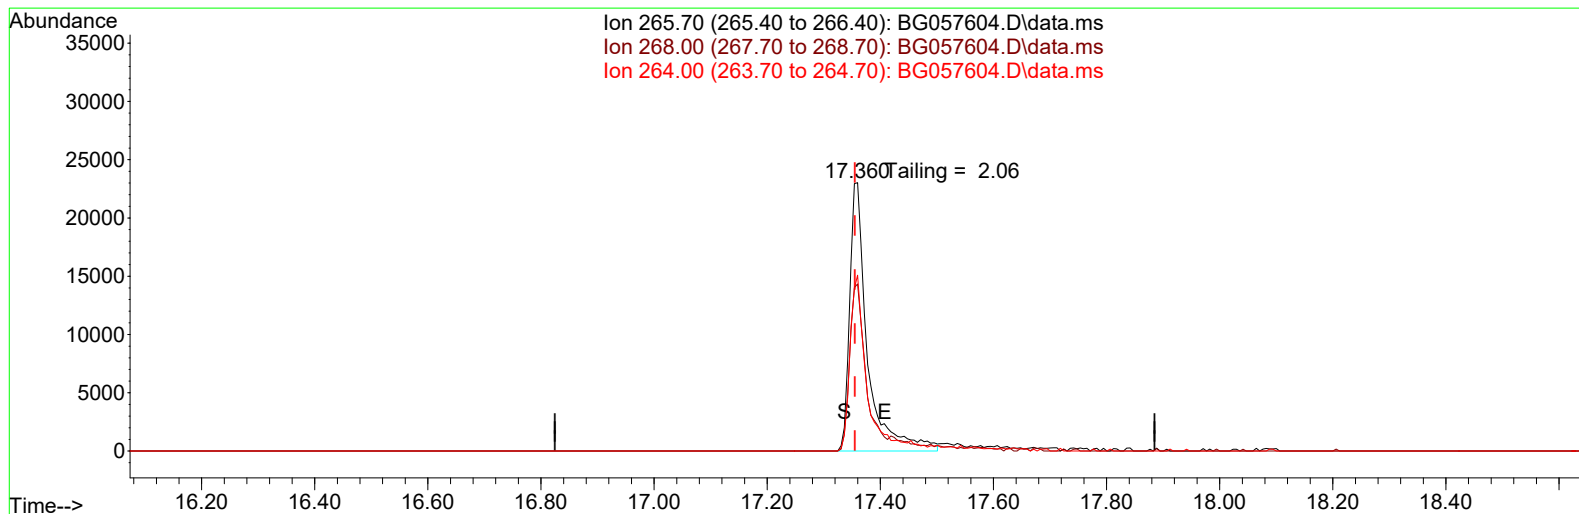

TIC: BG057604.D\data.ms

(70) Pentachlorophenol (C)

17.360min (+ 0.005) 31179.61 ng




response 49048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.27
264.00	64.00	65.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053023\
Data File : BG057604.D
Acq On : 30 May 2023 12:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 31 08:14:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 03:25:39 2023
Response via : Initial Calibration

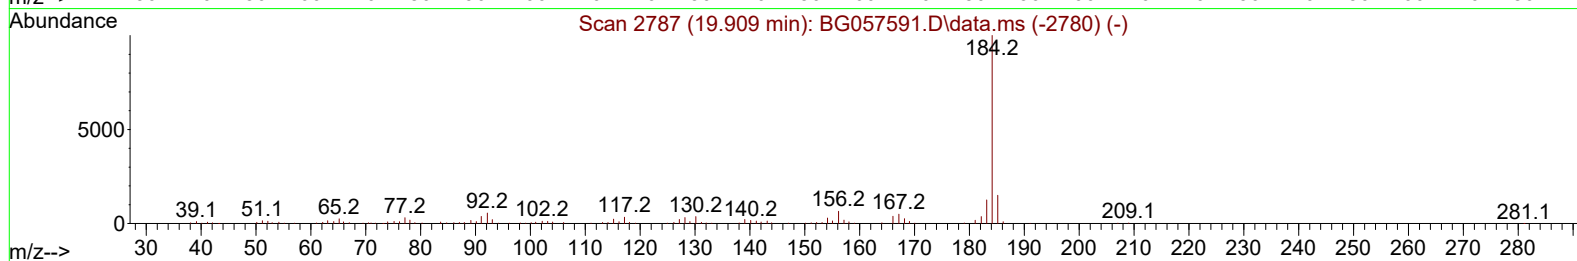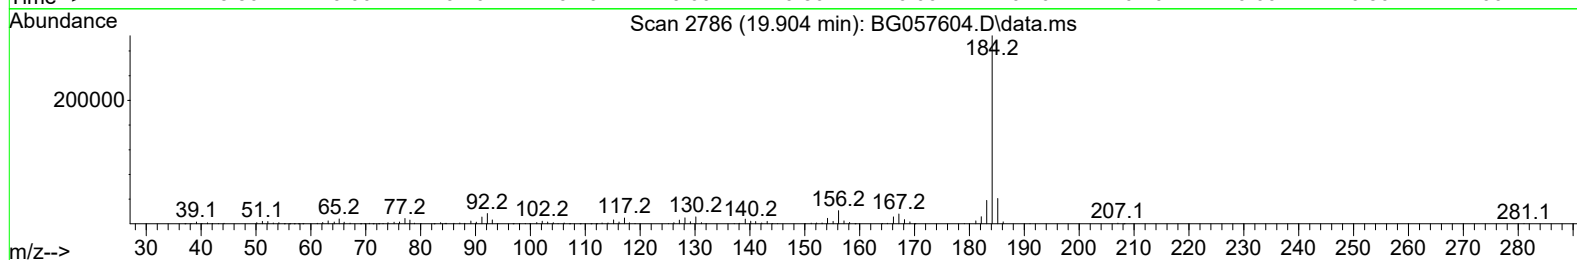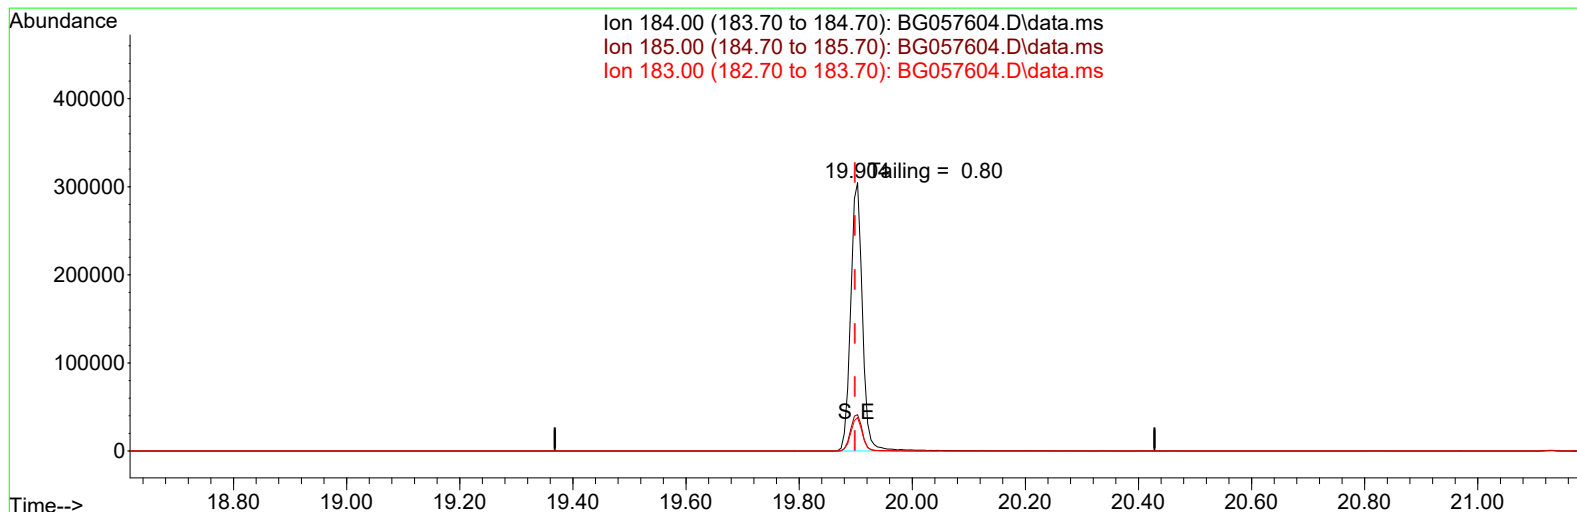

TIC: BG057604.D\data.ms

(77) Benzidine

19.904min (+ 0.005) 0.00 ng

response 442538

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.52
183.00	12.50	12.49
0.00	0.00	0.00