


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053119\
 Data File : BG040974.D
 Acq On : 31 May 2019 10:09
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 18:39:57 2019

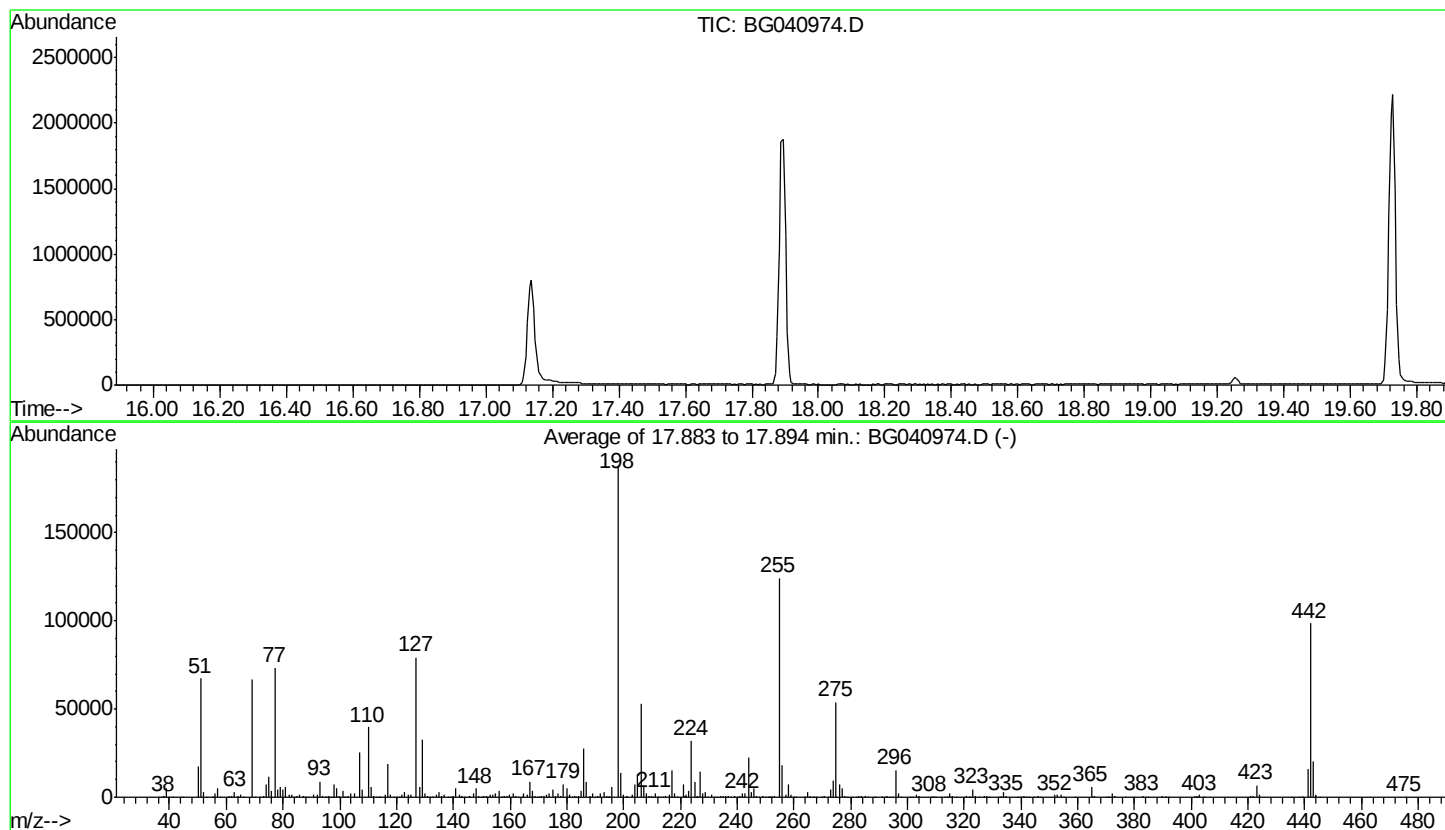

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	67325	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.7	67146	PASS
70	69	0.00	2	0.4	276	PASS
127	198	10	80	42.2	79432	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	188026	PASS
199	198	5	9	7.2	13575	PASS
275	198	10	60	28.7	53930	PASS
365	198	1	100	3.1	5911	PASS
441	198	0.01	100	8.4	15819	PASS
442	198	50	100	52.3	98410	PASS
443	442	15	24	20.7	20348	PASS