

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060119\
 Data File : BG041008.D
 Acq On : 1 Jun 2019 12:21
 Operator : HP/JU
 Sample : PB120099BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB120099BL

Quant Time: Jun 03 02:29:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 29 18:39:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	53206	20.00	ng	-0.01
21) Naphthalene-d8	10.95	136	221541	20.00	ng	0.00
39) Acenaphthene-d10	14.75	164	158534	20.00	ng	-0.01
64) Phenanthrene-d10	17.49	188	400876	20.00	ng	-0.01
76) Chrysene-d12	21.77	240	404651	20.00	ng	-0.01
87) Perylene-d12	25.12	264	418505	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	283572	96.11	ng	0.00
7) Phenol-d6	7.26	99	398355	87.42	ng	0.00
23) Nitrobenzene-d5	9.29	82	416657	83.49	ng	-0.01
42) 2,4,6-Tribromophenol	16.23	330	188806	80.22	ng	-0.01
45) 2-Fluorobiphenyl	13.37	172	980060	89.03	ng	-0.01
79) Terphenyl-d14	20.09	244	1553419	81.47	ng	-0.01


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060119\
Data File : BG041008.D
Acq On : 1 Jun 2019 12:21
Operator : HP/JU
Sample : PB120099BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120099BL

Quant Time: Jun 03 02:29:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 29 18:39:57 2019
Response via : Initial Calibration

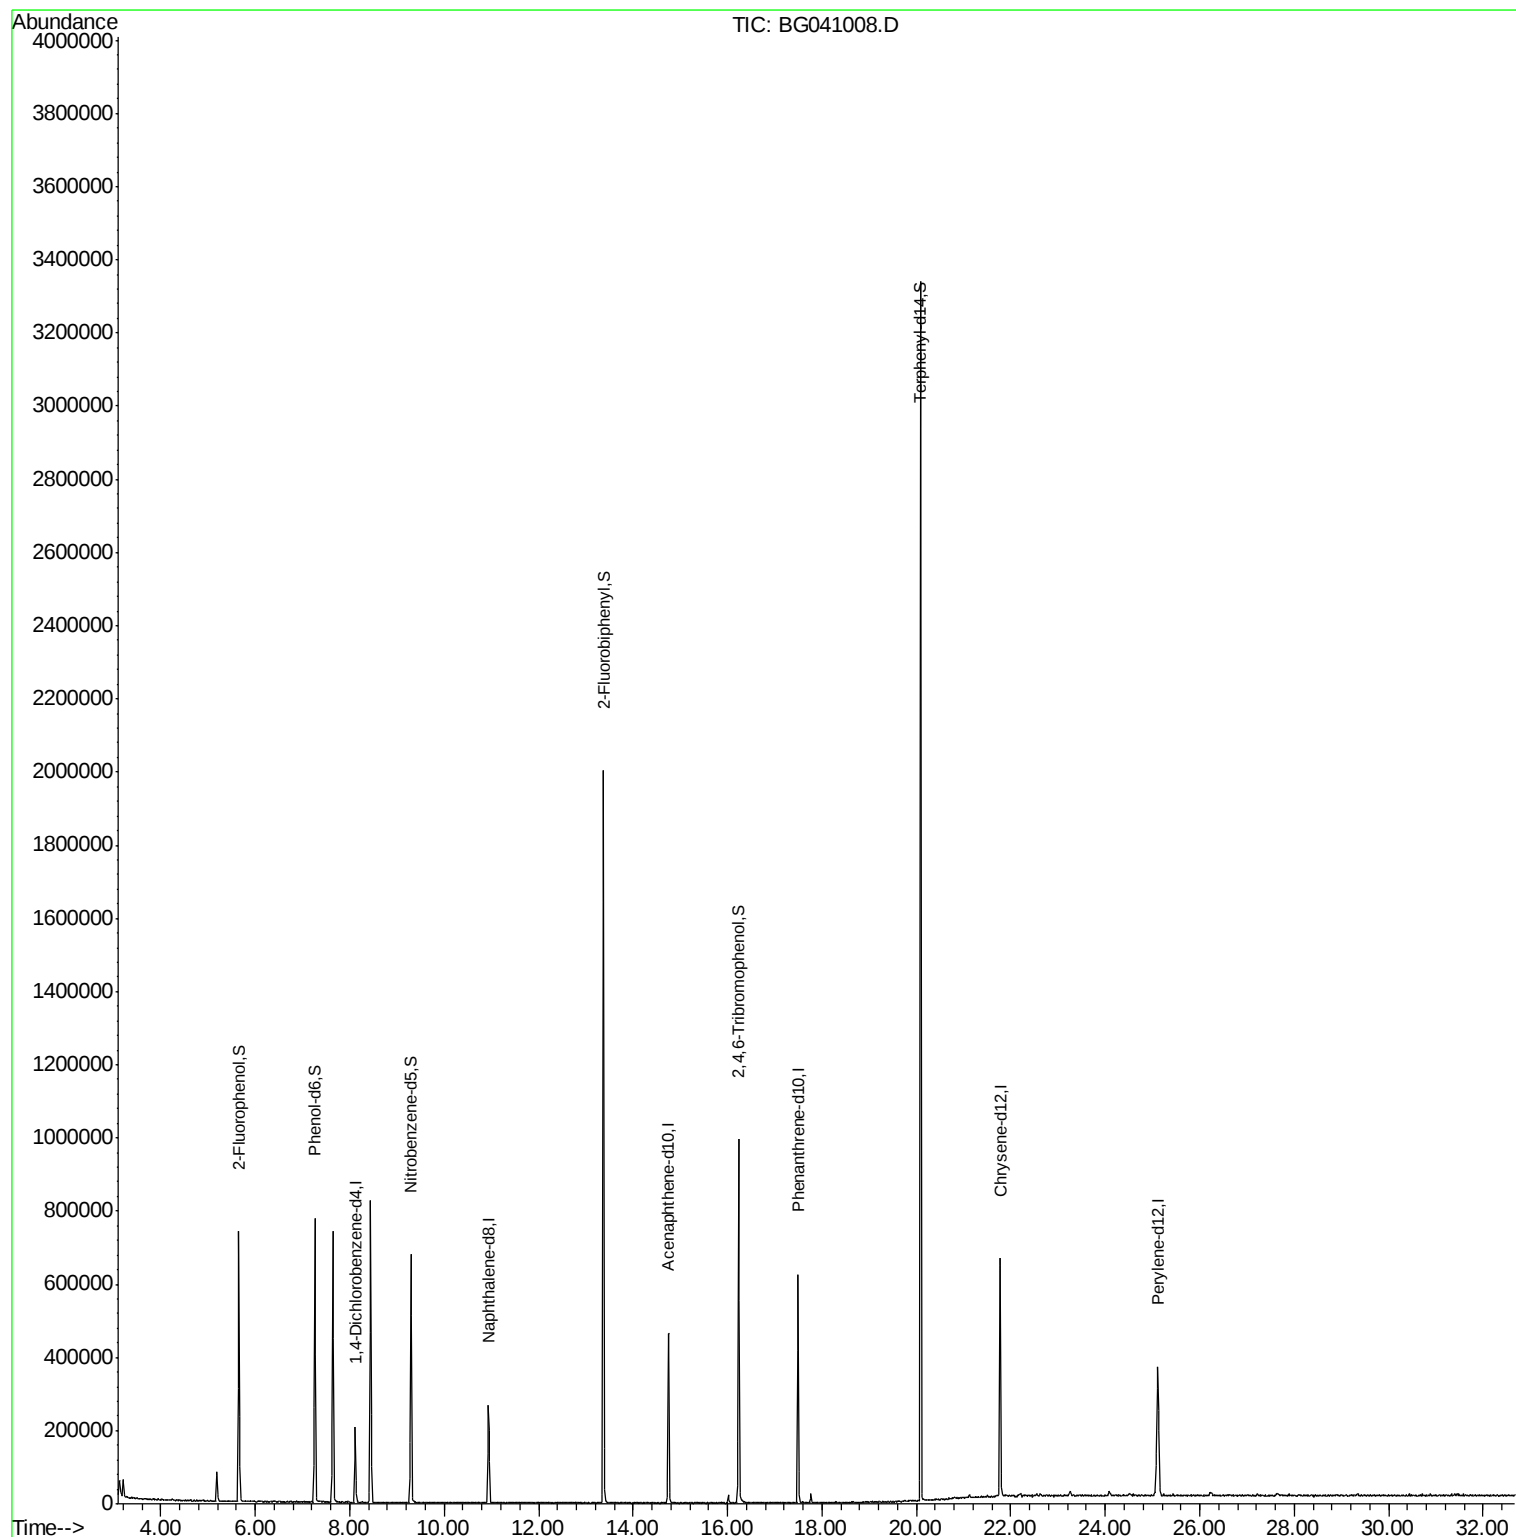







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.12 min Scan# 856
Delta R.T. -0.01 min
Lab File: BG041008.D
Acq: 1 Jun 2019 12:21

Instrument :
BNA_G
ClientSampleId :
PB120099BL




Tot Ion	Ratio	Lower	Upper
152	100		
150	154.5	120.6	180.8
115	68.0	45.1	67.7#

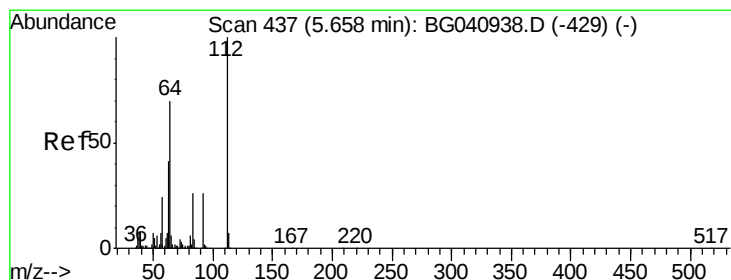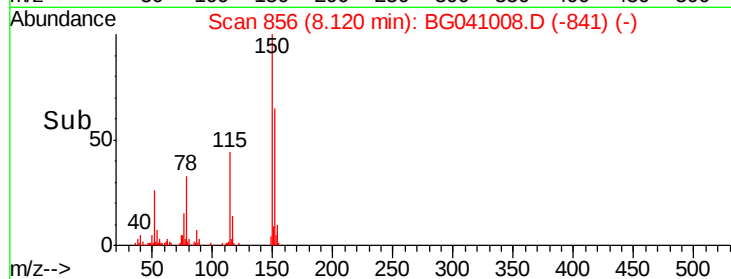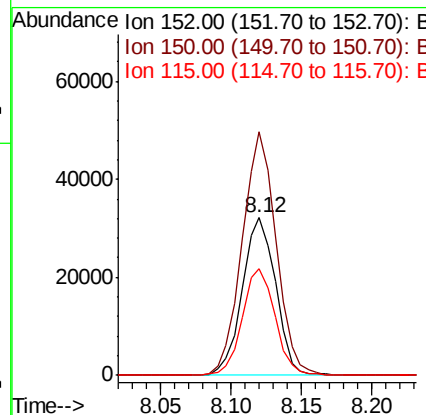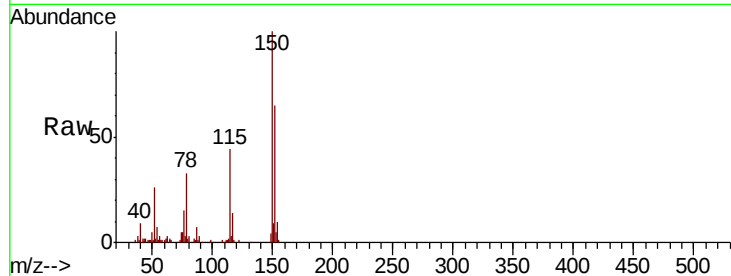

#5

2-Fluorophenol
Concen: 96.106 ng
RT: 5.65 min Scan# 436
Delta R.T. -0.01 min
Lab File: BG041008.D
Acq: 1 Jun 2019 12:21

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.9	56.2	84.2
63	42.3	32.8	49.2

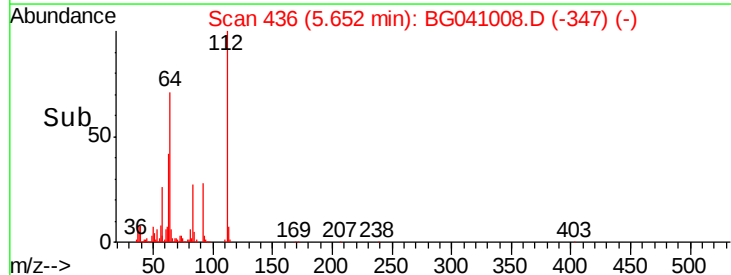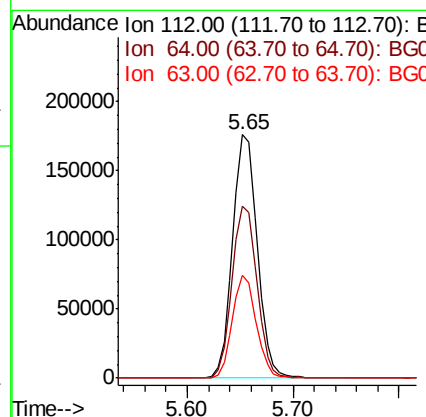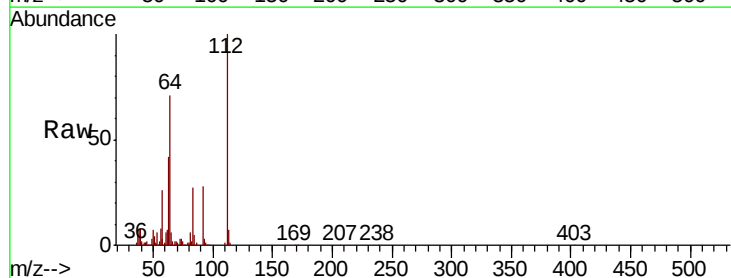



#7

Phenol-d6

Concen: 87.417 ng

RT: 7.26 min Scan# 710

Delta R.T. -0.01 min

Lab File: BG041008.D

Acq: 1 Jun 2019 12:21

Instrument :

BNA_G

ClientSampleId :

PB120099BL


Tot Ion: 99 Resp: 398355

Ion Ratio Lower Upper




99 100

42 24.8 17.9 26.9

71 44.4 35.4 53.0

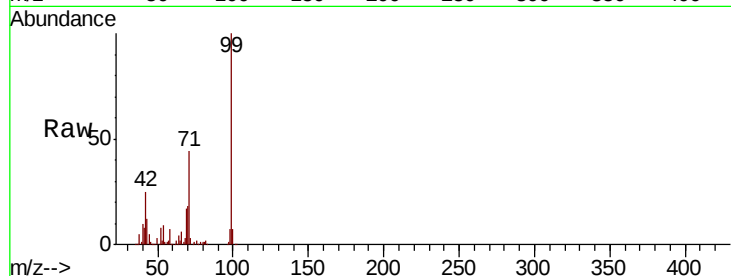

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

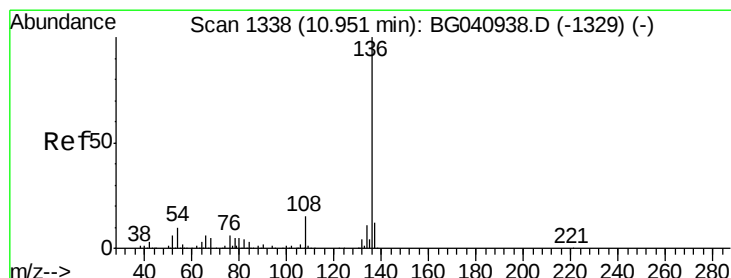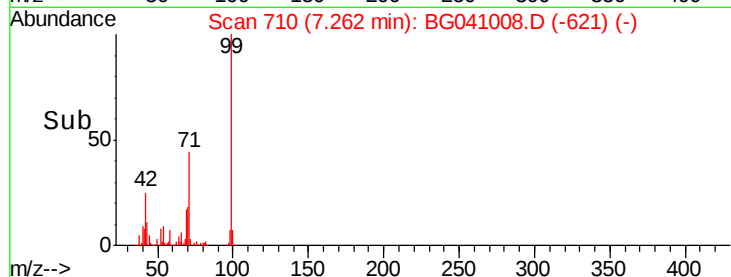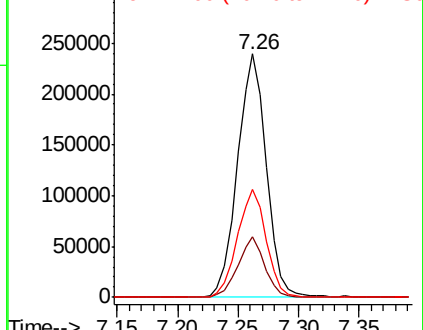

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.95 min Scan# 1337

Delta R.T. -0.01 min

Lab File: BG041008.D

Acq: 1 Jun 2019 12:21

Tgt Ion: 136 Resp: 221541


Ion Ratio Lower Upper

136 100



137 10.5 9.5 14.3

54 9.1 7.6 11.4

68 4.5 3.9 5.9

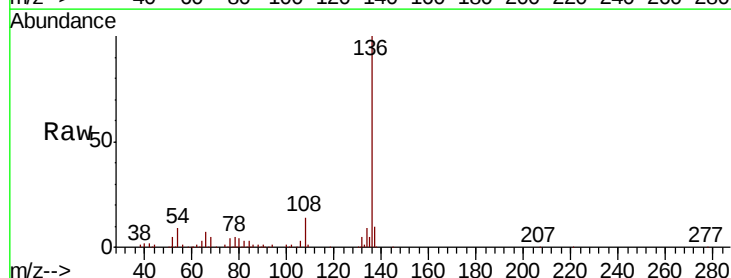

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



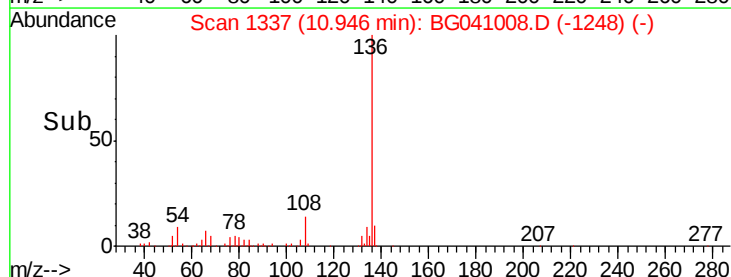
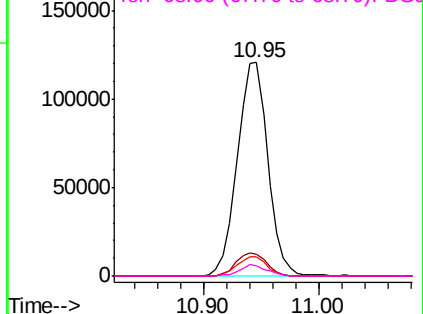




#23
Nitrobenzene-d5
Concen: 83.492 ng
RT: 9.29 min Scan# 1056
Delta R.T. -0.01 min
Lab File: BG041008.D
Acq: 1 Jun 2019 12:21




Instrument :
BNA_G
ClientSampleId :
PB120099BL


Tot Ion	82	Resp	416657
Ion Ratio	Lower	Upper	
82	100		
128	35.7	30.5	45.7
54	57.3	44.6	66.8

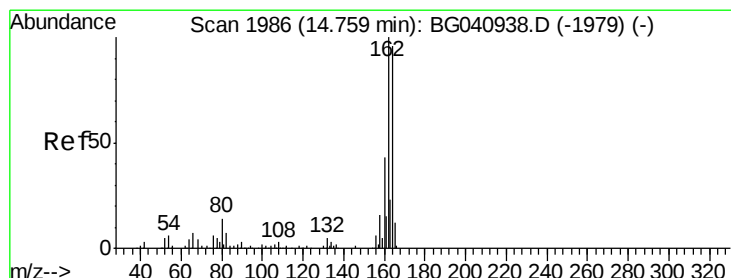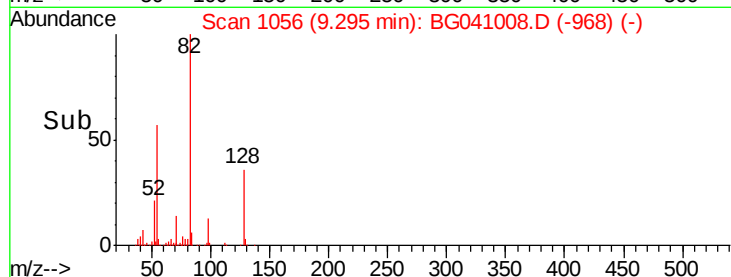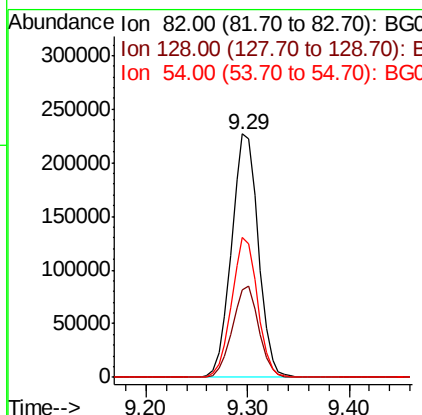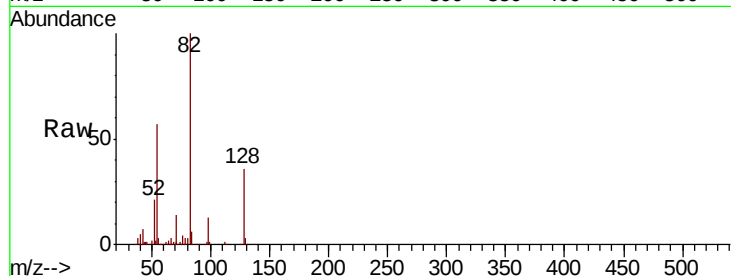

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.75 min Scan# 1984
Delta R.T. -0.01 min
Lab File: BG041008.D
Acq: 1 Jun 2019 12:21

Tgt Ion	164	Resp	158534
Ion Ratio	Lower	Upper	
164	100		
162	110.1	83.0	124.4
160	44.2	35.6	53.4

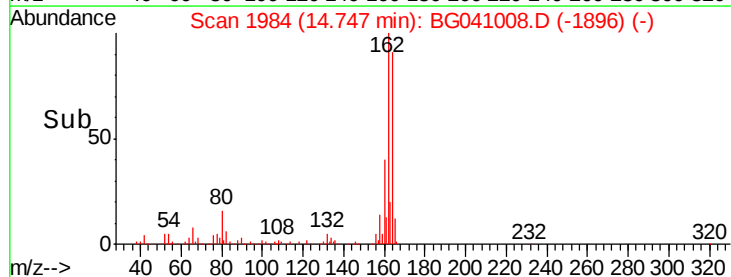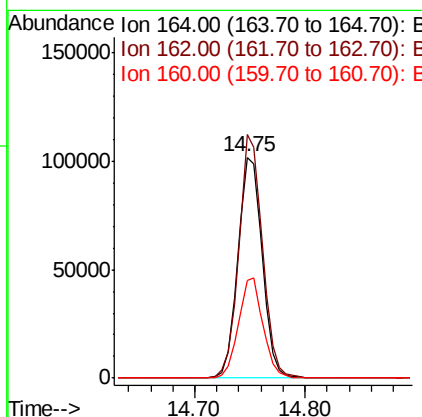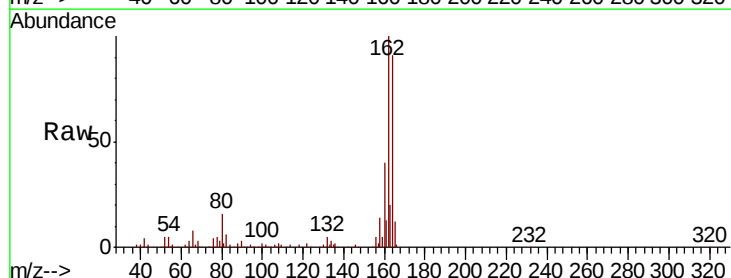


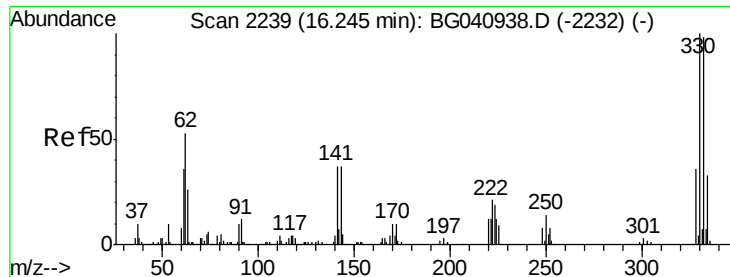

#42
 2,4,6-Tribromophenol
 Concen: 80.222 ng
 RT: 16.23 min Scan# 2237
 Delta R.T. -0.01 min
 Lab File: BG041008.D
 Acq: 1 Jun 2019 12:21

Instrument :
 BNA_G
 ClientSampleId :
 PB120099BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	78.5	117.7
141	36.3	28.7	43.1



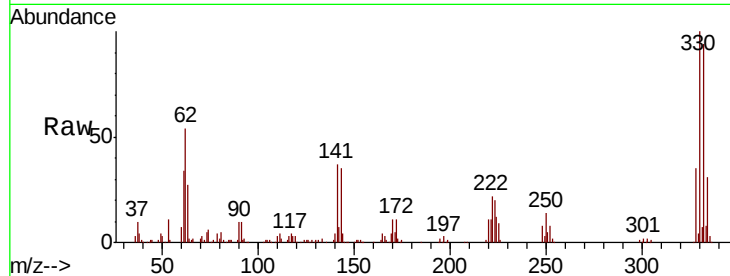


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

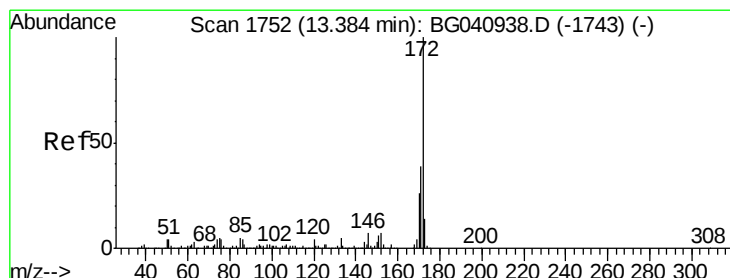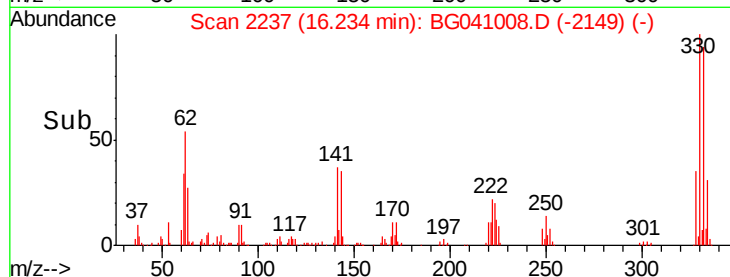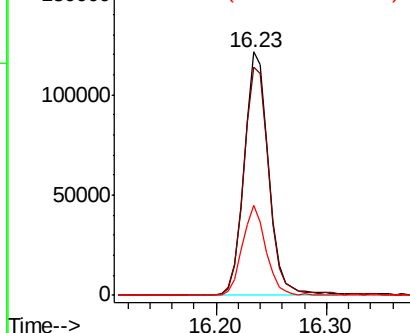

#45
 2-Fluorobiphenyl
 Concen: 89.028 ng
 RT: 13.37 min Scan# 1750
 Delta R.T. -0.01 min
 Lab File: BG041008.D
 Acq: 1 Jun 2019 12:21

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.8	31.1	46.7
170	26.4	20.5	30.7


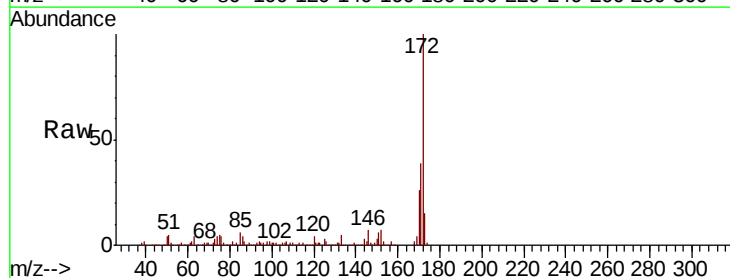



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

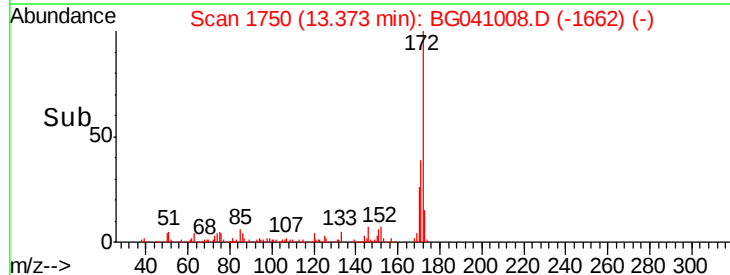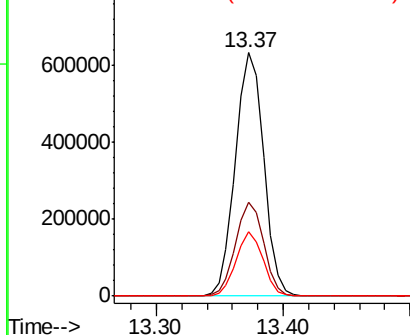


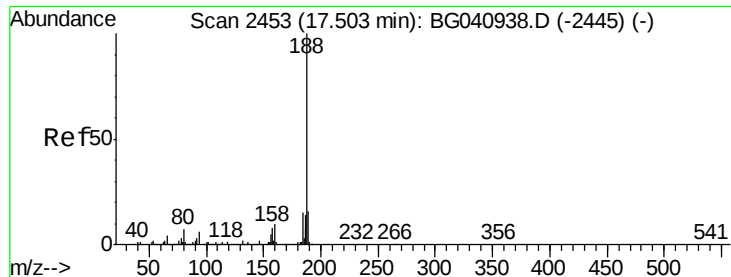




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.49 min Scan# 2451
Delta R.T. -0.01 min
Lab File: BG041008.D
Acq: 1 Jun 2019 12:21

Instrument :
BNA_G
ClientSampleId :
PB120099BL

Tot Ion:188 Resp: 400876
Ion Ratio Lower Upper
188 100
94 5.7 4.7 7.1
80 7.2 5.8 8.8

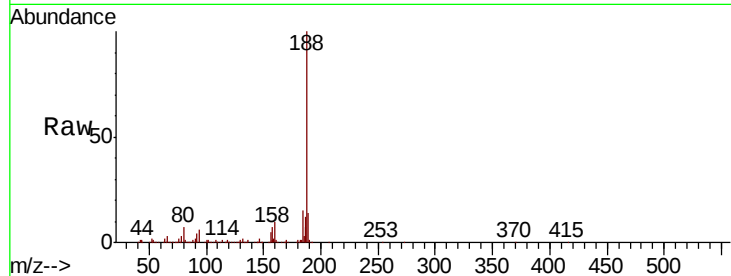


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

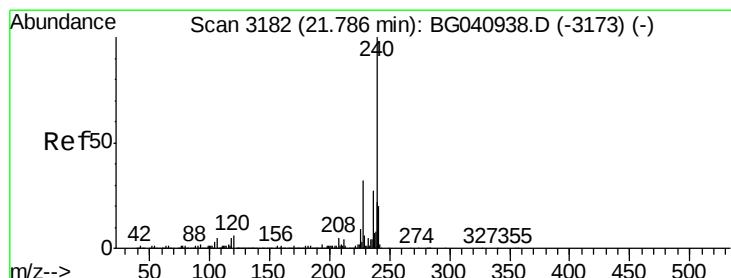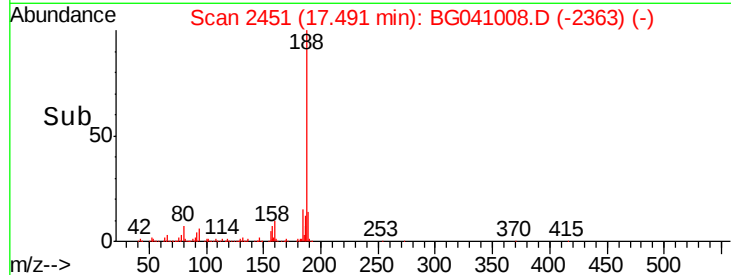
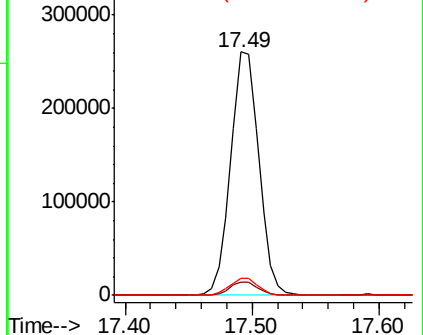



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.77 min Scan# 3180
Delta R.T. -0.01 min
Lab File: BG041008.D
Acq: 1 Jun 2019 12:21

Tgt Ion:240 Resp: 404651
Ion Ratio Lower Upper
240 100
120 5.2 4.5 6.7
236 26.5 21.3 31.9

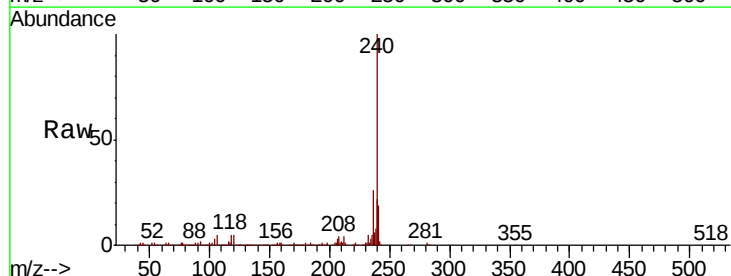

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

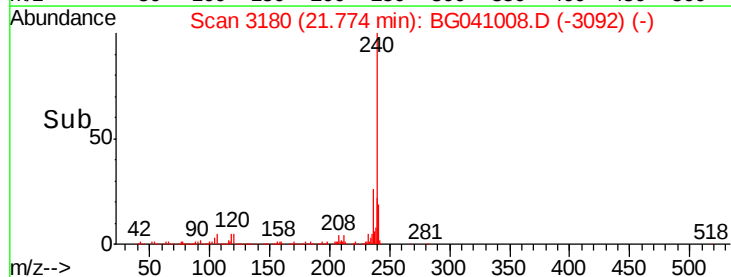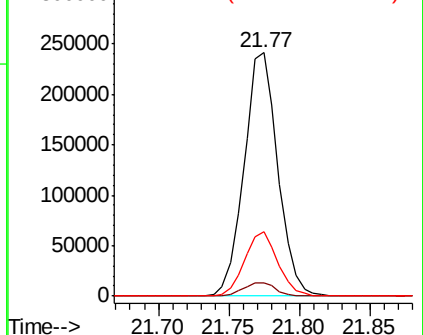

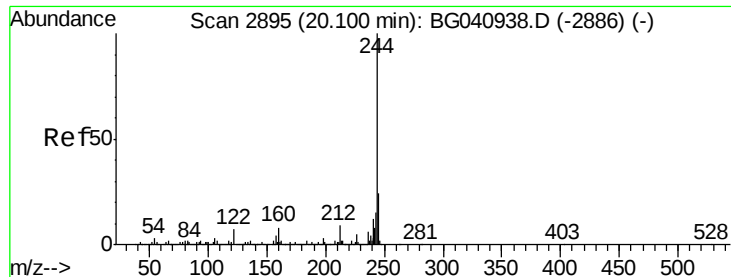

#79

Terphenyl-d14

Concen: 81.475 ng

RT: 20.09 min Scan# 2893

Delta R.T. -0.01 min

Lab File: BG041008.D

Acq: 1 Jun 2019 12:21

Instrument :

BNA_G

ClientSampleId :

PB120099BL


Tot Ion:244 Resp: 1553419

Ion Ratio Lower Upper




244 100

212 8.9 7.0 10.4

122 7.4 5.4 8.0

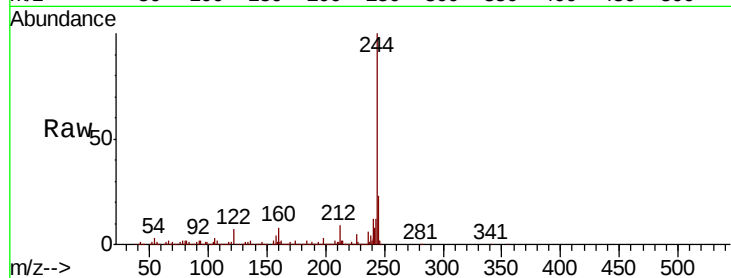

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

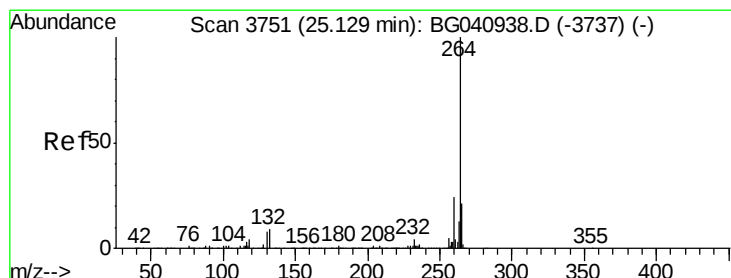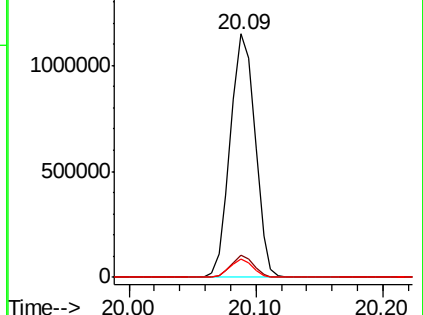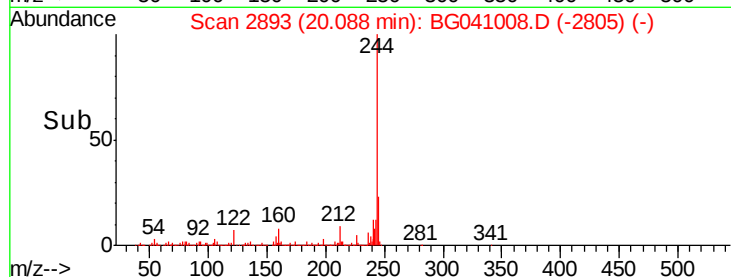

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.12 min Scan# 3749

Delta R.T. -0.01 min

Lab File: BG041008.D

Acq: 1 Jun 2019 12:21


Tgt Ion:264 Resp: 418505

Ion Ratio Lower Upper

264 100

260 23.0 19.0 28.4

265 22.8 17.0 25.4

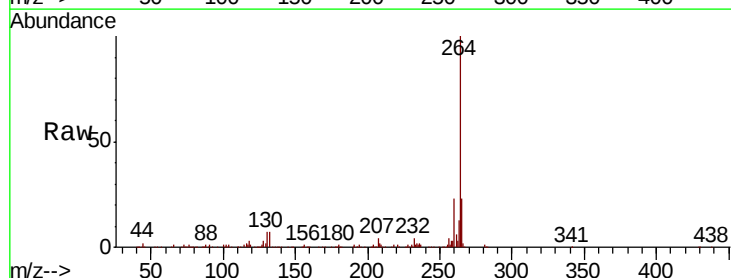

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

