


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060119\
 Data File : BG041004.D
 Acq On : 1 Jun 2019 9:49
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 18:39:57 2019

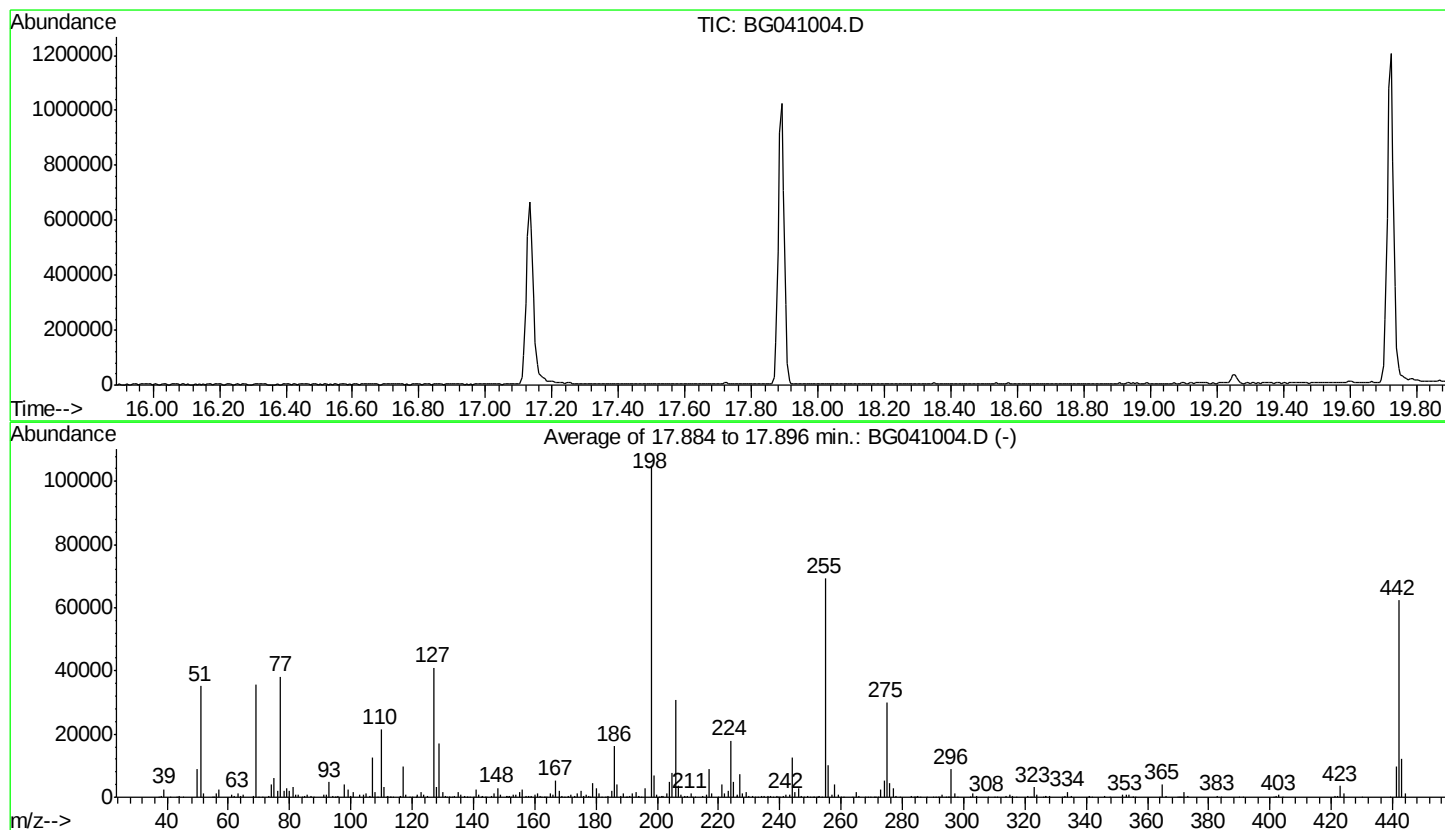

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	35130	PASS
68	69	0.00	2	0.9	314	PASS
69	198	0.00	100	33.9	35640	PASS
70	69	0.00	2	0.3	93	PASS
127	198	10	80	39.0	40954	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105018	PASS
199	198	5	9	6.7	7006	PASS
275	198	10	60	28.4	29872	PASS
365	198	1	100	3.8	3950	PASS
441	198	0.01	100	9.5	9929	PASS
442	198	50	100	59.4	62397	PASS
443	442	15	24	19.3	12042	PASS