




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060122\
 Data File : BG053780.D
 Acq On : 1 Jun 2022 11:32
 Operator : CG/JU
 Sample : PB145155BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK155

Manual IntegrationsAPPROVED

Quant Time: Jun 02 04:07:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 01 00:25:02 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/02/2022
 Supervised By :mohammad ahmed 06/06/2022

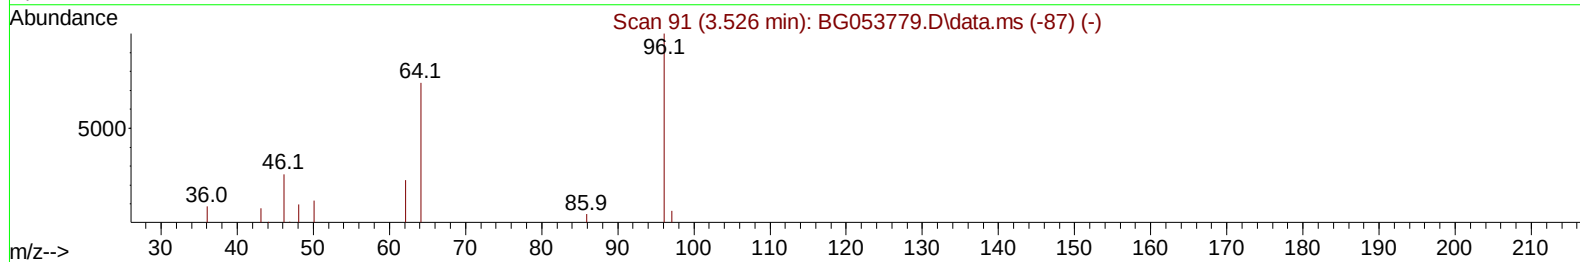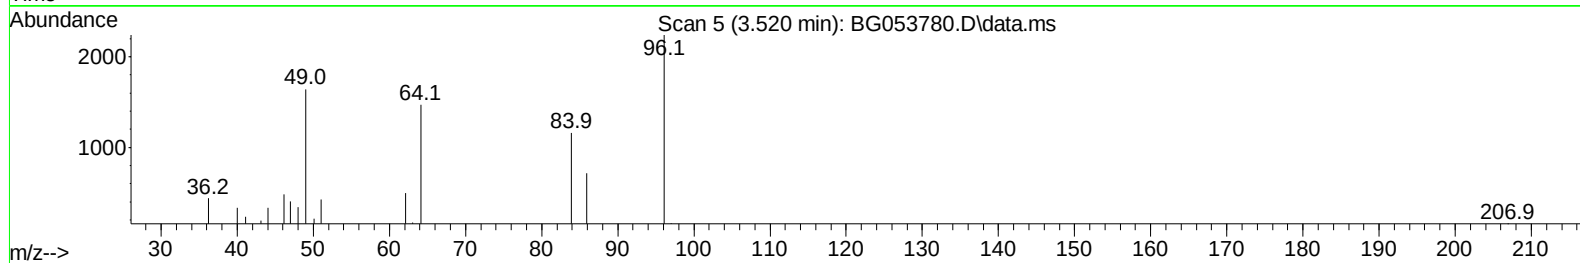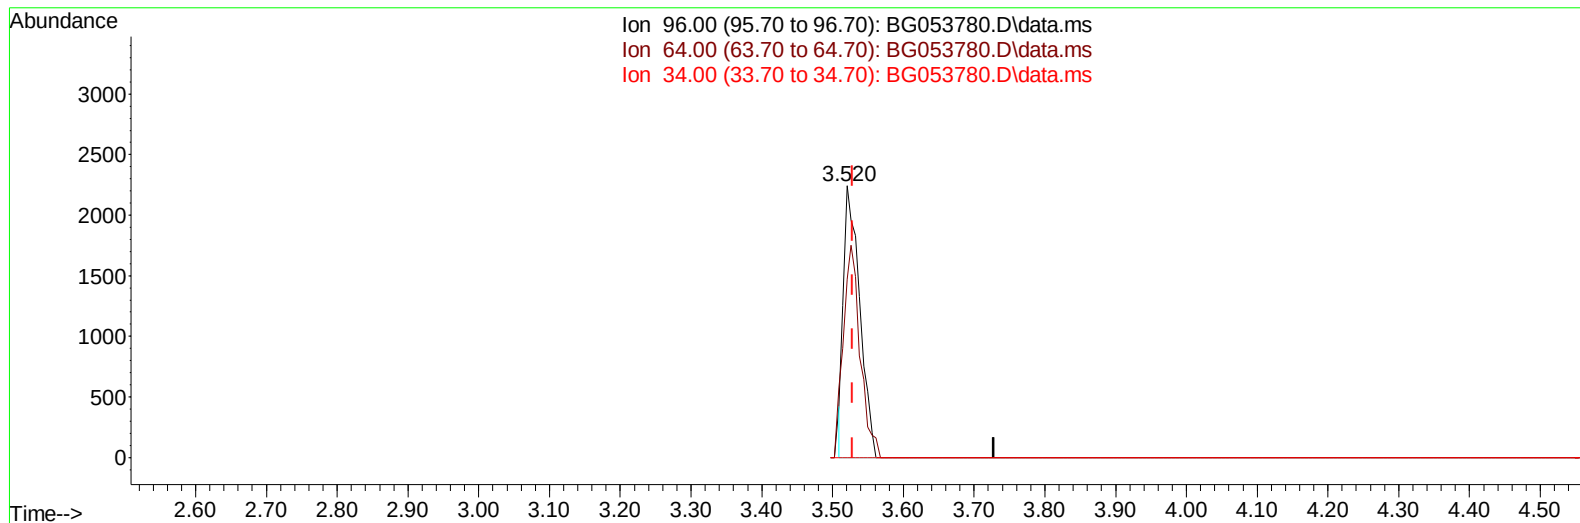

TIC: BG053780.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.520min (-0.008) 6.82 ng/uL

response 3565

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	73.20	65.68
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060122\
 Data File : BG053780.D
 Acq On : 1 Jun 2022 11:32
 Operator : CG/JU
 Sample : PB145155BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK155

Manual IntegrationsAPPROVED

Quant Time: Jun 02 04:07:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 01 00:25:02 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/02/2022
 Supervised By :mohammad ahmed 06/06/2022

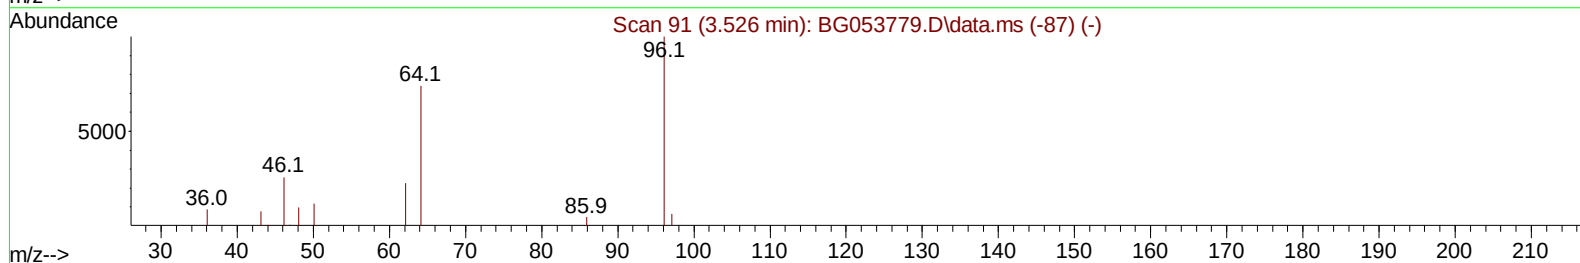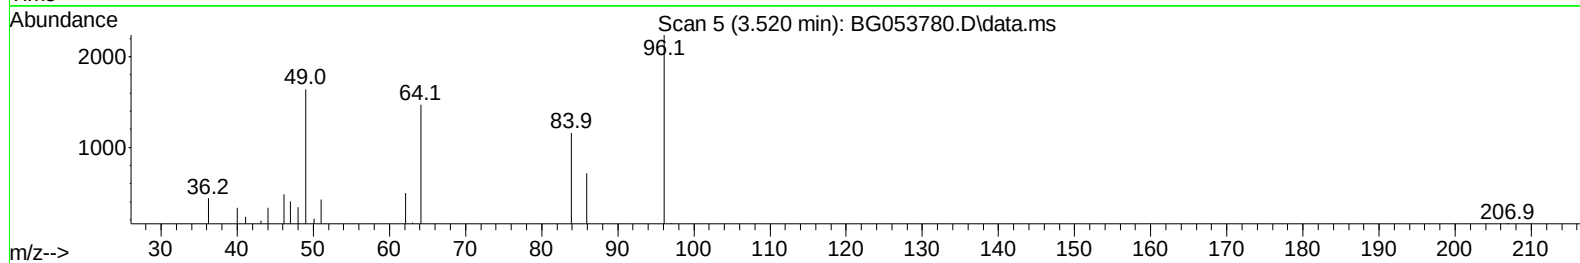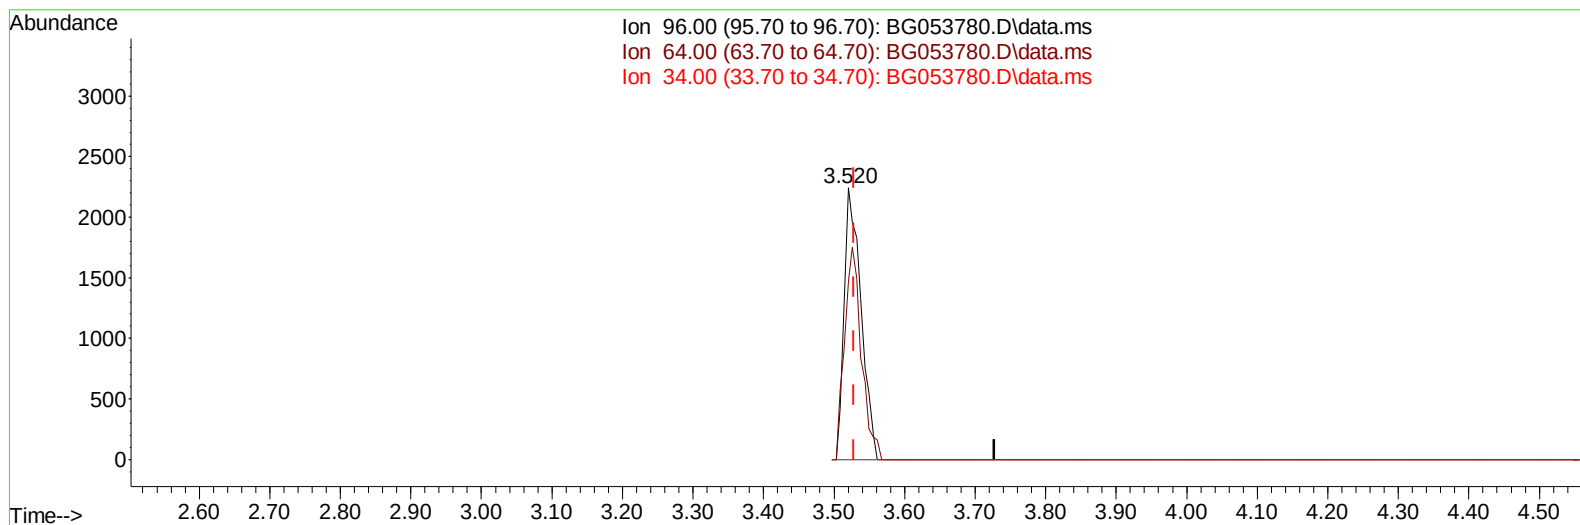

TIC: BG053780.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.520min (-0.008) 7.11 ng/uL m

response 3714

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	73.20	65.68
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060122\
 Data File : BG053780.D
 Acq On : 1 Jun 2022 11:32
 Operator : CG/JU
 Sample : PB145155BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK155

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/02/2022
 Supervised By :mohammad ahmed 06/06/2022

Quant Time: Jun 02 04:07:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 01 00:25:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.097	152	19758	20.000	ng/ul	0.00
20) Naphthalene-d8	10.906	136	78374	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.719	164	54246	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	134055	20.000	ng/ul	0.00
79) Chrysene-d12	21.740	240	153428	20.000	ng/ul	0.00
88) Perylene-d12	25.013	264	151254	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.520	96	3714m	7.110	ng/uL	0.00
4) Pyridine-d5	3.938	84	45854	39.814	ng/ul	-0.01
7) Phenol-d5	7.240	99	57783	38.456	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	37814	38.934	ng/ul	0.00
11) 2-Chlorophenol-d4	7.627	132	46915	39.269	ng/ul	0.00
15) 4-Methylphenol-d8	8.791	113	47285	37.992	ng/ul	0.00
21) Nitrobenzene-d5	9.255	128	20748	44.286	ng/ul	0.00
24) 2-Nitrophenol-d4	9.983	143	20427	43.929	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.518	165	46558	36.866	ng/ul	0.00
31) 4-Chloroaniline-d4	11.029	131	66634	38.461	ng/ul	0.00
46) Dimethylphthalate-d6	14.120	166	167562	40.198	ng/ul	0.00
49) Acenaphthylene-d8	14.413	160	181404	38.946	ng/ul	0.00
54) 4-Nitrophenol-d4	14.884	143	22163	38.668	ng/ul	0.00
60) Fluorene-d10	15.712	176	141408	38.735	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.812	200	20033	37.377	ng/ul	0.00
73) Anthracene-d10	17.563	188	249193	41.156	ng/ul	0.00
81) Pyrene-d10	19.842	212	329875	40.395	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.795	264	325150	42.984	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060122\
Data File : BG053780.D
Acq On : 1 Jun 2022 11:32
Operator : CG/JU
Sample : PB145155BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK155

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/02/2022
Supervised By :mohammad ahmed 06/06/2022

Quant Time: Jun 02 04:07:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 01 00:25:02 2022
Response via : Initial Calibration

