

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060122\
 Data File : BG053780.D
 Acq On : 1 Jun 2022 11:32
 Operator : CG/JU
 Sample : PB145155BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK155

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.520	3	5	12	rVB2	6248	9407	1.16%	0.137%
2	3.814	54	55	58	rBV3	807	939	0.12%	0.014%
3	3.938	73	76	89	rBV	75366	136972	16.86%	1.995%
4	4.084	100	101	107	rBV4	1179	2142	0.26%	0.031%
5	4.272	131	133	139	rVB5	1404	2487	0.31%	0.036%
6	5.166	282	285	287	rBV3	876	865	0.11%	0.013%
7	5.277	299	304	305	rVB4	600	865	0.11%	0.013%
8	5.307	305	309	312	rBV3	624	1063	0.13%	0.015%
9	6.129	448	449	454	rBV3	917	970	0.12%	0.014%
10	6.605	526	530	533	rBV2	675	1052	0.13%	0.015%
11	7.240	631	638	645	rVV	99758	173771	21.39%	2.532%
12	7.416	661	668	676	rBV	72153	128906	15.87%	1.878%
13	7.627	696	704	712	rBV	93582	169647	20.88%	2.471%
14	8.097	777	784	792	rVB	66709	114752	14.13%	1.672%
15	8.791	895	902	911	rVV	121754	213746	26.31%	3.114%
16	9.255	973	981	994	rBV	86299	160825	19.80%	2.343%
17	9.983	1097	1105	1115	rVB	58255	107679	13.25%	1.569%
18	10.518	1188	1196	1205	rBV	109109	204476	25.17%	2.979%
19	10.906	1255	1262	1270	rBV	86455	159614	19.65%	2.325%
20	11.029	1276	1283	1293	rVB	116257	220106	27.09%	3.207%
21	11.411	1344	1348	1350	rBV2	644	1187	0.15%	0.017%
22	11.834	1417	1420	1424	rBV3	585	836	0.10%	0.012%
23	12.480	1525	1530	1531	rBV	1711	2230	0.27%	0.032%
24	12.739	1573	1574	1579	rVB3	677	885	0.11%	0.013%
25	14.120	1803	1809	1817	rBV	224807	342334	42.14%	4.987%
26	14.413	1852	1859	1867	rVB	233406	385491	47.45%	5.616%
27	14.719	1904	1911	1918	rBV	138680	228234	28.09%	3.325%
28	14.884	1931	1939	1949	rBV	94543	157566	19.40%	2.295%
29	14.948	1949	1950	1954	rVV2	1067	989	0.12%	0.014%
30	15.712	2073	2080	2088	rBV	321457	509475	62.71%	7.422%
31	15.812	2092	2097	2103	rBV	71024	102542	12.62%	1.494%
32	15.871	2106	2107	2109	rBV	1012	910	0.11%	0.013%
33	15.953	2115	2121	2126	rVB3	2879	3964	0.49%	0.058%
34	16.488	2210	2212	2217	rVB4	1170	1376	0.17%	0.020%
35	16.693	2245	2247	2250	rBV2	722	865	0.11%	0.013%
36	16.805	2264	2266	2270	rVB3	843	859	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060122\
 Data File : BG053780.D
 Acq On : 1 Jun 2022 11:32
 Operator : CG/JU
 Sample : PB145155BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK155

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
 Title : SVOA CALIBRATION

37	16.899	2279	2282	2284	rBV2	919	996	0.12%	0.015%
38	17.287	2346	2348	2352	rVV3	765	1023	0.13%	0.015%
39	17.339	2355	2357	2360	rVB	1045	1066	0.13%	0.016%
40	17.463	2372	2378	2387	rVB	195109	303482	37.36%	4.421%
41	17.563	2387	2395	2402	rBV2	386370	606291	74.63%	8.833%
42	18.086	2480	2484	2487	rVB4	1398	1545	0.19%	0.023%
43	18.139	2491	2493	2497	rBV	1119	1239	0.15%	0.018%
44	18.426	2539	2542	2545	rBV3	1368	1804	0.22%	0.026%
45	18.603	2570	2572	2574	rBV3	1213	1310	0.16%	0.019%
46	19.108	2656	2658	2660	rBV3	1103	977	0.12%	0.014%
47	19.414	2705	2710	2714	rBV4	7213	11475	1.41%	0.167%
48	19.478	2718	2721	2726	rVB2	5666	7790	0.96%	0.113%
49	19.842	2777	2783	2791	rBV	537084	798649	98.31%	11.635%
50	21.740	3100	3106	3114	rVB	233537	386879	47.62%	5.636%
51	24.795	3615	3626	3637	rVB2	279039	812399	100.00%	11.835%
52	25.013	3655	3663	3675	rVB2	131926	377212	46.43%	5.495%




Sum of corrected areas: 6864164

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060122\
Data File : BG053780.D
Acq On : 1 Jun 2022 11:32
Operator : CG/JU
Sample : PB145155BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK155

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

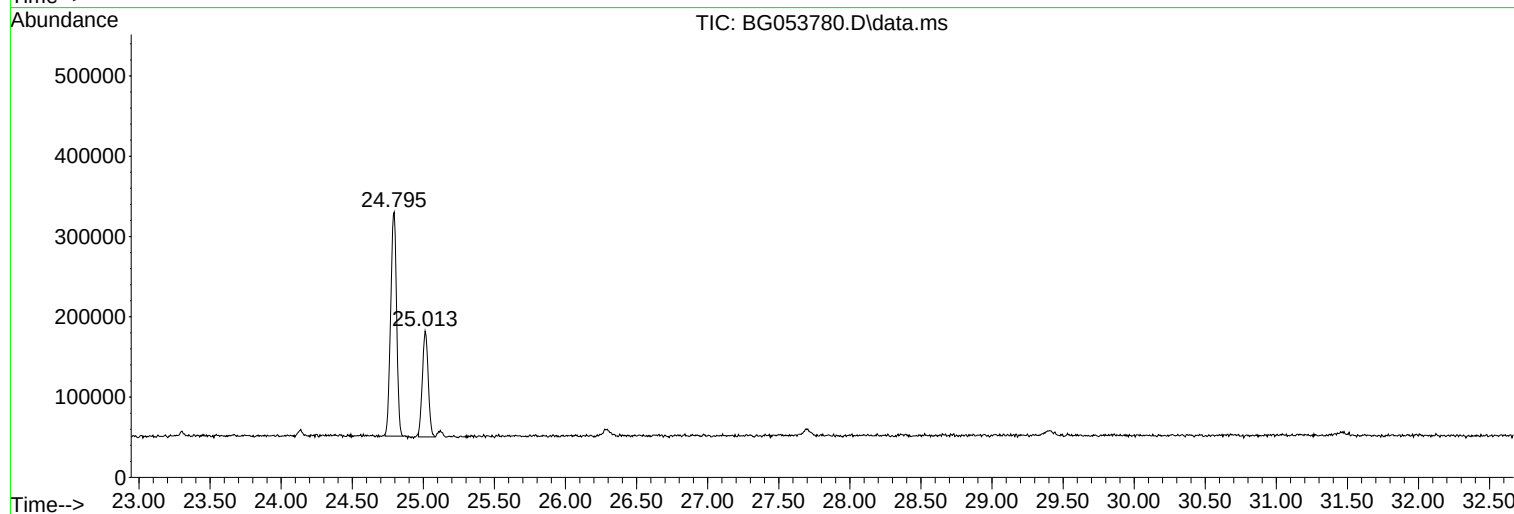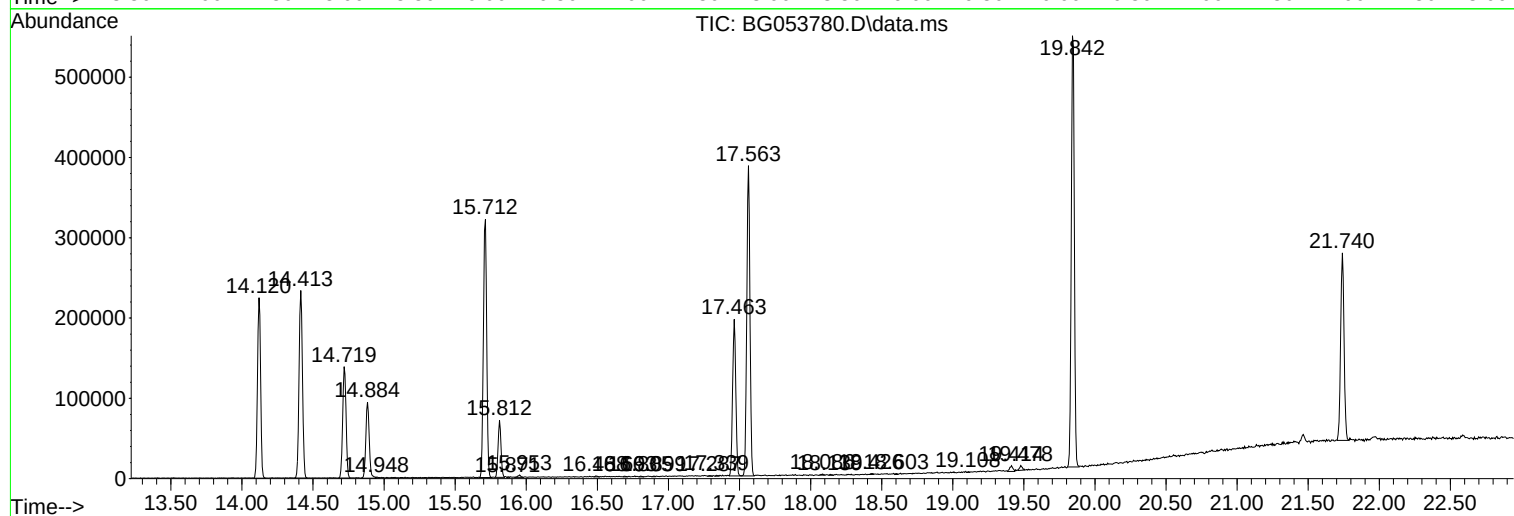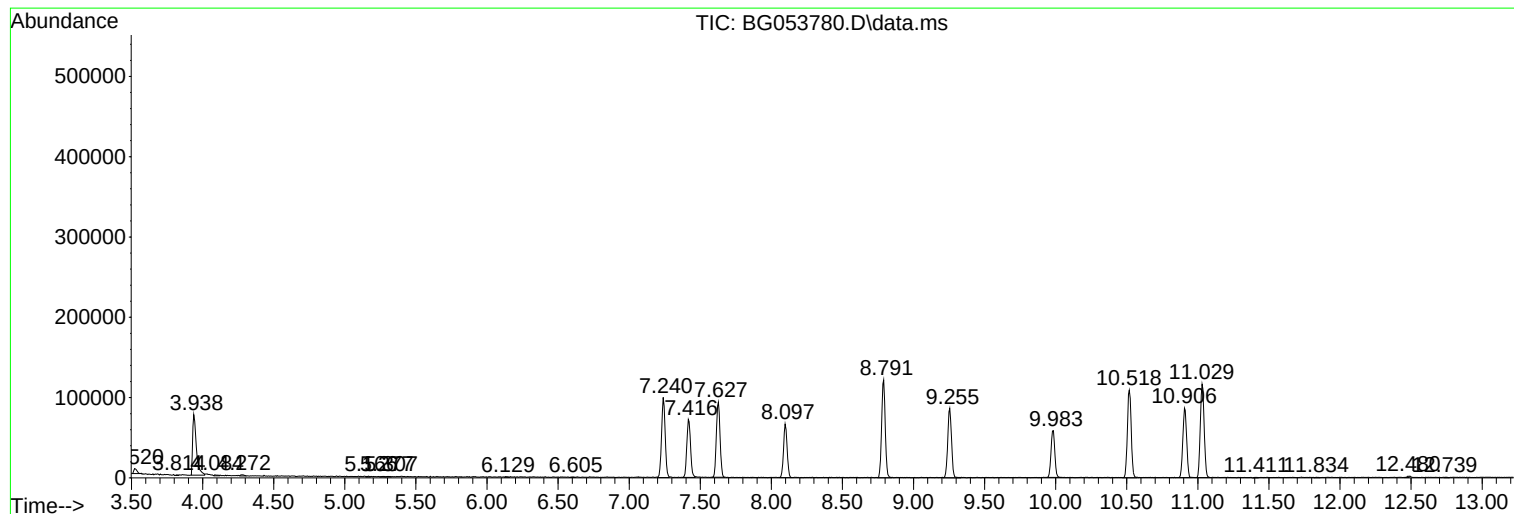

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060122\
Data File : BG053780.D
Acq On : 1 Jun 2022 11:32
Operator : CG/JU
Sample : PB145155BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK155

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060122\
Data File : BG053780.D
Acq On : 1 Jun 2022 11:32
Operator : CG/JU
Sample : PB145155BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK155

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc