

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060319\
 Data File : BG041050.D
 Acq On : 4 Jun 2019 1:07
 Operator : HP/JU
 Sample : K3105-01 2X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 101-102

Quant Time: Jun 04 08:08:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 29 18:39:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	89406	20.00	ng	0.00
21) Naphthalene-d8	10.95	136	330981	20.00	ng	0.00
39) Acenaphthene-d10	14.76	164	207398	20.00	ng	0.00
64) Phenanthrene-d10	17.50	188	444409	20.00	ng	0.00
76) Chrysene-d12	21.79	240	464135	20.00	ng	0.00
87) Perylene-d12	25.16	264	366071	20.00	ng	0.04

System Monitoring Compounds

5) 2-Fluorophenol	5.66	112	234844	47.37	ng	0.00
7) Phenol-d6	7.27	99	334460	43.68	ng	0.00
23) Nitrobenzene-d5	9.30	82	235405	31.57	ng	0.00
42) 2,4,6-Tribromophenol	16.25	330	133652	43.41	ng	0.00
45) 2-Fluorobiphenyl	13.38	172	492091	34.17	ng	0.00
79) Terphenyl-d14	20.10	244	681906	31.18	ng	0.00

Target Compounds


						Qvalue
19) n-Nitroso-di-n-propylamine	9.30	70	32922	5.587	ng	# 77
32) Benzoic acid	10.29	122	54	8.141	ng	# 1
41) Hexachlorocyclopentadiene	12.85	237	73	8.250	ng	# 26
49) Acenaphthylene	14.49	152	82802	4.174	ng	98
50) Dimethylphthalate	14.19	163	62264	3.547	ng	97
54) 2,4-Dinitrophenol	14.83	184	66	8.293	ng	# 1
58) Fluorene	15.80	166	49155	3.053	ng	96
65) 4,6-Dinitro-2-methylphenol	15.89	198	160	8.645	ng	# 1
70) Pentachlorophenol	17.32	266	202	4.312	ng	93
71) Phenanthrene	17.55	178	458231	19.795	ng	99
72) Anthracene	17.64	178	150987	6.613	ng	99
75) Fluoranthene	19.55	202	1171229	40.963	ng	97
78) Pyrene	19.92	202	1205610	39.958	ng	98
81) Benzo(a)anthracene	21.77	228	689071	22.303	ng	96
83) Chrysene	21.84	228	684818	23.162	ng	94
86) Indeno(1,2,3-cd)pyrene	29.01	276	190637	5.264	ng	# 93
88) Benzo(b)fluoranthene	24.08	252	691080	31.125	ng	# 81
89) Benzo(k)fluoranthene	24.08	252	691080	31.453	ng	# 80
90) Benzo(a)pyrene	25.01	252	470582	22.214	ng	# 94
92) Benzo(g,h,i)perylene	30.23	276	139615	6.789	ng	# 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060319\
Data File : BG041050.D
Acq On : 4 Jun 2019 1:07
Operator : HP/JU
Sample : K3105-01 2X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
101-102

Quant Time: Jun 04 08:08:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 29 18:39:57 2019
Response via : Initial Calibration

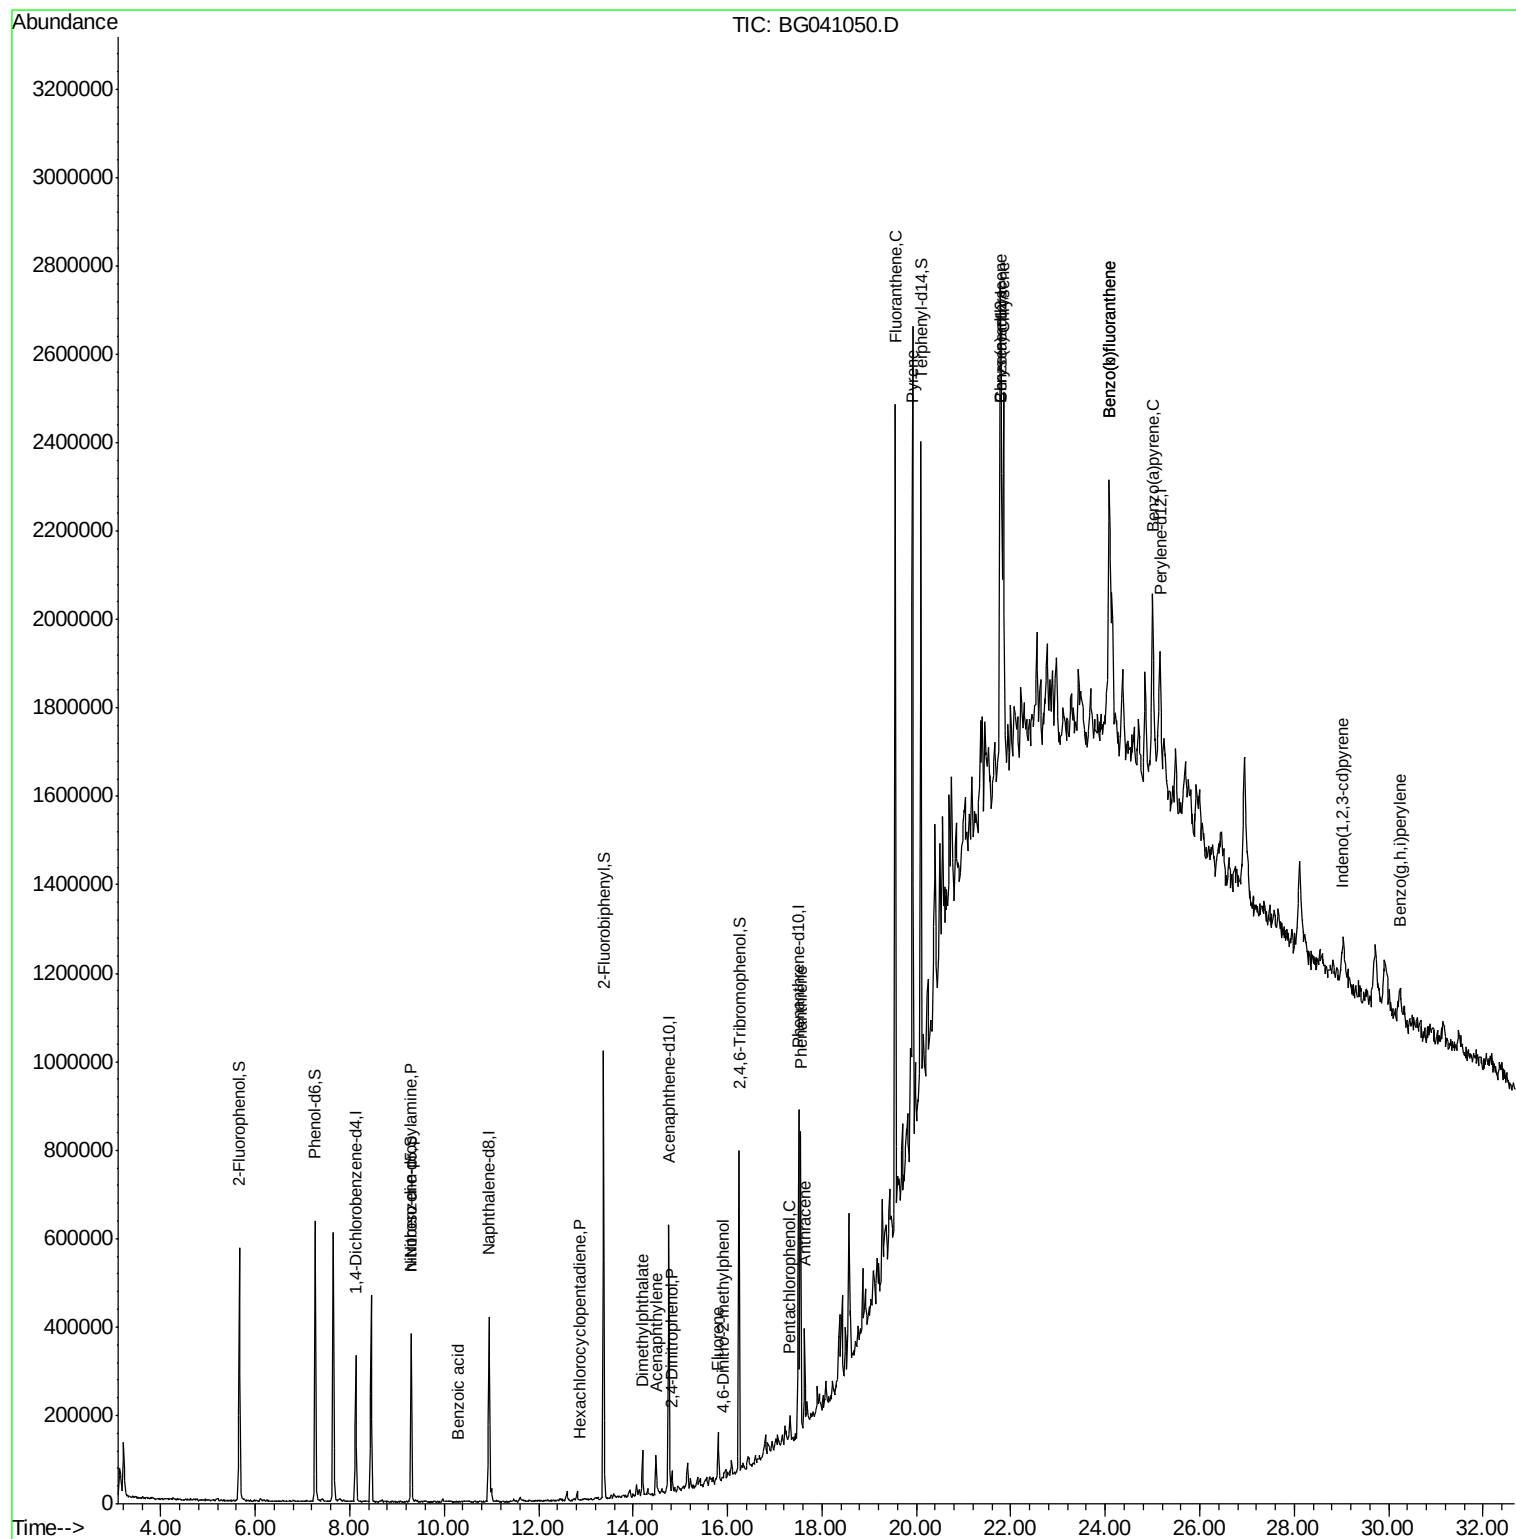




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.13 min Scan# 858
Delta R.T. 0.00 min
Lab File: BG041050.D
Acq: 4 Jun 2019 1:07

Instrument :
BNA_G
ClientSampleId :
101-102

Tgt Ion	Ratio	Lower	Upper
152	100		
150	152.2	120.6	180.8
115	56.9	45.1	67.7






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

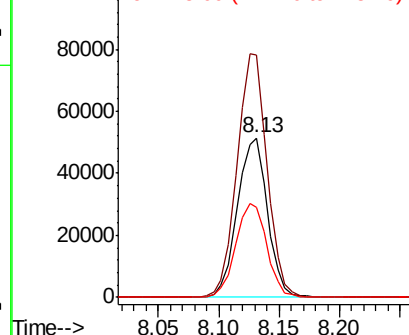

#5

2-Fluorophenol
Concen: 47.365 ng
RT: 5.66 min Scan# 438
Delta R.T. 0.01 min
Lab File: BG041050.D
Acq: 4 Jun 2019 1:07

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.2	56.2	84.2
63	39.2	32.8	49.2








Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

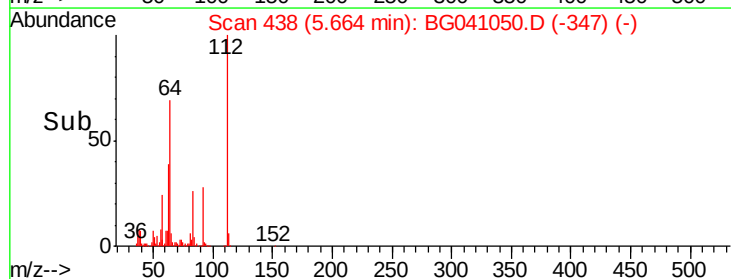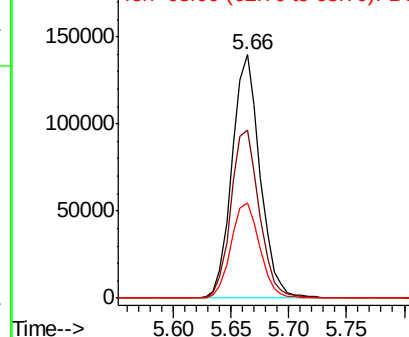

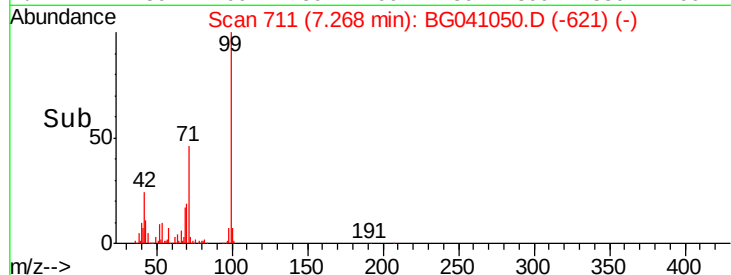

#7

Phenol-d6

Concen: 43.678 ng

RT: 7.27 min Scan# 711

Delta R.T. 0.00 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07

Instrument :

BNA_G

ClientSampleId :

101-102





Tgt Ion: 99 Resp: 334460

Ion Ratio Lower Upper

99 100

42 23.6 17.9 26.9

71 46.2 35.4 53.0

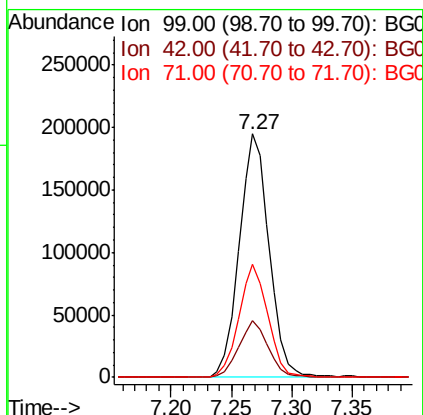

#19

n-Nitroso-di-n-propylamine

Concen: 5.587 ng

RT: 9.30 min Scan# 1057

Delta R.T. 0.36 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07

Tgt Ion: 70 Resp: 32922


Ion Ratio Lower Upper


70 100

42 51.1 51.5 77.3#

101 0.0 8.1 12.1#

130 2.2 16.6 24.8#

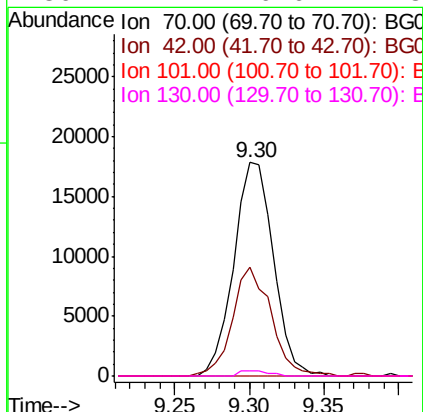







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.95 min Scan# 1338
Delta R.T. 0.00 min
Lab File: BG041050.D
Acq: 4 Jun 2019 1:07

Instrument :
BNA_G
ClientSampleId :
101-102

Tgt Ion:	136	Resp:	330981
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.5	14.3
54	8.0	7.6	11.4
68	4.1	3.9	5.9




Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


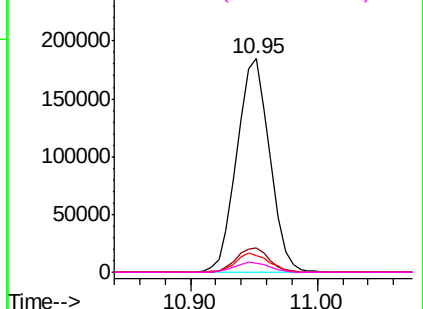



#23
Nitrobenzene-d5
Concen: 31.574 ng
RT: 9.30 min Scan# 1057
Delta R.T. -0.01 min
Lab File: BG041050.D
Acq: 4 Jun 2019 1:07

Tgt Ion:	82	Resp:	235405
Ion	Ratio	Lower	Upper
82	100		
128	37.8	30.5	45.7
54	55.3	44.6	66.8



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC




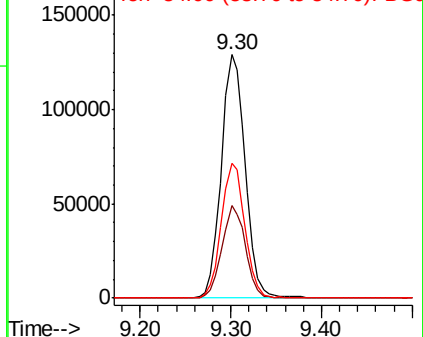


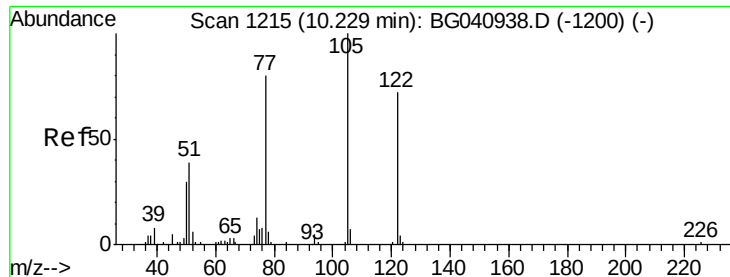

#32
Benzoic acid
Concen: 8.141 ng
RT: 10.29 min Scan# 1225
Delta R.T. 0.06 min
Lab File: BG041050.D
Acq: 4 Jun 2019 1:07




Instrument :
BNA_G
ClientSampleId :
101-102


Tgt Ion	Ratio	Lower	Upper
122	100		
105	0.0	114.8	154.8#
77	0.0	89.9	129.9#

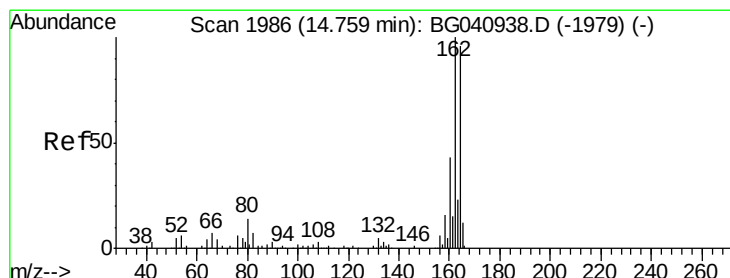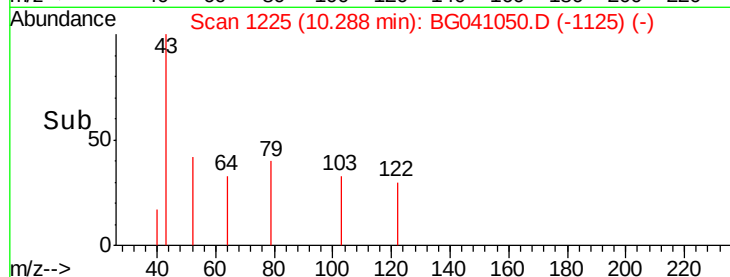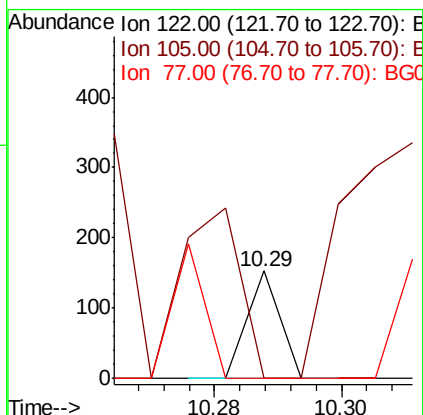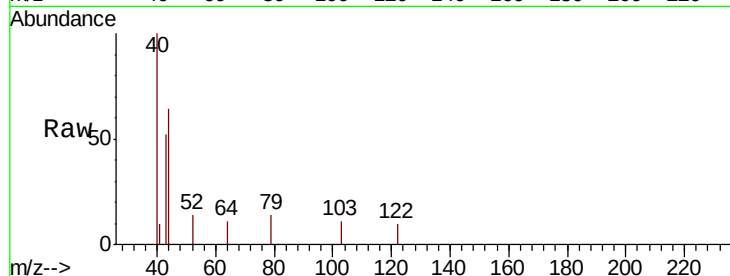

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.76 min Scan# 1986
Delta R.T. 0.00 min
Lab File: BG041050.D
Acq: 4 Jun 2019 1:07

Tgt Ion	Ratio	Lower	Upper
164	100		
162	107.1	83.0	124.4
160	47.4	35.6	53.4


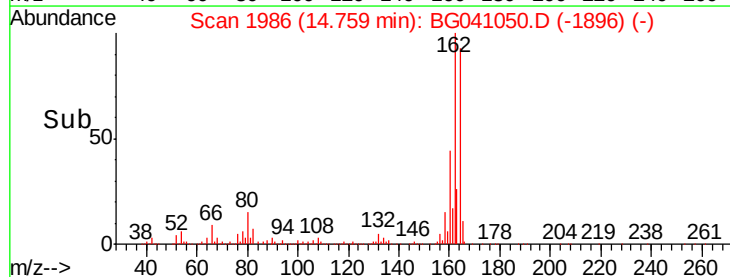
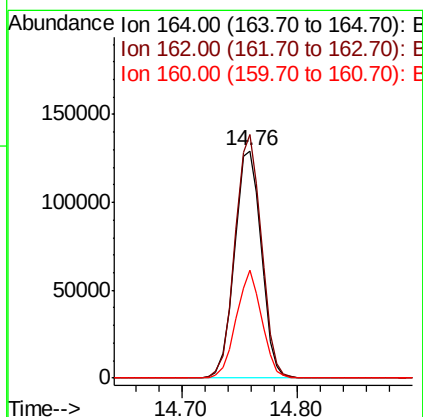
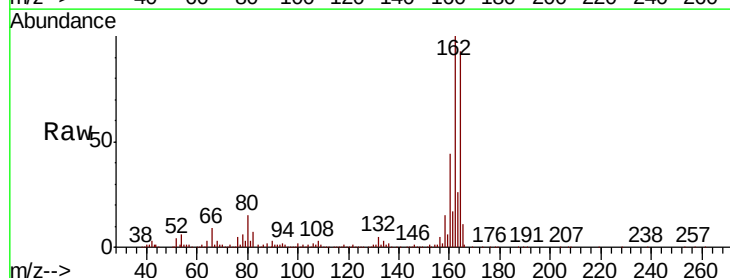


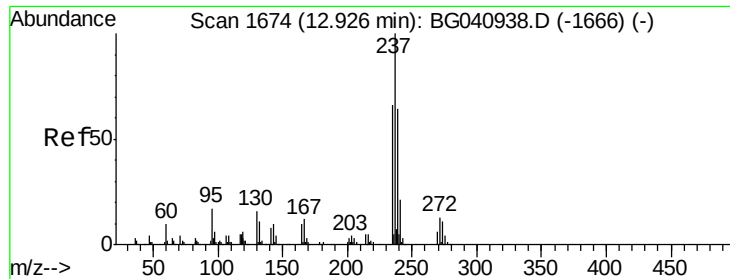

#41
 Hexachlorocyclopentadiene
 Concen: 8.250 ng
 RT: 12.85 min Scan# 1661
 Delta R.T. -0.08 min
 Lab File: BG041050.D
 Acq: 4 Jun 2019 1:07




Instrument :
 BNA_G
 ClientSampled :
 101-102


Tgt Ion	Ratio	Lower	Upper
237	100		
235	0.0	45.5	85.5#
272	0.0	0.0	32.9

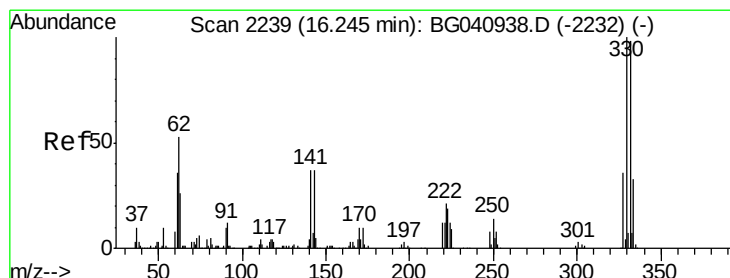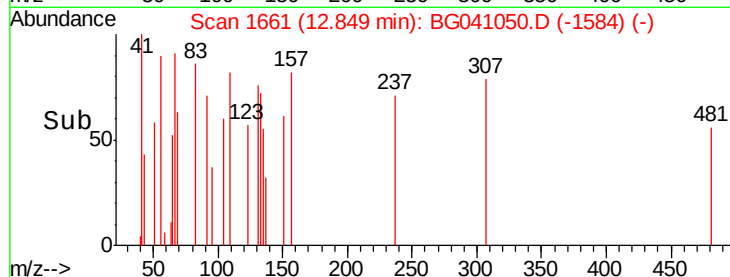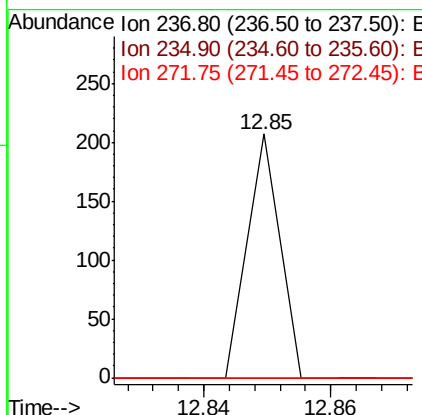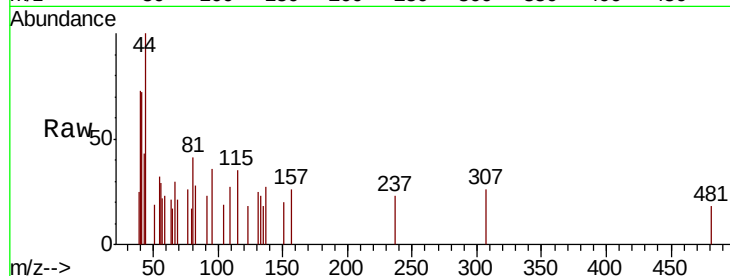

#42
 2,4,6-Tribromophenol
 Concen: 43.408 ng
 RT: 16.25 min Scan# 2239
 Delta R.T. 0.00 min
 Lab File: BG041050.D
 Acq: 4 Jun 2019 1:07

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.1	78.5	117.7
141	36.5	28.7	43.1

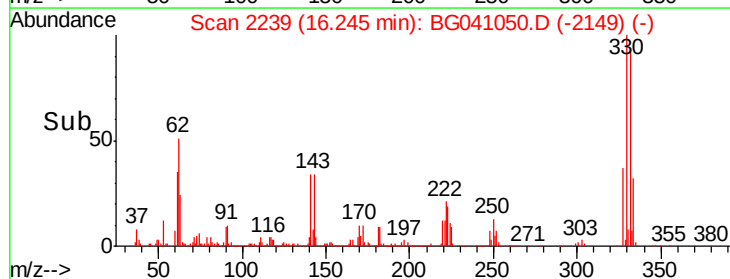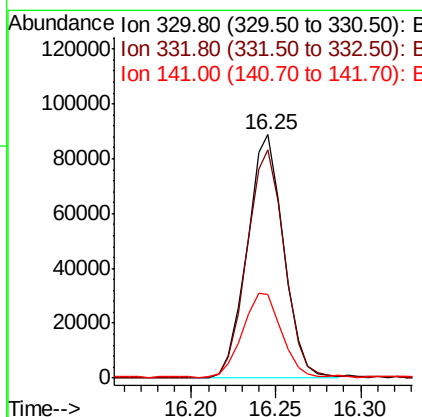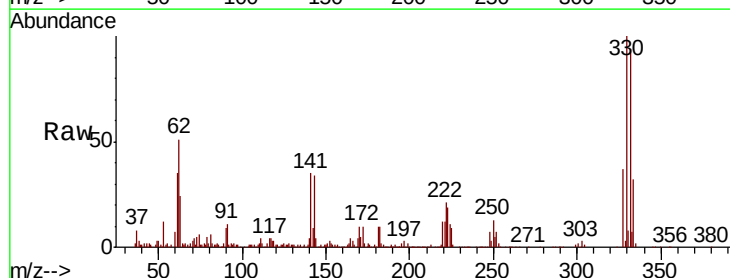



#45

2-Fluorobiphenyl

Concen: 34.169 ng

RT: 13.38 min Scan# 1751

Delta R.T. -0.01 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07

Instrument :

BNA_G

ClientSampleId :

101-102


Tgt Ion:172 Resp: 492091

Ion Ratio Lower Upper

172 100

171 37.2 31.1 46.7




170 25.0 20.5 30.7



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

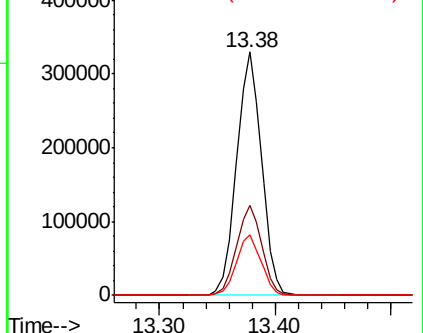

#49

Acenaphthylene

Concen: 4.174 ng

RT: 14.49 min Scan# 1940

Delta R.T. 0.00 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07


Tgt Ion:152 Resp: 82802

Ion Ratio Lower Upper

152 100

151 20.6 17.4 26.0



153 13.6 11.0 16.4




Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

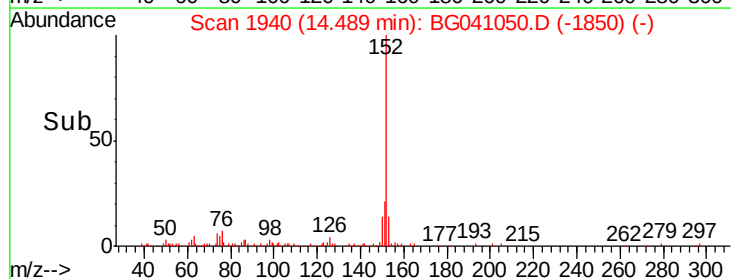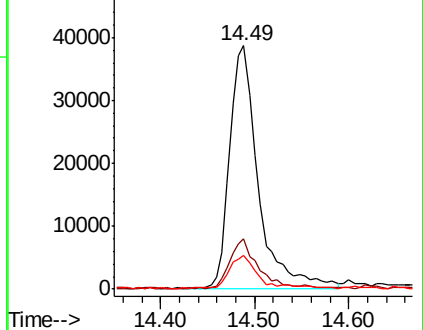







#50
Dimethylphthalate
Concen: 3.547 ng
RT: 14.19 min Scan# 1890
Delta R.T. -0.01 min
Lab File: BG041050.D
Acq: 4 Jun 2019 1:07

Instrument :
BNA_G
ClientSampleId :
101-102

Tgt Ion	Ratio	Lower	Upper
163	100		
194	5.0	3.8	5.8
164	9.5	8.7	13.1




Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

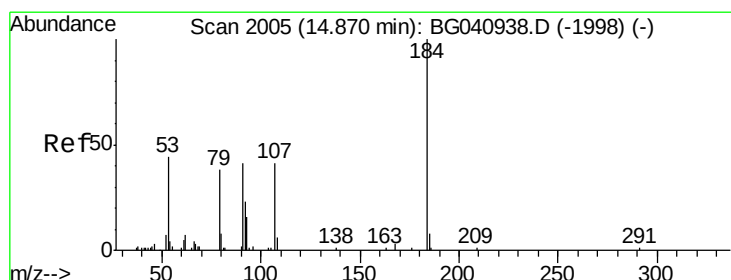
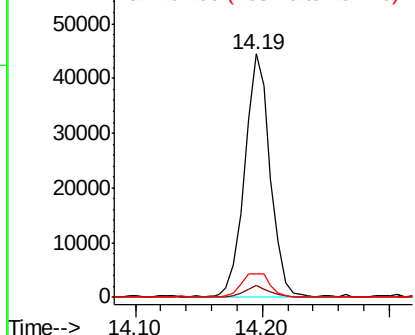



#54
2,4-Dinitrophenol
Concen: 8.293 ng
RT: 14.83 min Scan# 1998
Delta R.T. -0.04 min
Lab File: BG041050.D
Acq: 4 Jun 2019 1:07

Tgt Ion	Ratio	Lower	Upper
184	100		
63	323.4	49.8	74.6#
154	4266.0	52.2	78.4#



Abundance Ion 184.00 (183.70 to 184.70): E
Ion 63.00 (62.70 to 63.70): BG
Ion 154.00 (153.70 to 154.70): E

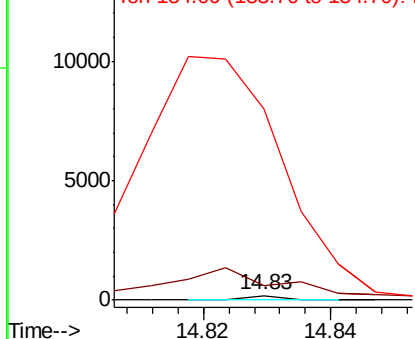

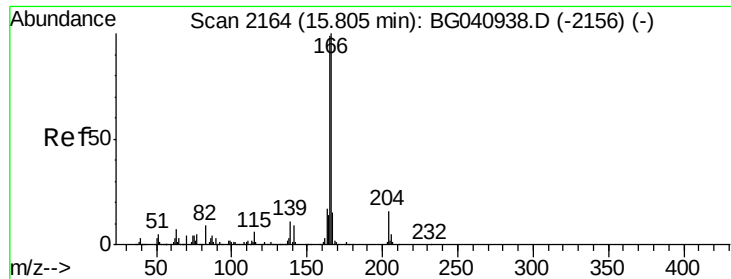

#58

Fluorene

Concen: 3.053 ng

RT: 15.80 min Scan# 2163

Delta R.T. -0.01 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07

Instrument :

BNA_G

ClientSampleId :

101-102


Tgt Ion:166 Resp: 49155

Ion Ratio Lower Upper

166 100

165 95.1 79.2 118.8




167 15.9 11.8 17.6



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

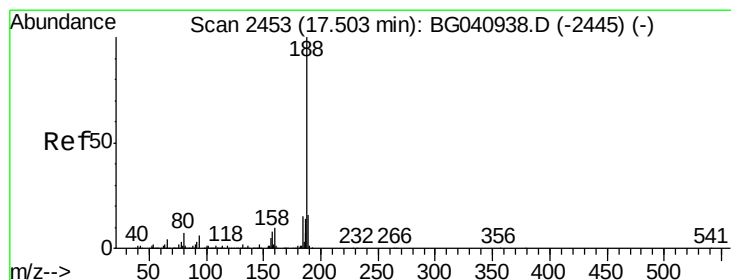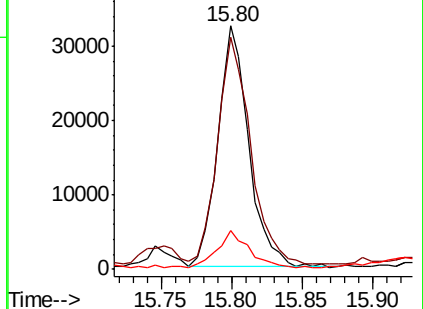

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.50 min Scan# 2453

Delta R.T. 0.00 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07


Tgt Ion:188 Resp: 444409

Ion Ratio Lower Upper

188 100

94 5.4 4.7 7.1



80 7.2 5.8 8.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

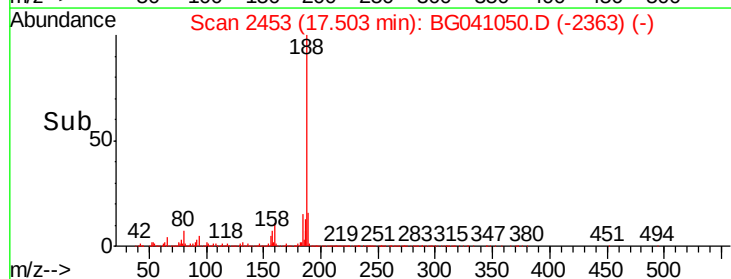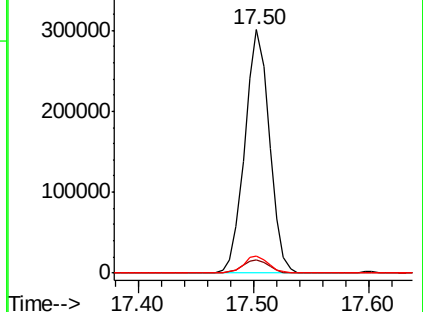



#65

4,6-Dinitro-2-methylphenol

Concen: 8.645 ng

RT: 15.89 min Scan# 2179

Delta R.T. 0.02 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07

Instrument :

BNA_G

ClientSampled :

101-102


Tgt Ion:198 Resp: 160

Ion Ratio Lower Upper

198 100

51 107.5 21.6 61.6#




105 258.3 17.5 57.5#



Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BG

Ion 105.00 (104.70 to 105.70): E

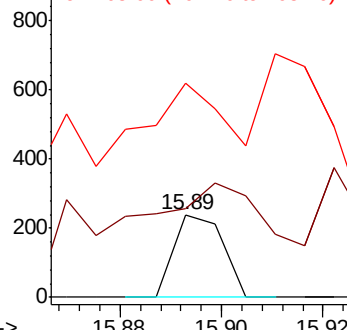

#70

Pentachlorophenol

Concen: 4.312 ng

RT: 17.32 min Scan# 2422

Delta R.T. 0.18 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07


Tgt Ion:266 Resp: 202

Ion Ratio Lower Upper

266 100

268 70.6 53.1 79.7



264 69.4 49.9 74.9




Abundance Ion 265.70 (265.40 to 266.40): E

Ion 268.00 (267.70 to 268.70): E

Ion 264.00 (263.70 to 264.70): E




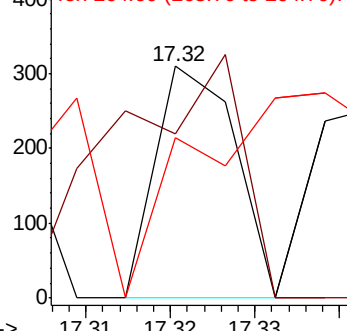


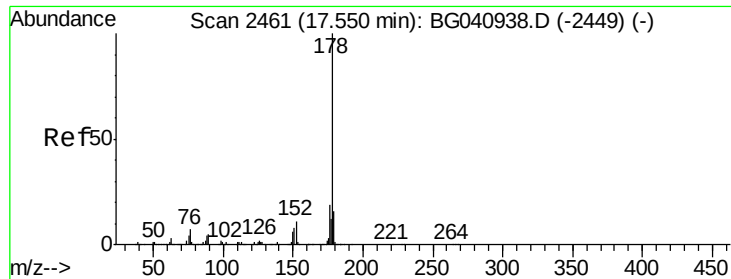

#71
Phenanthrene
Concen: 19.795 ng
RT: 17.55 min Scan# 2461
Delta R.T. 0.00 min
Lab File: BG041050.D
Acq: 4 Jun 2019 1:07




Instrument :
BNA_G
ClientSampleId :
101-102


Tgt Ion:178 Resp: 458231
Ion Ratio Lower Upper
178 100
176 19.0 15.5 23.3
179 16.6 12.7 19.1

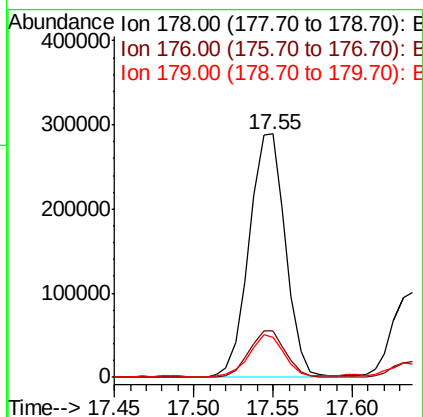

#72
Anthracene
Concen: 6.613 ng
RT: 17.64 min Scan# 2476
Delta R.T. 0.00 min
Lab File: BG041050.D
Acq: 4 Jun 2019 1:07

Tgt Ion:178 Resp: 150987
Ion Ratio Lower Upper
178 100
176 19.3 15.6 23.4
179 15.8 13.0 19.4

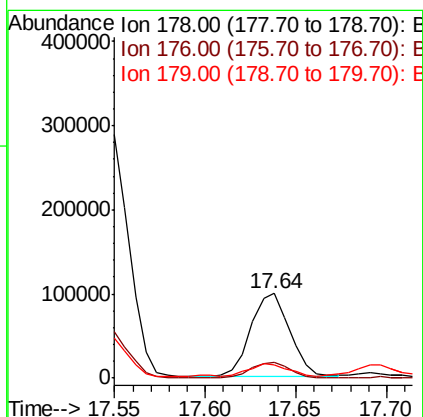

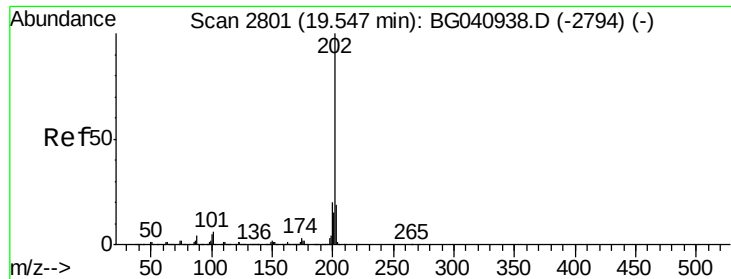

#75

Fluoranthene

Concen: 40.963 ng

RT: 19.55 min Scan# 2802

Delta R.T. 0.01 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07

Instrument :

BNA_G

ClientSampled :

101-102


Tgt Ion:202 Resp: 1171229

Ion Ratio Lower Upper

202 100

101 6.3 0.0 26.2




203 20.4 0.0 38.7



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

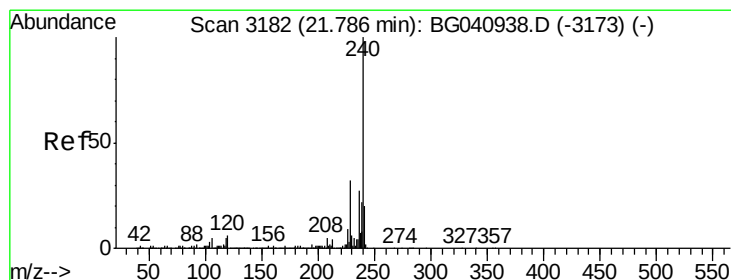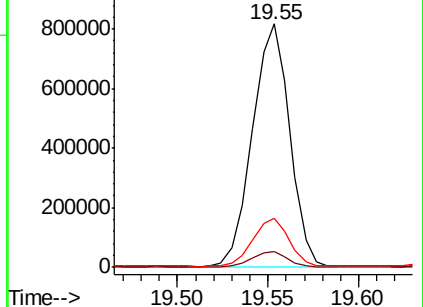

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.79 min Scan# 3183

Delta R.T. 0.01 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07


Tgt Ion:240 Resp: 464135

Ion Ratio Lower Upper

240 100

120 6.4 4.5 6.7



236 28.6 21.3 31.9




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

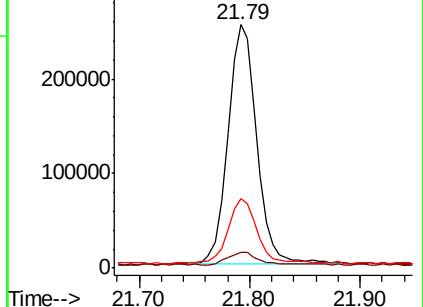



#78

Pyrene

Concen: 39.958 ng

RT: 19.92 min Scan# 2864

Delta R.T. 0.01 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07

Instrument :

BNA_G

ClientSampleId :

101-102


Tgt Ion:202 Resp: 1205610

Ion Ratio Lower Upper

202 100

200 22.6 17.5 26.3




203 21.0 15.6 23.4



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

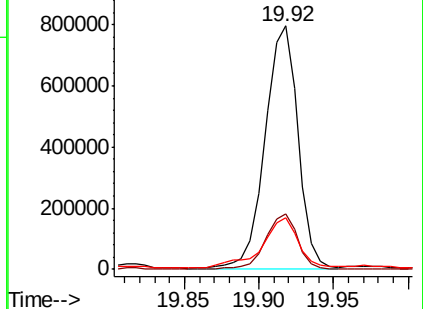

#79

Terphenyl-d14

Concen: 31.181 ng

RT: 20.10 min Scan# 2895

Delta R.T. 0.00 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07


Tgt Ion:244 Resp: 681906

Ion Ratio Lower Upper

244 100

212 8.5 7.0 10.4



122 6.0 5.4 8.0




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

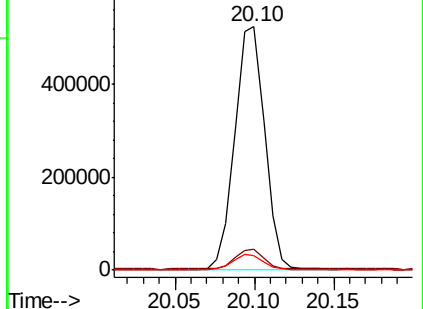



#81

Benzo(a)anthracene

Concen: 22.303 ng

RT: 21.77 min Scan# 3180

Delta R.T. 0.01 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07

Instrument :

BNA_G

ClientSampleId :

101-102


Tgt Ion:228 Resp: 689071

Ion Ratio Lower Upper

228 100

226 31.3 23.5 35.3




229 23.0 16.7 25.1



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

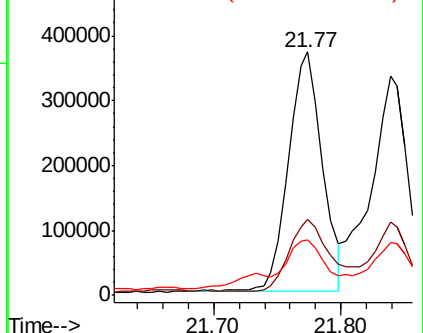

#83

Chrysene

Concen: 23.162 ng

RT: 21.84 min Scan# 3191

Delta R.T. 0.01 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07


Tgt Ion:228 Resp: 684818

Ion Ratio Lower Upper

228 100

226 33.4 24.6 37.0



229 24.2 16.6 24.8




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

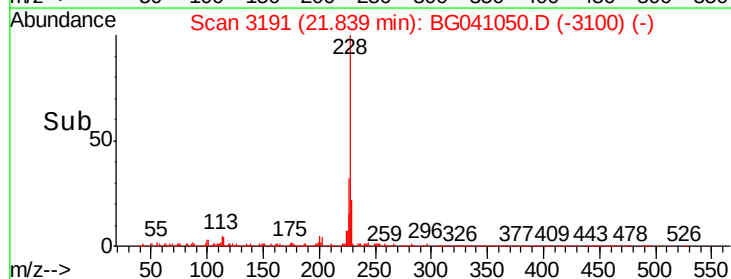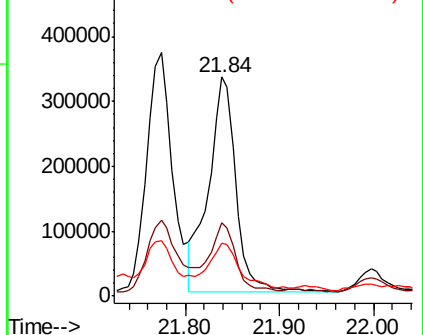

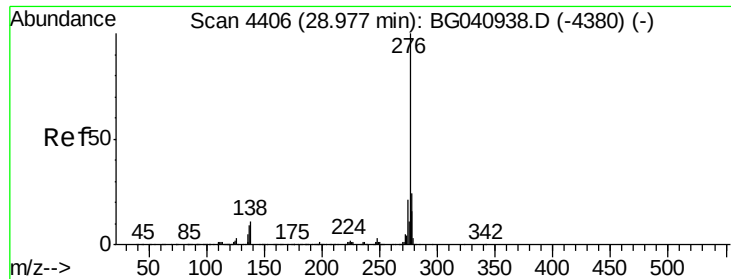

#86

Indeno(1,2,3-cd)pyrene

Concen: 5.264 ng

RT: 29.01 min Scan# 4412

Delta R.T. 0.04 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07

Instrument :

BNA_G

ClientSampleId :

101-102


Tgt Ion:276 Resp: 190637

Ion Ratio Lower Upper

276 100

138 9.7 5.7 8.5#

277 22.2 20.8 31.2






Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

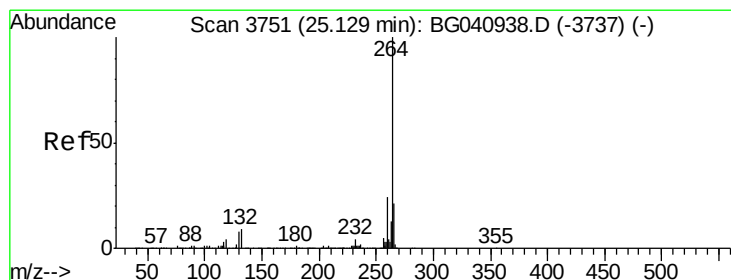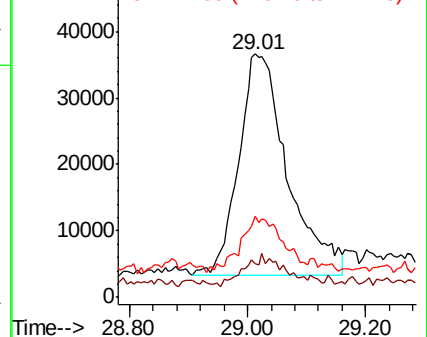

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.16 min Scan# 3757

Delta R.T. 0.04 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07


Tgt Ion:264 Resp: 366071

Ion Ratio Lower Upper

264 100

260 24.9 19.0 28.4

265 26.3 17.0 25.4#






Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

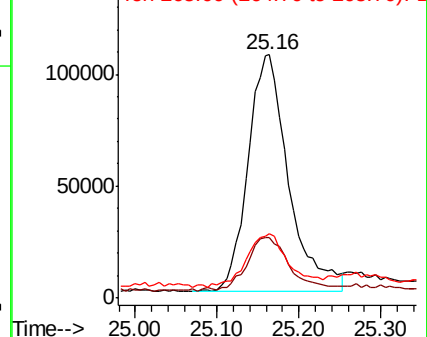

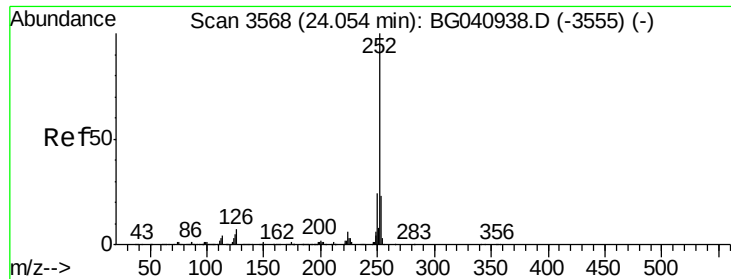

#88

Benzo(b)fluoranthene

Concen: 31.125 ng

RT: 24.08 min Scan# 3573

Delta R.T. 0.03 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07


Instrument :

BNA_G

ClientSampleId :

101-102




Tgt Ion:	252	Resp:	691080
Ion Ratio	Lower	Upper	
252	100		
253	33.0	18.4	27.6#
125	9.4	4.3	6.5#

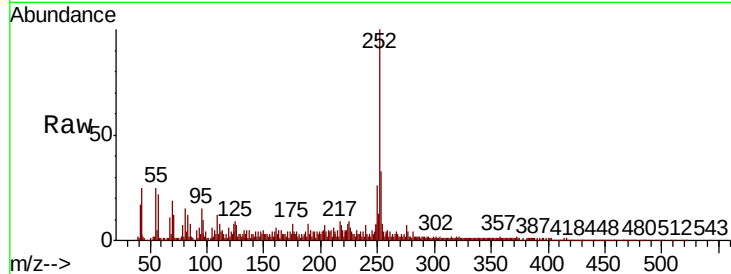

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

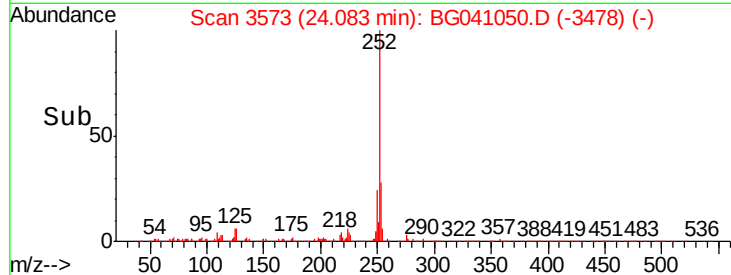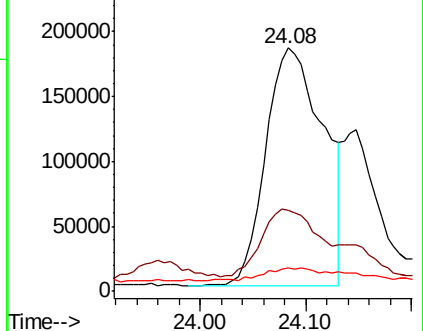

#89

Benzo(k)fluoranthene

Concen: 31.453 ng


RT: 24.08 min Scan# 3573

Delta R.T. -0.05 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07



Tgt Ion:	252	Resp:	691080
Ion Ratio	Lower	Upper	
252	100		
253	33.0	17.8	26.6#
125	9.4	4.7	7.1#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

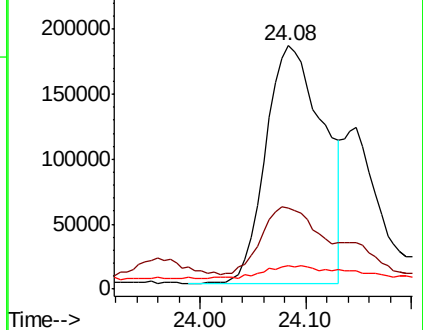

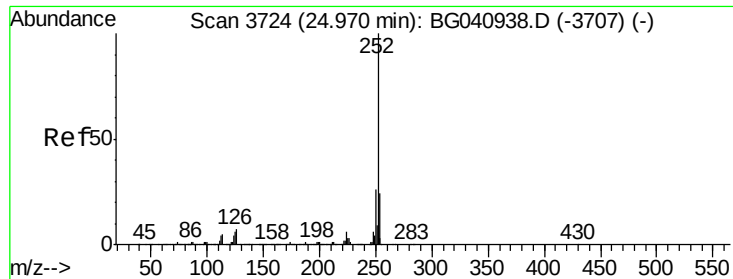

#90

Benzo(a)pyrene

Concen: 22.214 ng

RT: 25.01 min Scan# 3730

Delta R.T. 0.04 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07

Instrument :

BNA_G

ClientSampleId :

101-102


Tgt Ion:252 Resp: 470582

Ion Ratio Lower Upper

252 100

253 26.7 19.5 29.3

125 9.5 5.1 7.7#



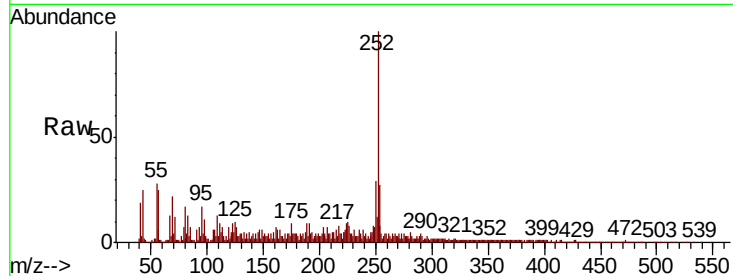


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

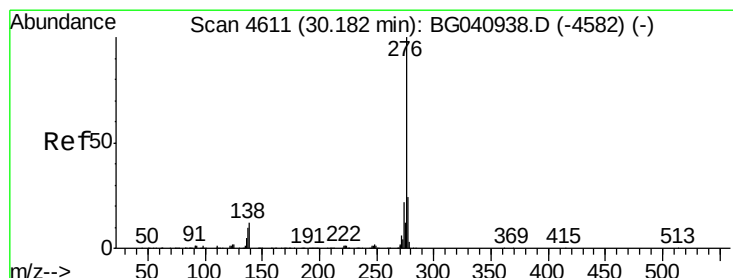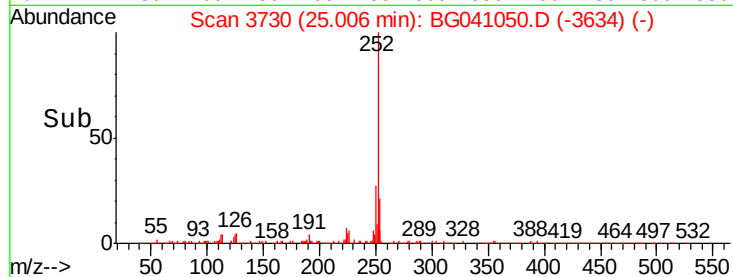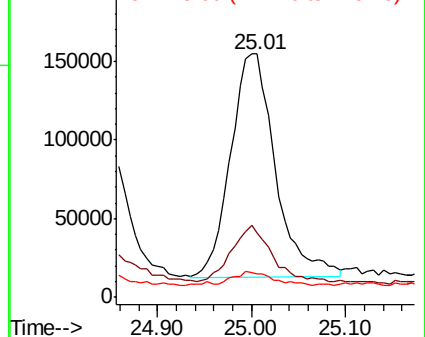

#92

Benzo(g,h,i)perylene

Concen: 6.789 ng

RT: 30.23 min Scan# 4620

Delta R.T. 0.05 min

Lab File: BG041050.D

Acq: 4 Jun 2019 1:07


Tgt Ion:276 Resp: 139615

Ion Ratio Lower Upper

276 100

277 34.4 19.4 29.0#

138 15.8 9.7 14.5#

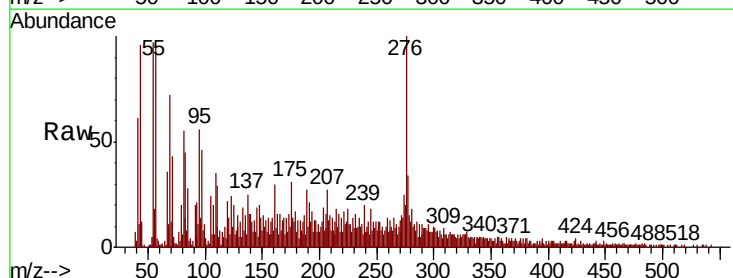

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

