
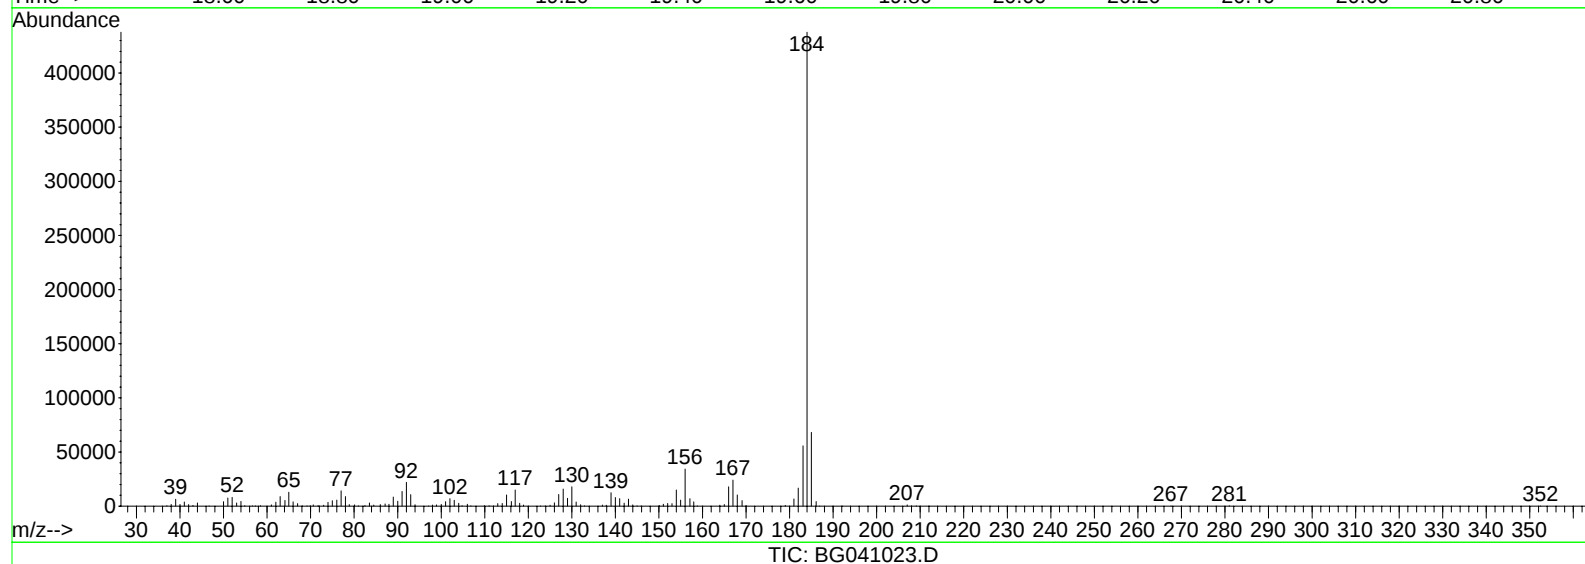


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060319\
Data File : BG041023.D
Acq On : 3 Jun 2019 8:01
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 01:27:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 23:08:34 2019
Response via : Initial Calibration

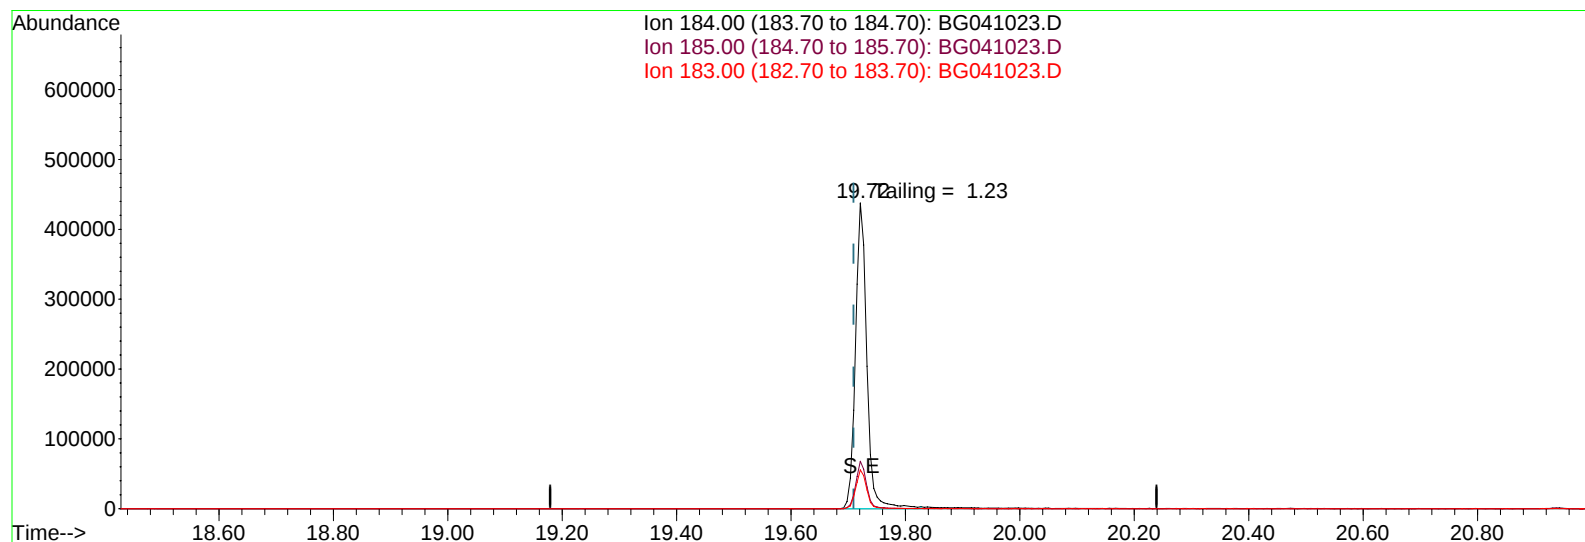

(77) Benzidine



19.721min (+0.012) 415854.40ng

response 615061

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	15.55
183.00	13.40	12.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060319\
Data File : BG041023.D
Acq On : 3 Jun 2019 8:01
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 01:27:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 23:08:34 2019
Response via : Initial Calibration

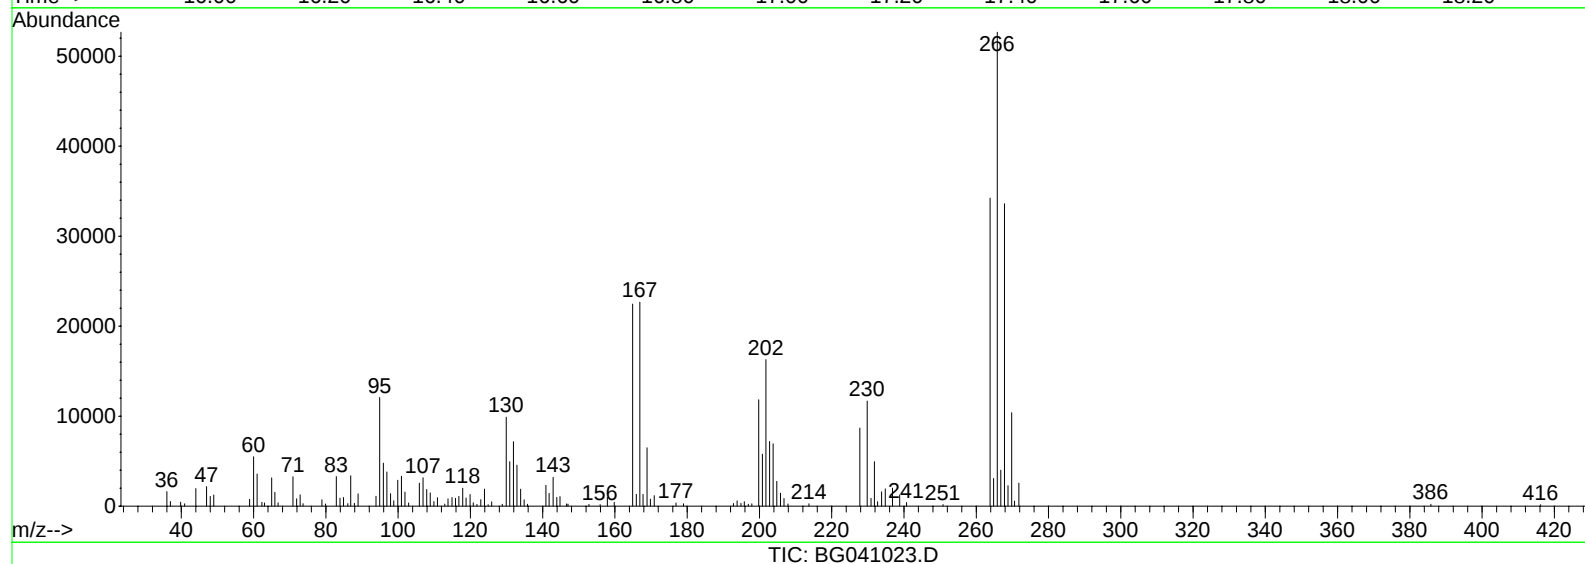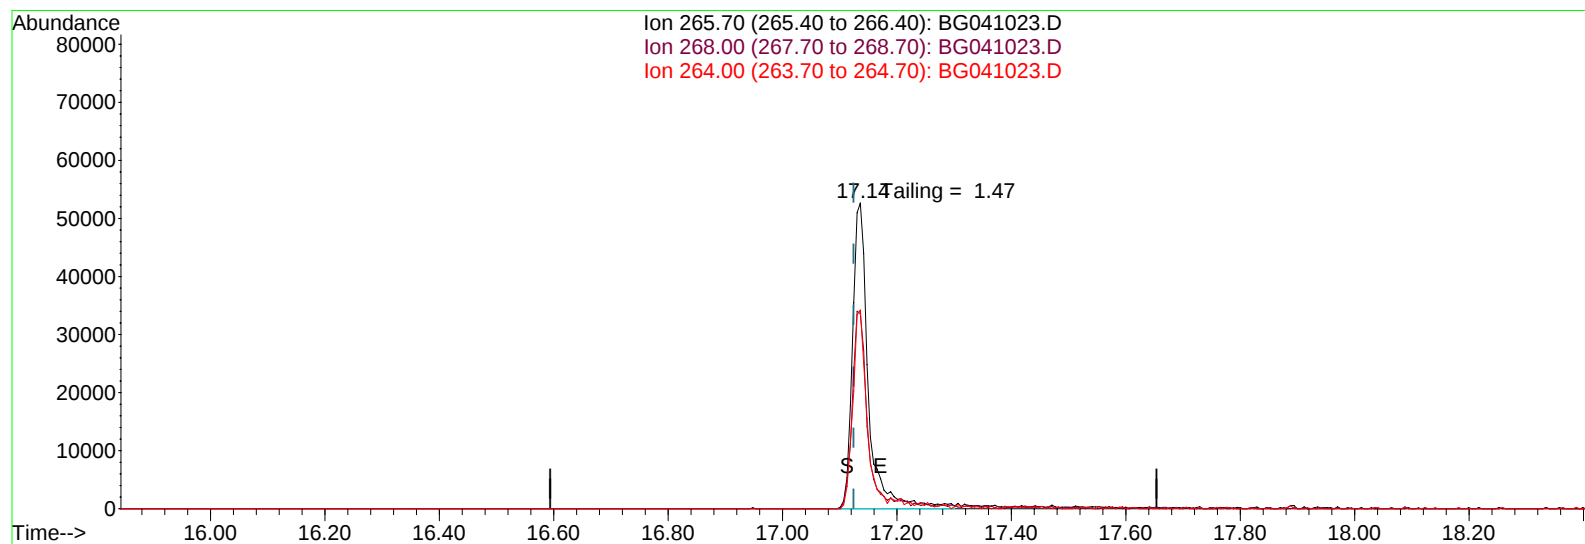

(70) Pentachlorophenol (C)

17.136min (+0.012) 197792.07ng

response 101315

Ion	Exp%	Act%
265.70	100	100
268.00	66.40	63.80
264.00	62.40	65.00
0.00	0.00	0.00