


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060319\
 Data File : BG041023.D
 Acq On : 3 Jun 2019 8:01
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 18:39:57 2019

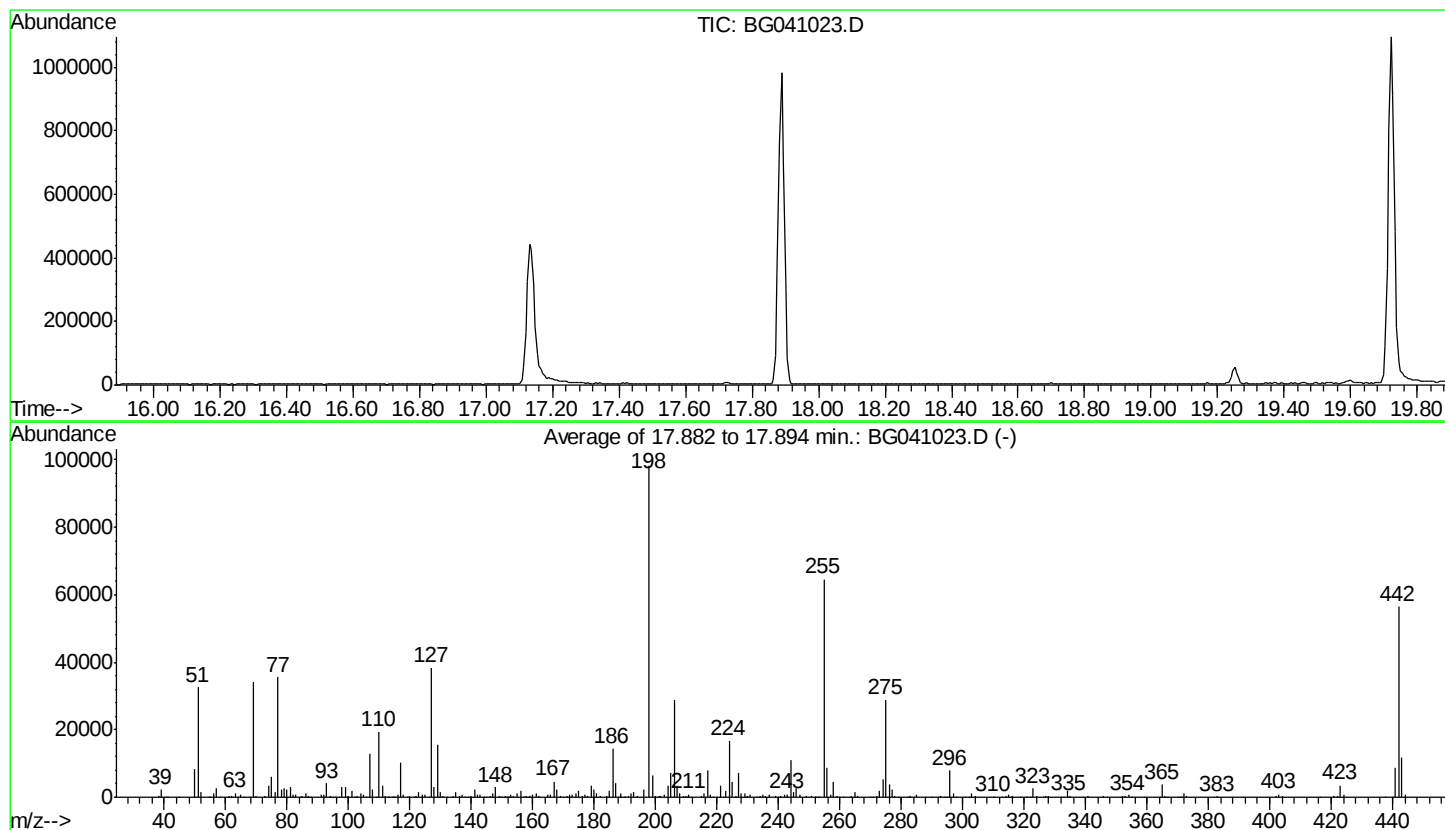

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	32488	PASS
68	69	0.00	2	0.5	171	PASS
69	198	0.00	100	34.7	34053	PASS
70	69	0.00	2	0.6	217	PASS
127	198	10	80	39.2	38488	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98234	PASS
199	198	5	9	6.7	6546	PASS
275	198	10	60	29.4	28842	PASS
365	198	1	100	3.7	3666	PASS
441	198	0.01	100	9.0	8858	PASS
442	198	50	100	57.5	56498	PASS
443	442	15	24	20.9	11791	PASS