


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060319\
 Data File : BG041037.D
 Acq On : 3 Jun 2019 16:53
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 18:39:57 2019

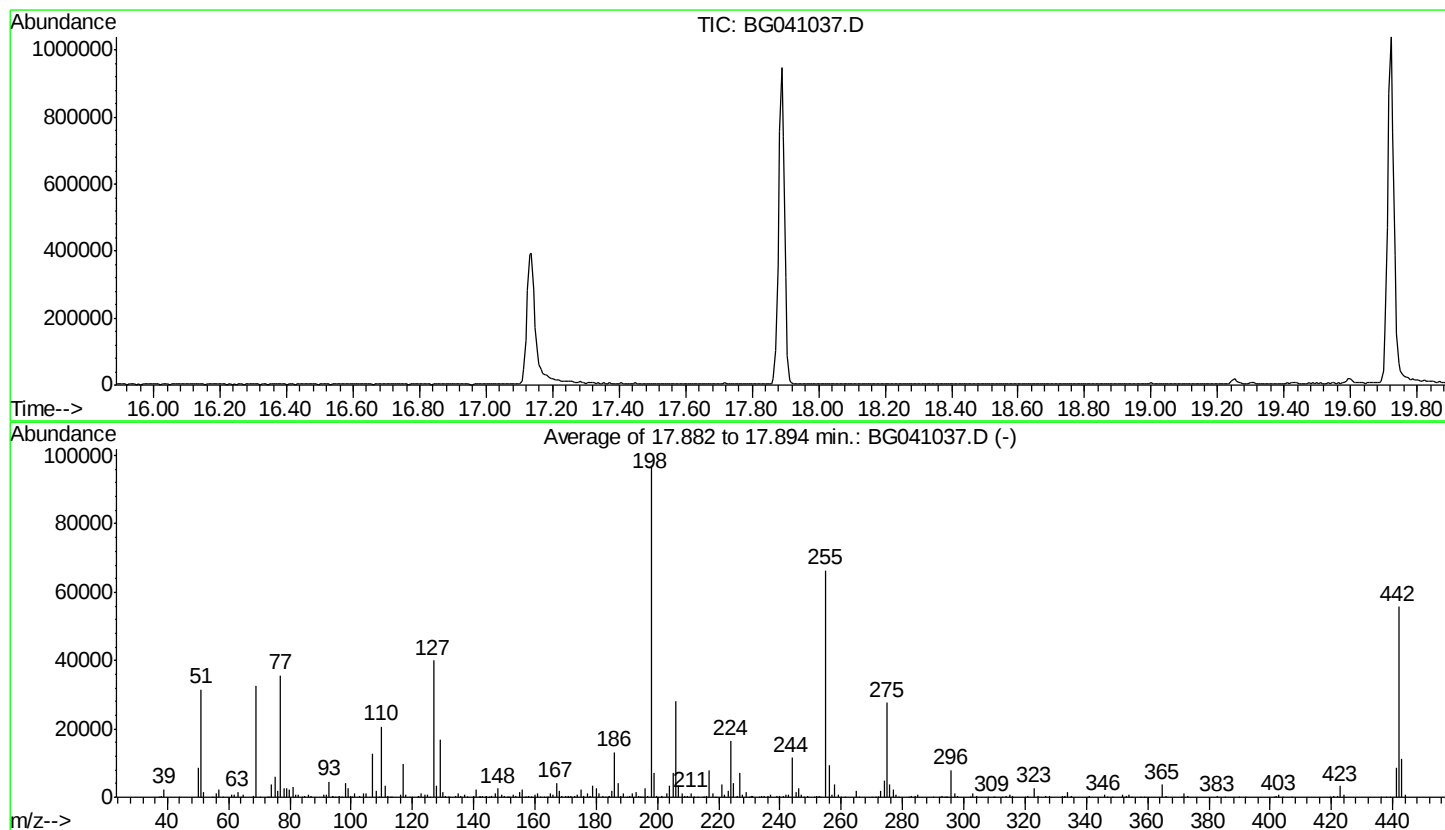

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	31554	PASS
68	69	0.00	2	0.8	273	PASS
69	198	0.00	100	33.7	32672	PASS
70	69	0.00	2	0.5	163	PASS
127	198	10	80	41.2	39960	PASS
197	198	0.00	2	0.4	360	PASS
198	198	100	100	100.0	97042	PASS
199	198	5	9	7.4	7217	PASS
275	198	10	60	28.5	27677	PASS
365	198	1	100	3.7	3574	PASS
441	198	0.01	100	8.7	8454	PASS
442	198	50	100	57.5	55760	PASS
443	442	15	24	19.9	11088	PASS