

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060320\
 Data File : BG045580.D
 Acq On : 3 Jun 2020 14:18
 Operator : CG/JU
 Sample : PB129260BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB129260BL

Quant Time: Jun 03 15:05:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 01 15:07:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.95	152	57204	20.00	ng	0.00
21) Naphthalene-d8	10.76	136	224061	20.00	ng	0.00
39) Acenaphthene-d10	14.60	164	158134	20.00	ng	0.00
64) Phenanthrene-d10	17.34	188	383904	20.00	ng	0.00
76) Chrysene-d12	21.60	240	425074	20.00	ng	0.00
87) Perylene-d12	24.75	264	440281	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	395274	135.04	ng	0.00
7) Phenol-d6	7.15	99	555921	133.44	ng	0.00
23) Nitrobenzene-d5	9.11	82	384829	93.66	ng	0.00
42) 2,4,6-Tribromophenol	16.09	330	280210	138.56	ng	0.00
45) 2-Fluorobiphenyl	13.22	172	892449	95.73	ng	0.00
79) Terphenyl-d14	19.96	244	1695324	93.02	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060320\
Data File : BG045580.D
Acq On : 3 Jun 2020 14:18
Operator : CG/JU
Sample : PB129260BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB129260BL

Quant Time: Jun 03 15:05:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

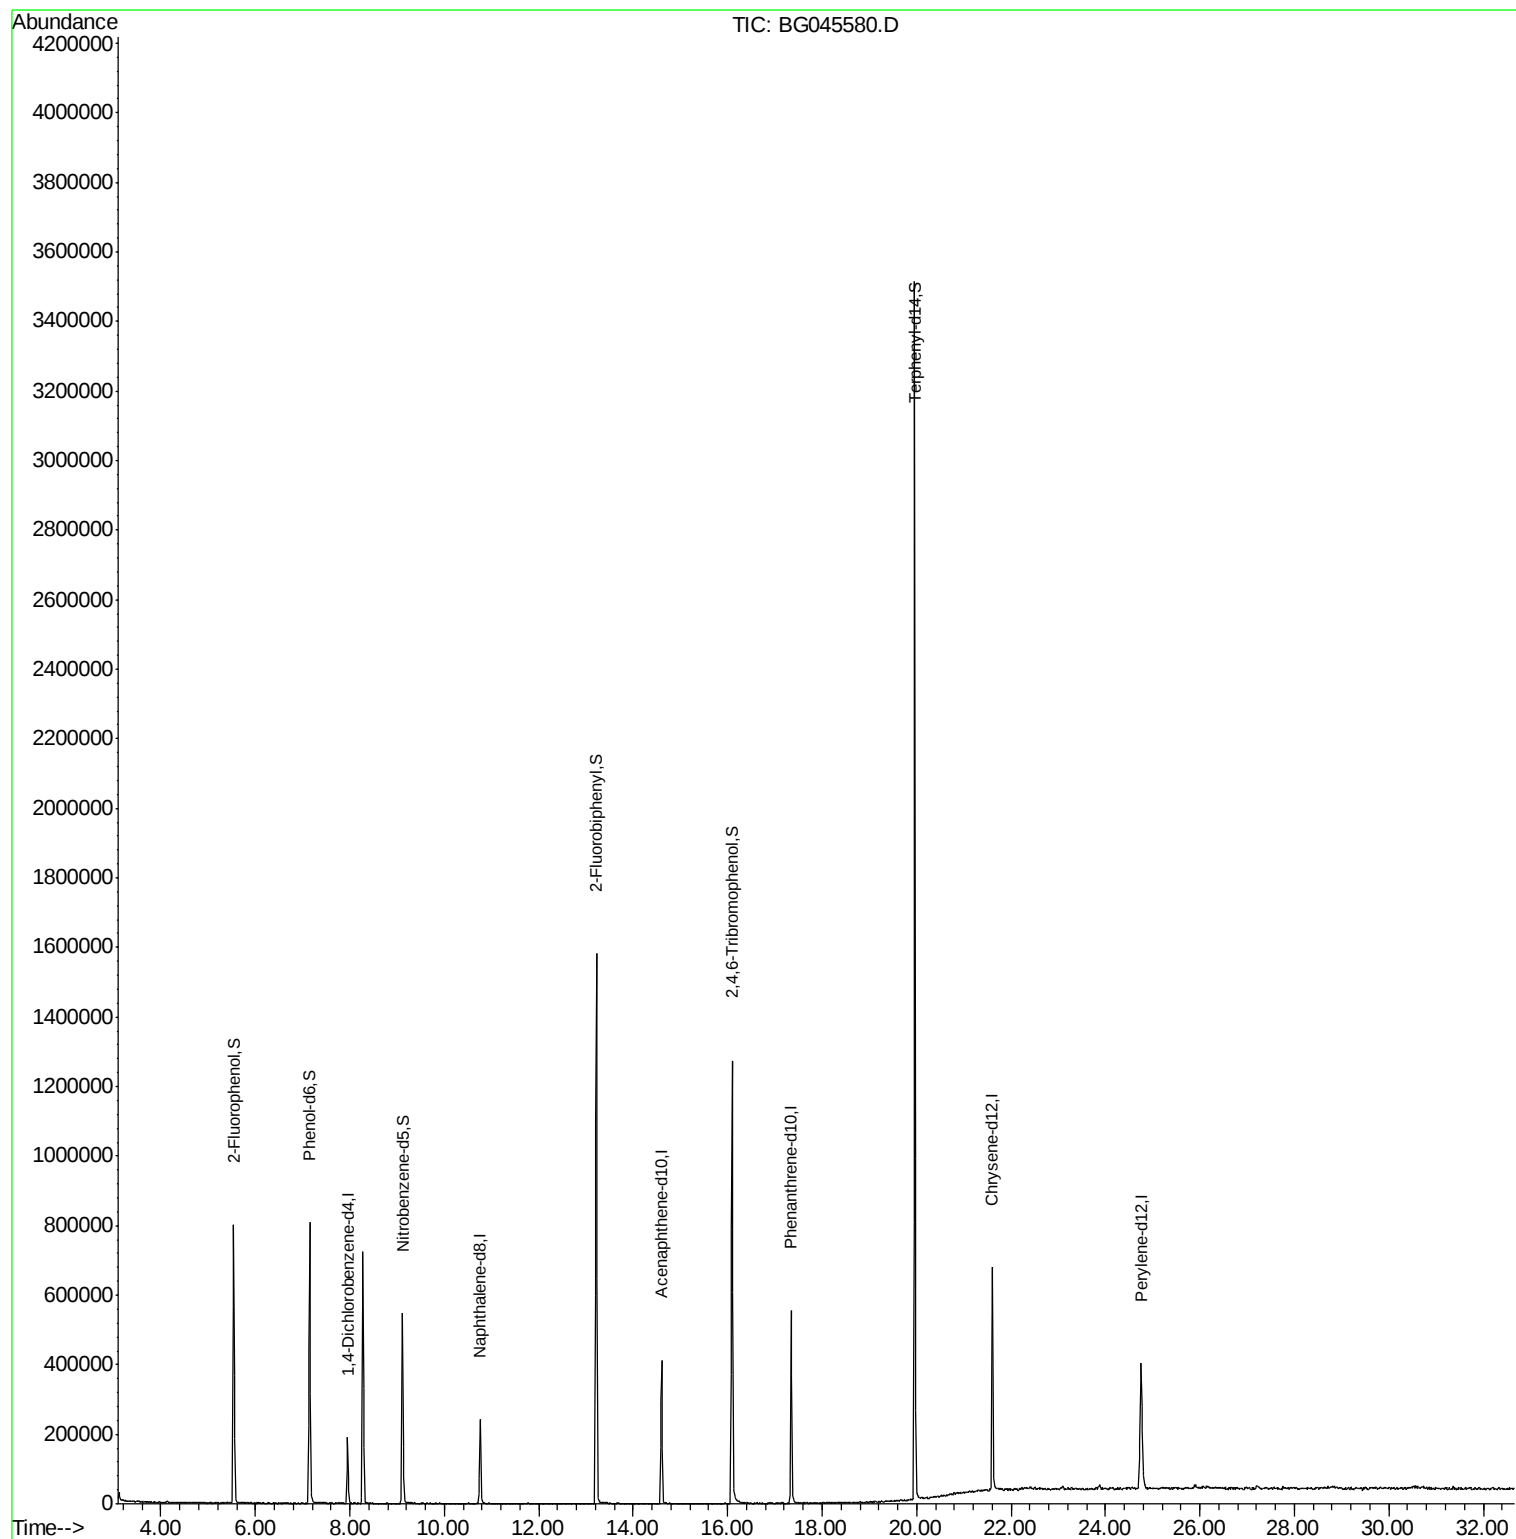

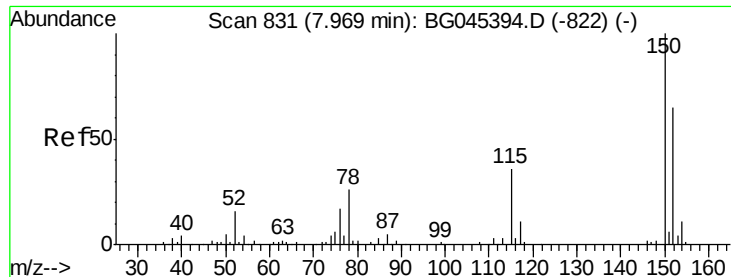


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.95 min Scan# 828
Delta R.T. -0.00 min
Lab File: BG045580.D
Acq: 3 Jun 2020 14:18

Instrument :
BNA_G
ClientSampleId :
PB129260BL

Tot Ion:152 Resp: 57204
Ion Ratio Lower Upper
152 100
150 156.4 122.4 183.6
115 57.1 44.2 66.4

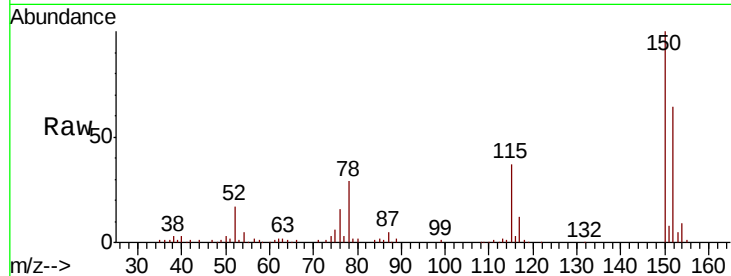


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

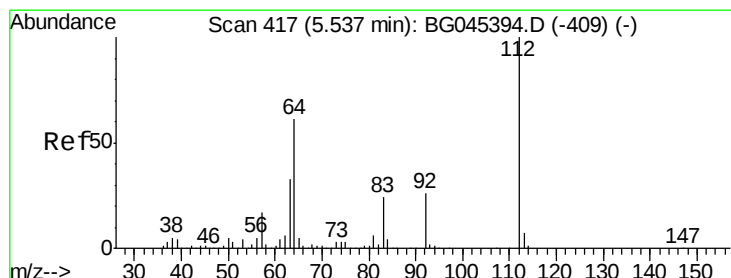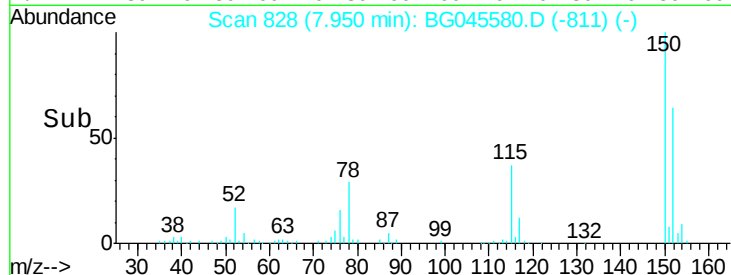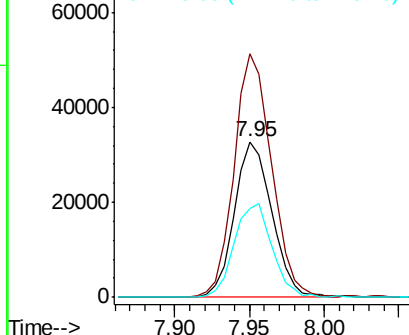



#5


2-Fluorophenol
Concen: 135.040 ng
RT: 5.54 min Scan# 418
Delta R.T. 0.00 min
Lab File: BG045580.D
Acq: 3 Jun 2020 14:18

Tgt Ion:112 Resp: 395274
Ion Ratio Lower Upper
112 100
64 56.4 48.6 72.8
63 32.5 26.5 39.7

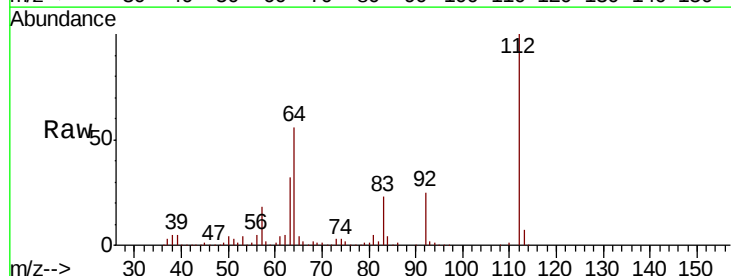

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

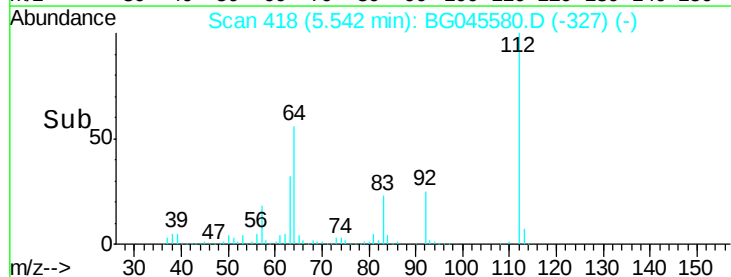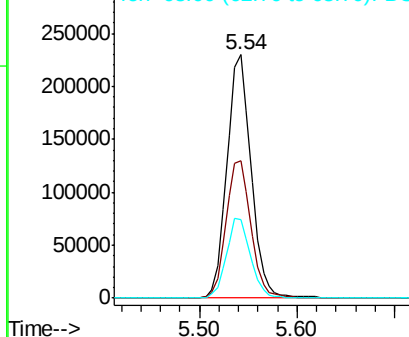

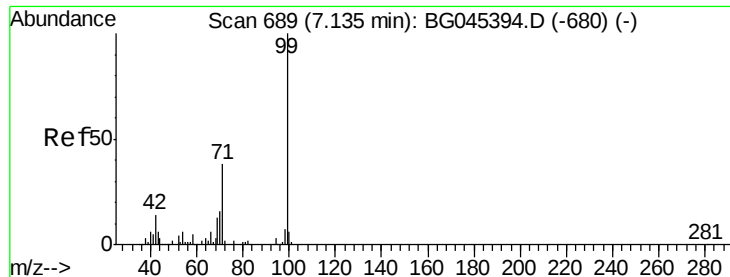

#7

Phenol-d6

Concen: 133.438 ng

RT: 7.15 min Scan# 691

Delta R.T. -0.00 min

Lab File: BG045580.D

Acq: 3 Jun 2020 14:18

Instrument :

BNA_G

ClientSampleId :

PB129260BL


Tot Ion: 99 Resp: 555921

Ion Ratio Lower Upper




99 100

42 13.8 11.3 16.9

71 39.6 30.8 46.2

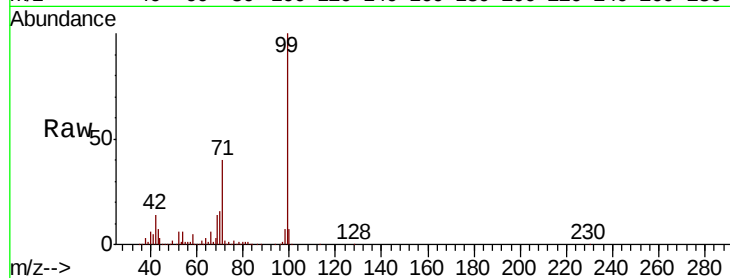

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

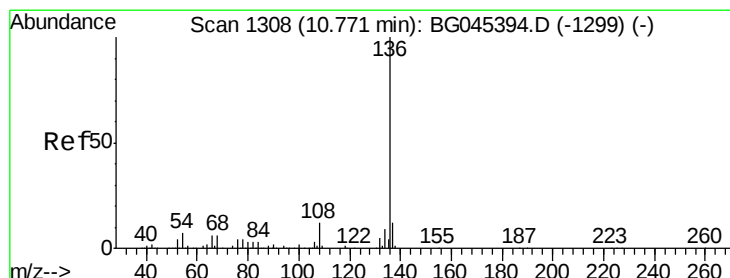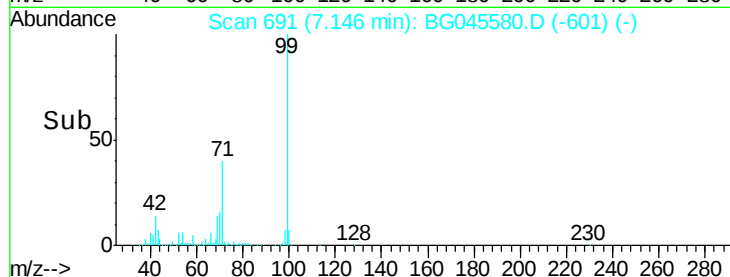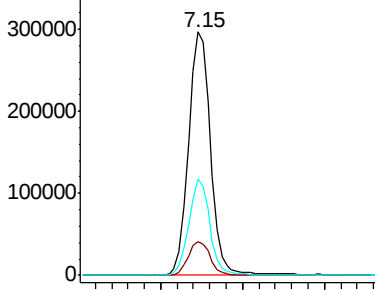

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.76 min Scan# 1306

Delta R.T. -0.00 min

Lab File: BG045580.D

Acq: 3 Jun 2020 14:18

Tgt Ion: 136 Resp: 224061


Ion Ratio Lower Upper

136 100



137 11.5 9.4 14.2


54 6.8 5.8 8.6

68 5.7 4.5 6.7

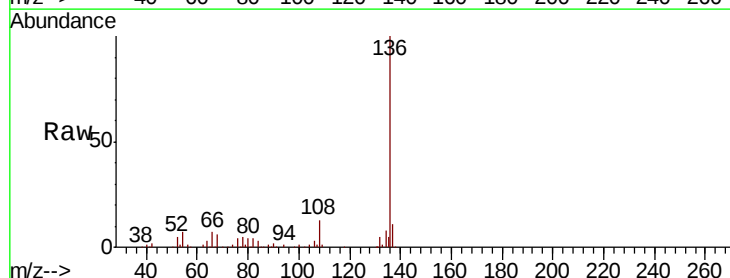

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



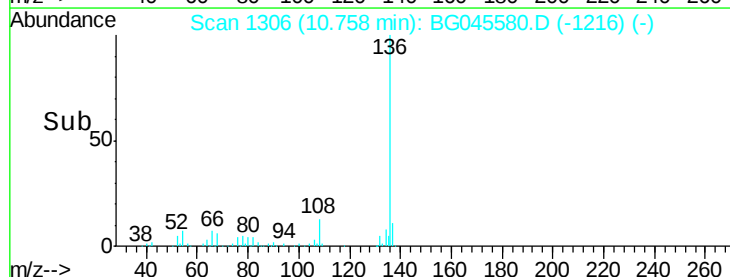
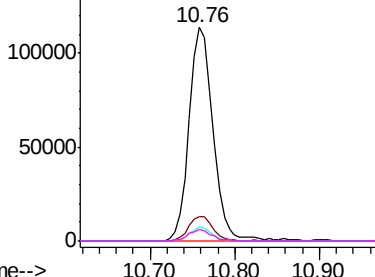


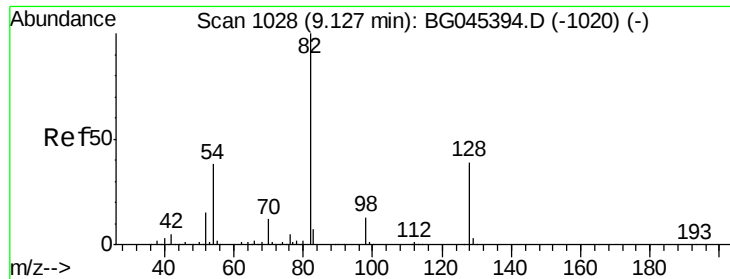

#23
Nitrobenzene-d5
Concen: 93.659 ng
RT: 9.11 min Scan# 1026
Delta R.T. -0.00 min
Lab File: BG045580.D
Acq: 3 Jun 2020 14:18




Instrument :
BNA_G
ClientSampleId :
PB129260BL


Tot Ion	82	Resp	384829
Ion Ratio	Lower	Upper	
82	100		
128	41.1	30.9	46.3
54	39.9	30.3	45.5

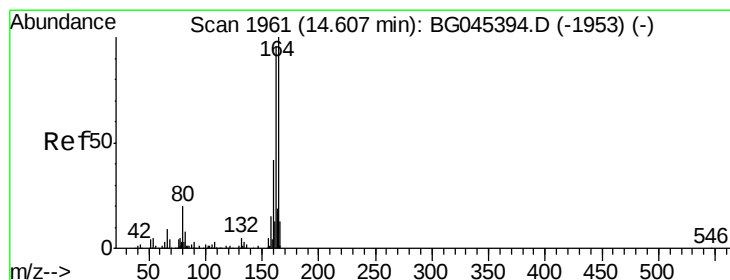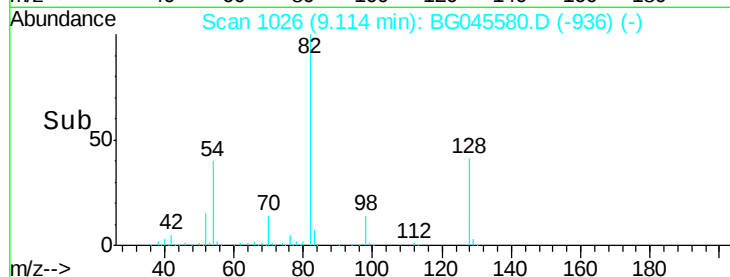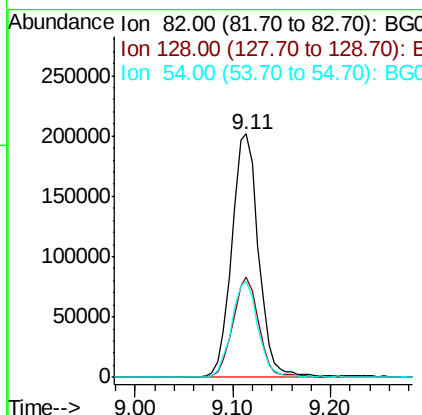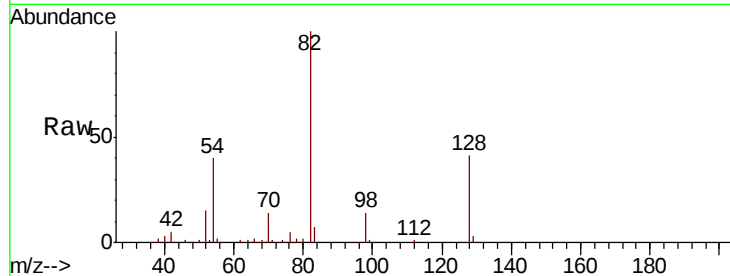

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.60 min Scan# 1960
Delta R.T. 0.00 min
Lab File: BG045580.D
Acq: 3 Jun 2020 14:18

Tgt Ion	164	Resp	158134
Ion Ratio	Lower	Upper	
164	100		
162	100.1	76.9	115.3
160	42.1	33.8	50.8


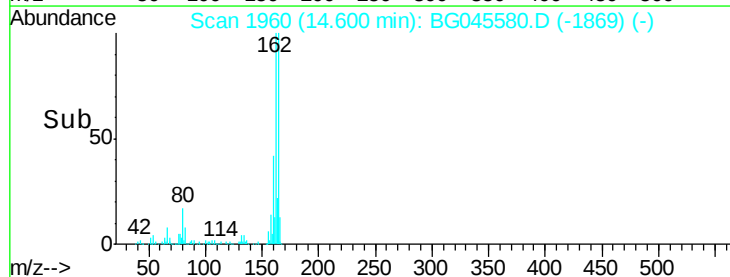
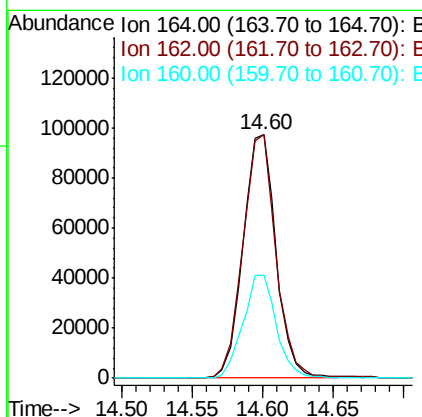
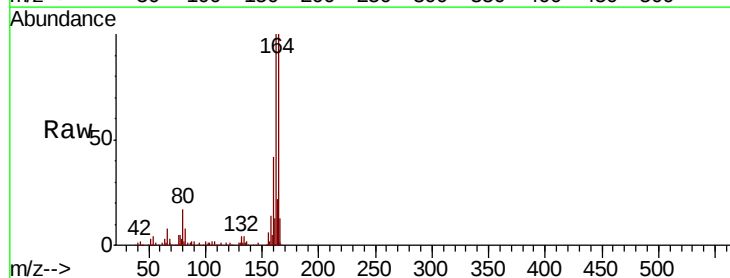


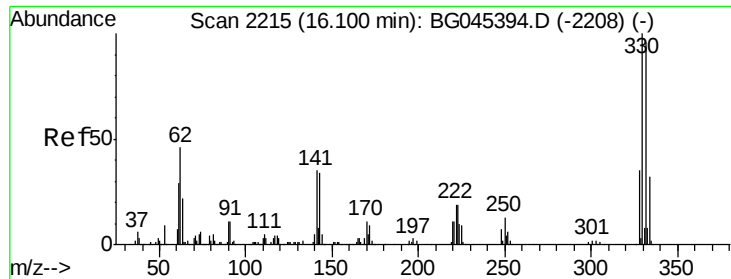

#42
 2,4,6-Tribromophenol
 Concen: 138.556 ng
 RT: 16.09 min Scan# 2214
 Delta R.T. -0.00 min
 Lab File: BG045580.D
 Acq: 3 Jun 2020 14:18




Instrument :
 BNA_G
 ClientSampleId :
 PB129260BL


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	78.2	117.4
141	34.8	28.2	42.4

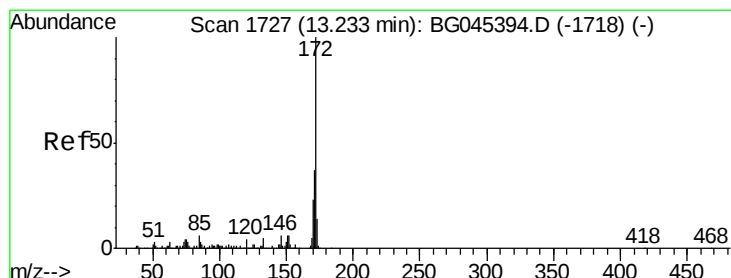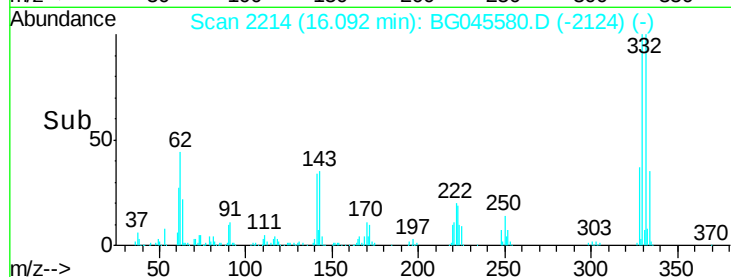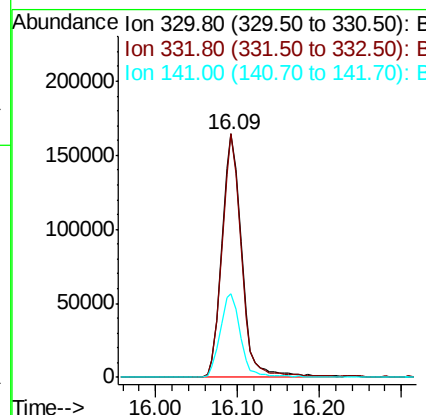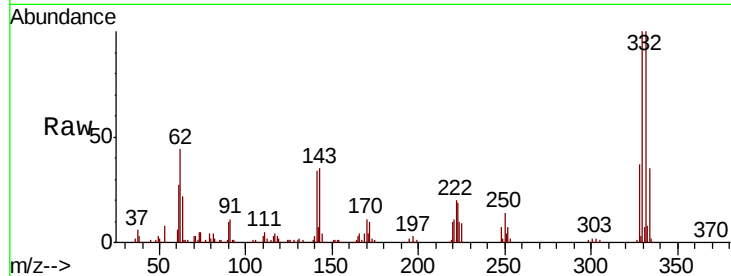

#45
 2-Fluorobiphenyl
 Concen: 95.728 ng
 RT: 13.22 min Scan# 1725
 Delta R.T. 0.00 min
 Lab File: BG045580.D
 Acq: 3 Jun 2020 14:18

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.5	44.3
170	24.2	18.5	27.7

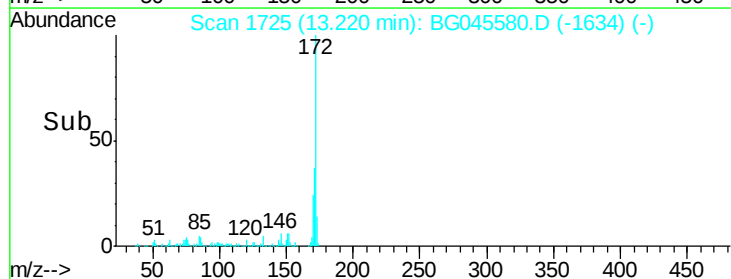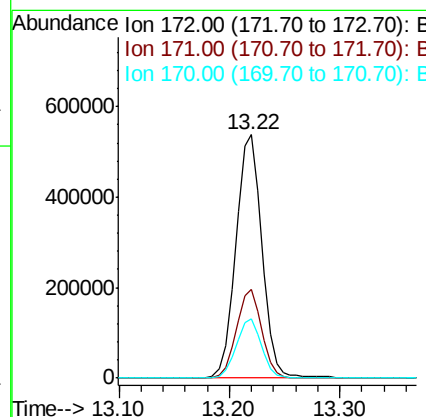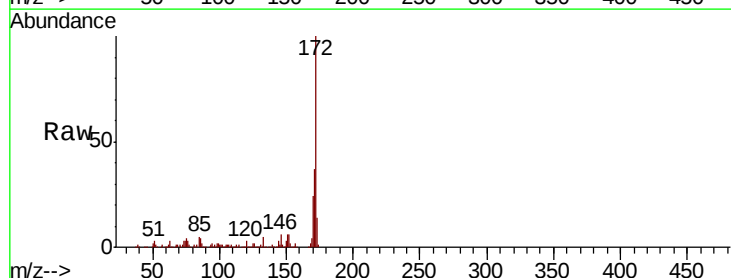

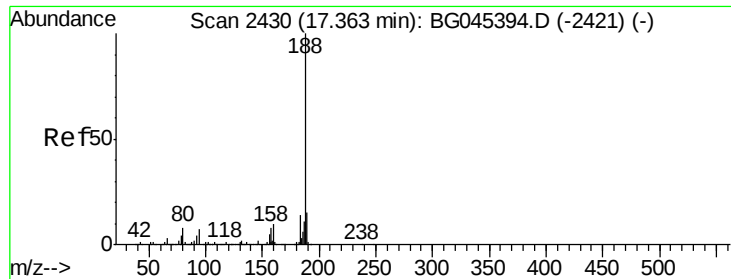

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.34 min Scan# 2427

Delta R.T. -0.00 min

Lab File: BG045580.D

Acq: 3 Jun 2020 14:18

Instrument :

BNA_G

ClientSampleId :

PB129260BL


Tot Ion:188 Resp: 383904

Ion Ratio Lower Upper

188 100

94 7.4 5.5 8.3




80 7.9 6.6 10.0

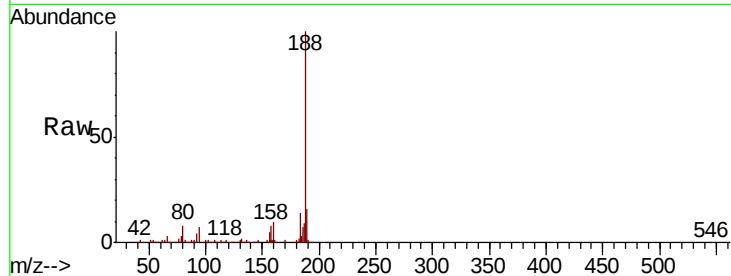

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

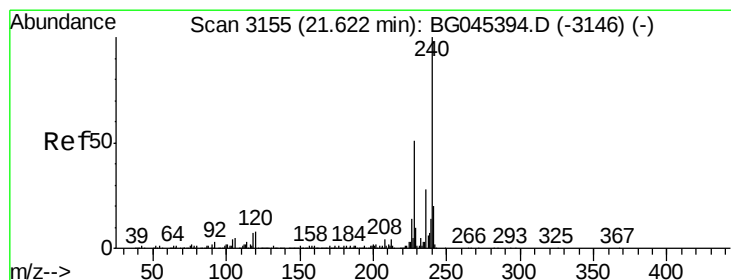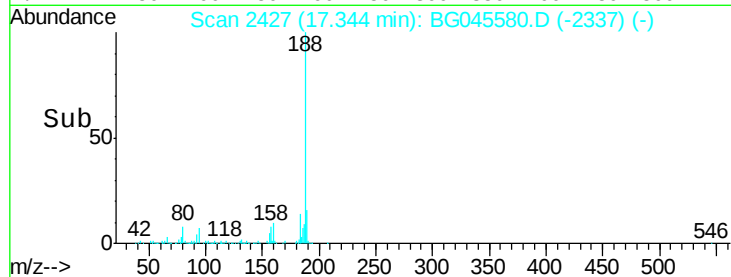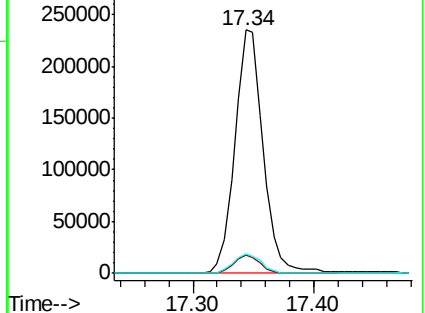

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.60 min Scan# 3152

Delta R.T. -0.00 min

Lab File: BG045580.D

Acq: 3 Jun 2020 14:18


Tgt Ion:240 Resp: 425074

Ion Ratio Lower Upper

240 100

120 7.6 6.1 9.1



236 26.5 22.3 33.5

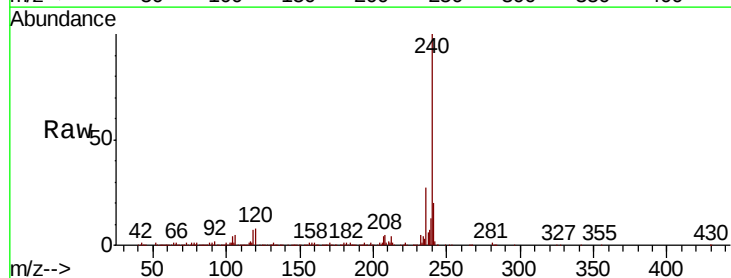


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

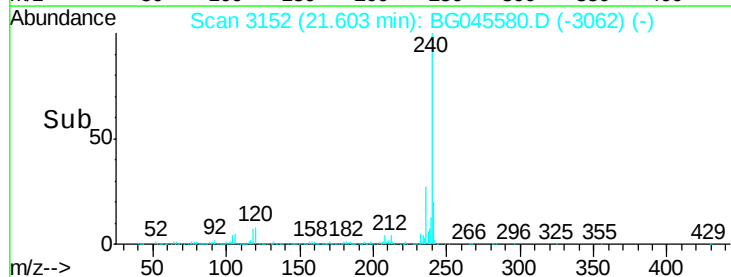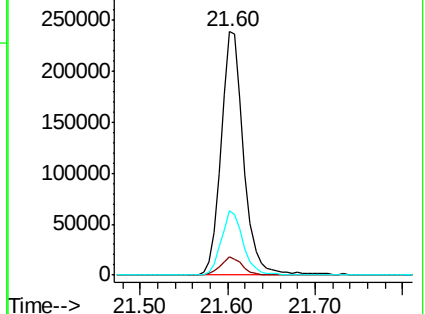

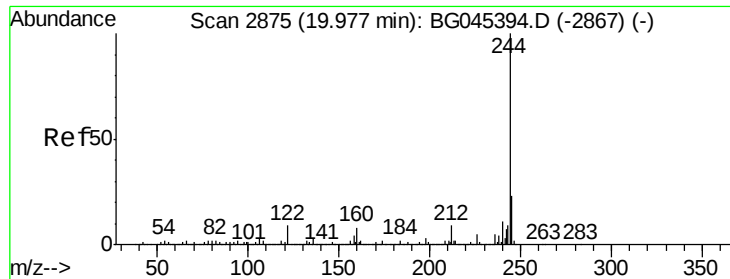

#79

Terphenyl-d14

Concen: 93.019 ng

RT: 19.96 min Scan# 2873

Delta R.T. 0.00 min

Lab File: BG045580.D

Acq: 3 Jun 2020 14:18

Instrument :

BNA_G

ClientSampleId :

PB129260BL


Tot Ion:244 Resp: 1695324

Ion Ratio Lower Upper

244 100

212 9.4 7.4 11.0




122 8.6 6.8 10.2

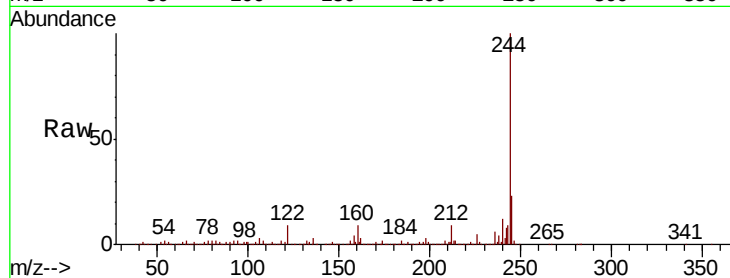

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

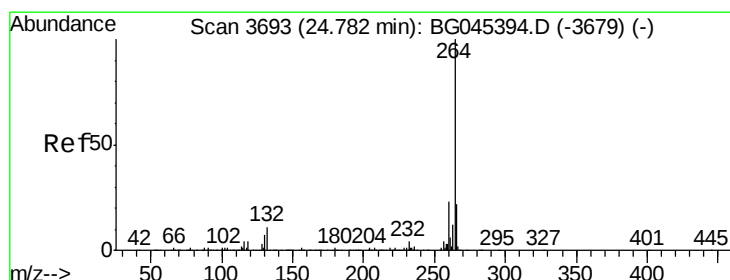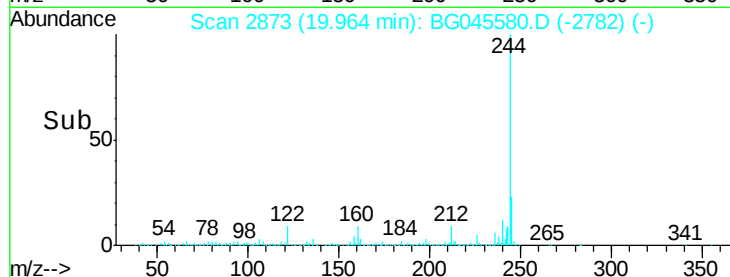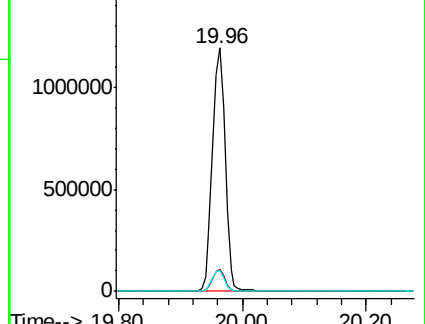

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.75 min Scan# 3688

Delta R.T. -0.00 min

Lab File: BG045580.D

Acq: 3 Jun 2020 14:18


Tgt Ion:264 Resp: 440281

Ion Ratio Lower Upper

264 100

260 21.3 18.2 27.4

265 20.9 17.6 26.4

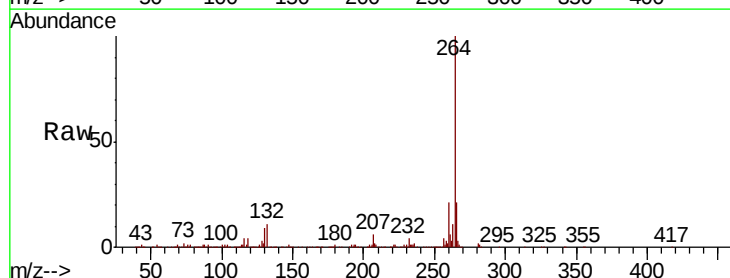

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

